

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121019\
 Data File : FB023180.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2019 12:22
 Operator : DD/AJ
 Sample : K6204-13MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 11 00:19:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	469072	19.096 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	796095	24.362 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	913150	26.187 ng/ml
3) t n-Heptane	7.758	297077	8.640 ng/ml
4) t Benzene	7.893	387023	9.289 ng/ml
6) t Toluene	10.632	1111719	27.597 ng/ml
7) t Ethylbenzene	13.072	350761	9.090 ng/ml
8) t m-Xylene	13.205	659474	18.122 ng/ml
9) t O-Xylene	13.933	639645	18.423 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	531793	18.963 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121019\
Data File : FB023180.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2019 12:22
Operator : DD/AJ
Sample : K6204-13MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 11 00:19:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

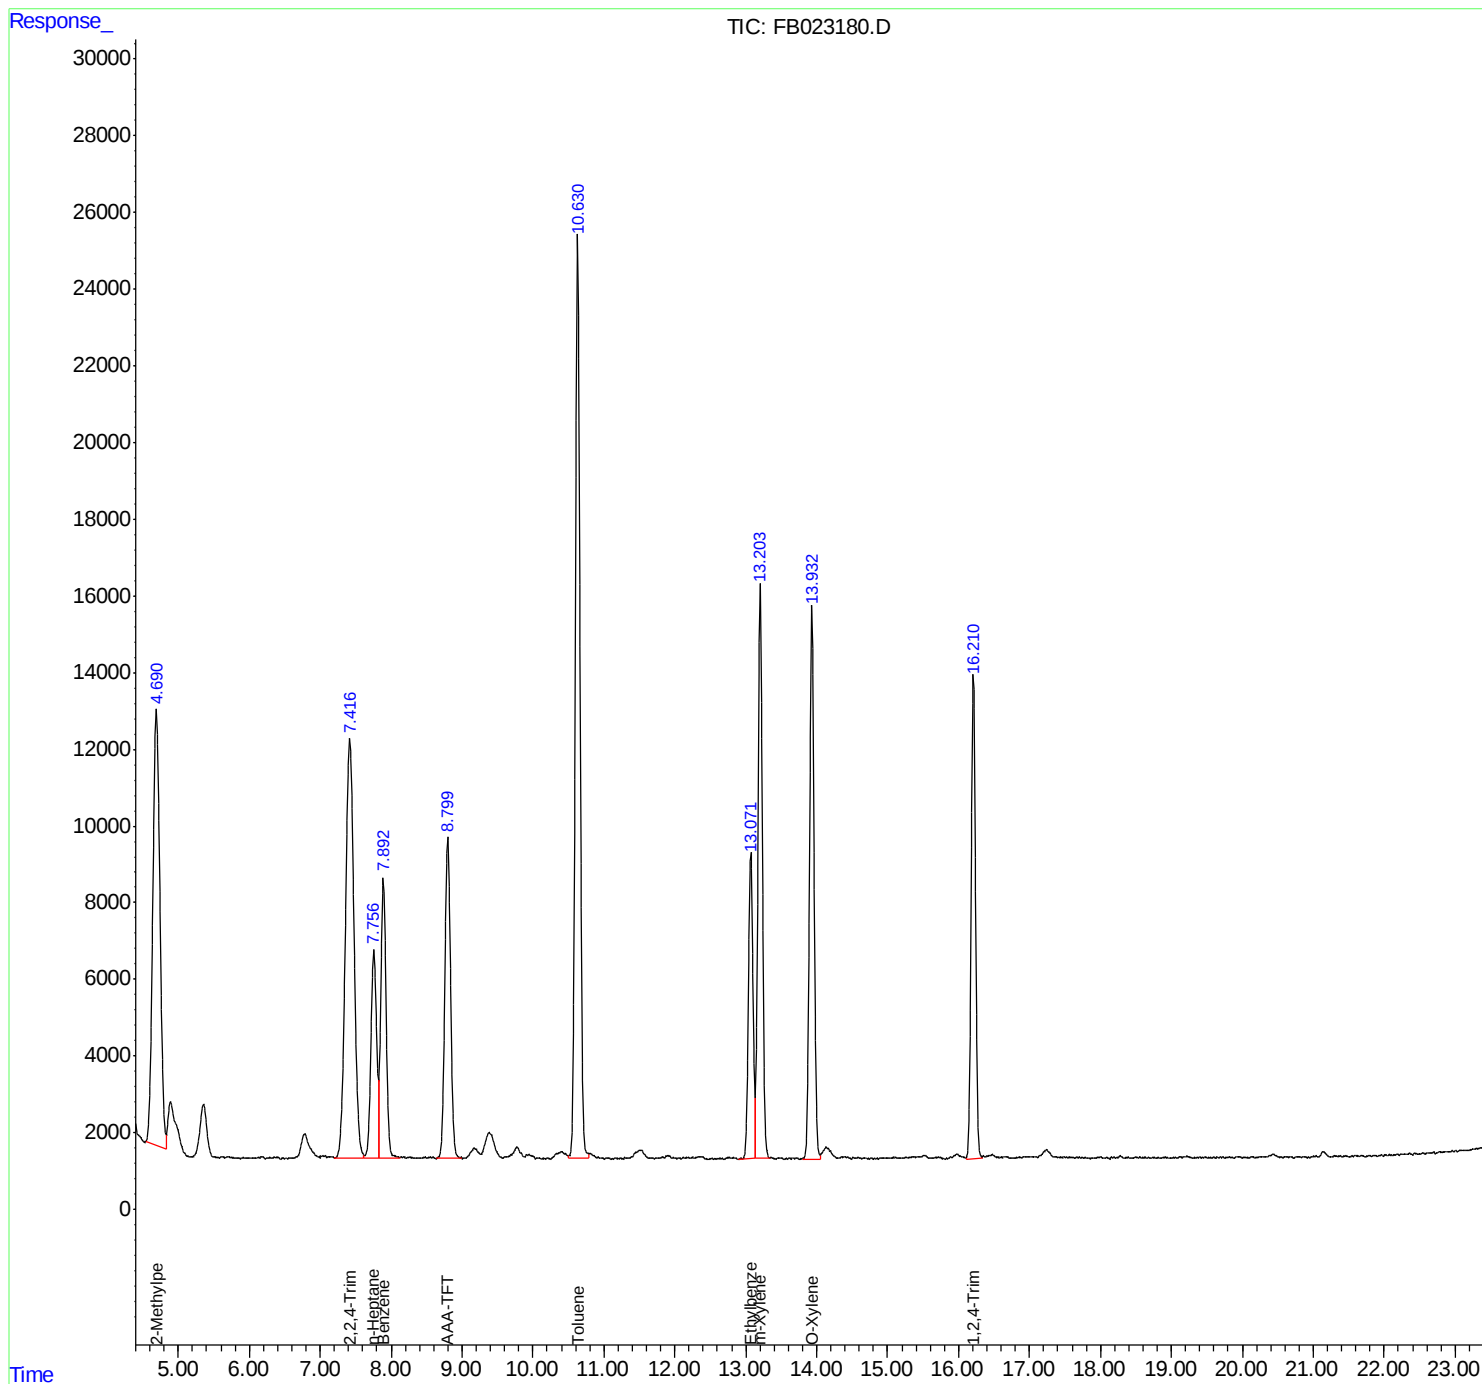

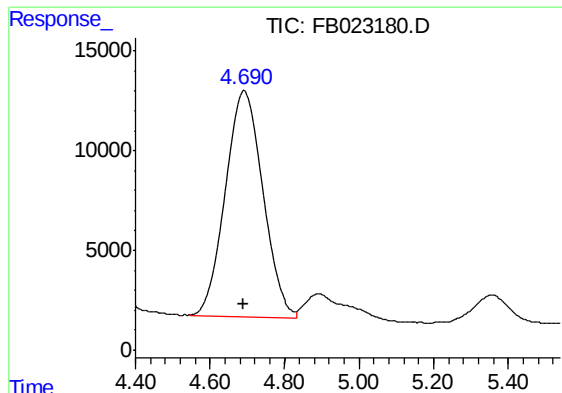


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 796095
Conc: 24.36 ng/ml

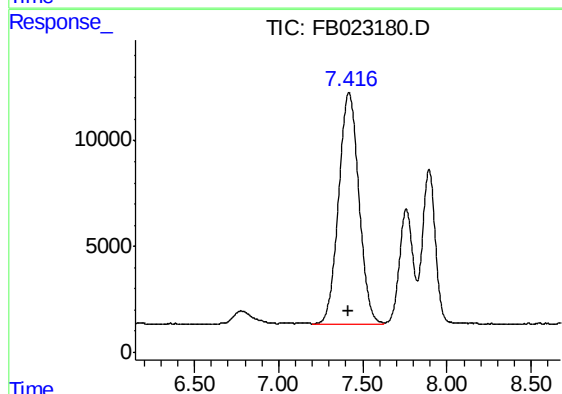


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 913150
Conc: 26.19 ng/ml

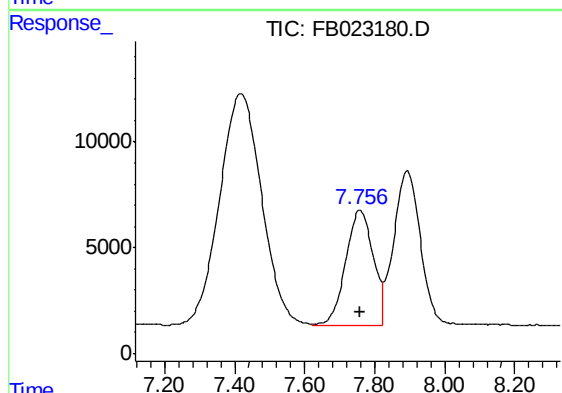


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 297077
Conc: 8.64 ng/ml

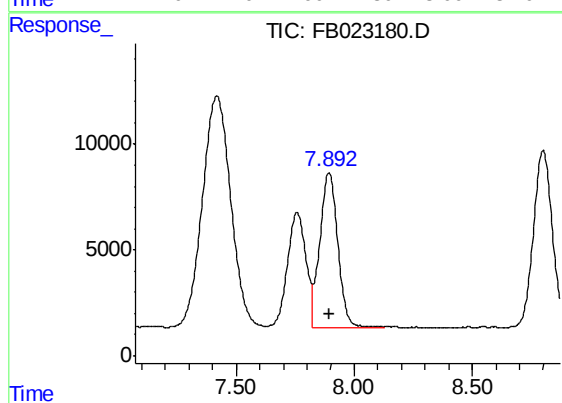


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 387023
Conc: 9.29 ng/ml

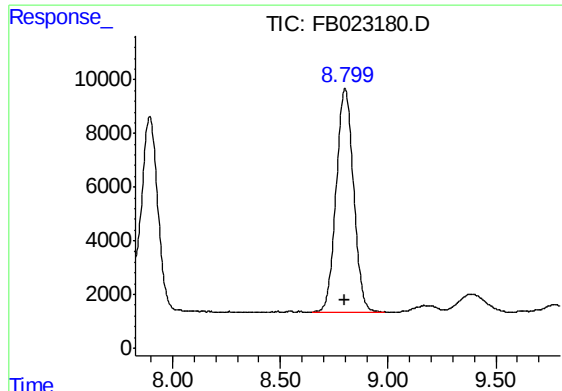


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 469072
Conc: 19.10 ng/ml

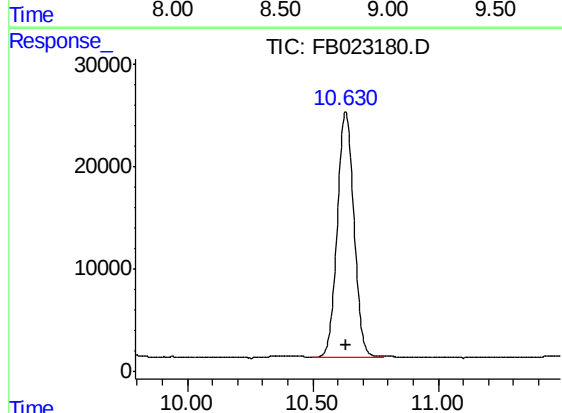


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 1111719
Conc: 27.60 ng/ml

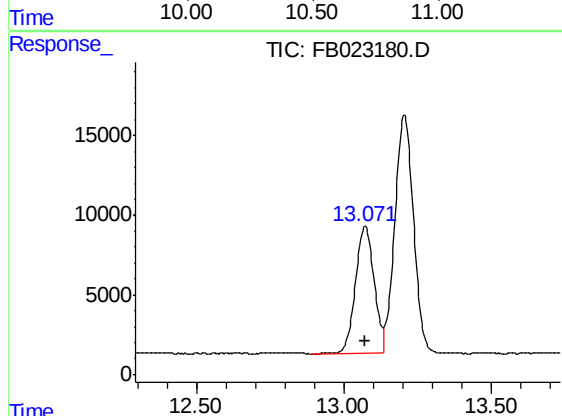


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.001 min
Response: 350761
Conc: 9.09 ng/ml

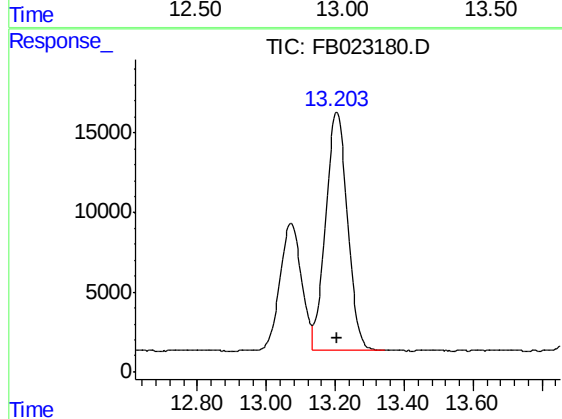


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.001 min
Response: 659474
Conc: 18.12 ng/ml

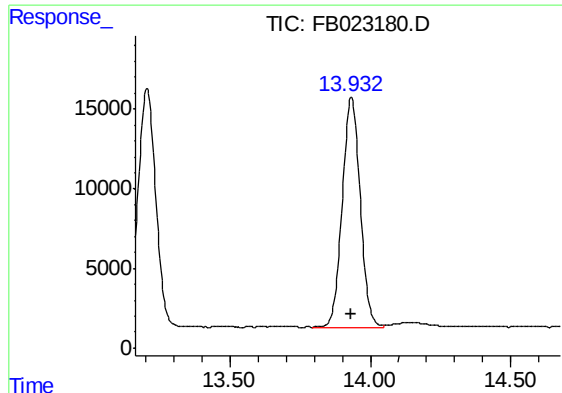

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 639645
Conc: 18.42 ng/ml

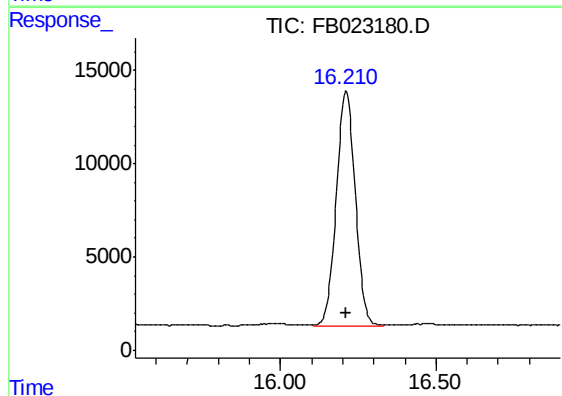

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 531793
Conc: 18.96 ng/ml