

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC010323AL\
 Data File : FC062551.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jan 2023 19:39
 Operator : YP/AJ
 Sample : N6248-12D
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 04 02:45:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 08 01:05:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.560	4528095	32.100 ug/ml
Spiked Amount 50.000		Recovery =	64.20%
12) S 1-chlorooctadecane (S...	12.998	3429277	32.174 ug/ml
Spiked Amount 50.000		Recovery =	64.35%
Target Compounds			
10) T n-Eicosane (C20)	12.607	196429	1.579 ug/ml
14) T n-Tetracosane (C24)	14.823	132128	1.102 ug/ml
16) T n-Octacosane (C28)	16.817	54059	0.476 ug/ml
17) T n-Tricontane (C30)	17.703	80758	0.722 ug/ml
18) T n-Dotriacontane (C32)	18.534	78192	0.704 ug/ml
19) T n-Tetratriacontane (C34)	19.315	55981	0.517 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC010323AL\
Data File : FC062551.D
Signal(s) : FID1A.ch
Acq On : 03 Jan 2023 19:39
Operator : YP/AJ
Sample : N6248-12D
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 04 02:45:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
Quant Title : GC Extractables
QLast Update : Thu Dec 08 01:05:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

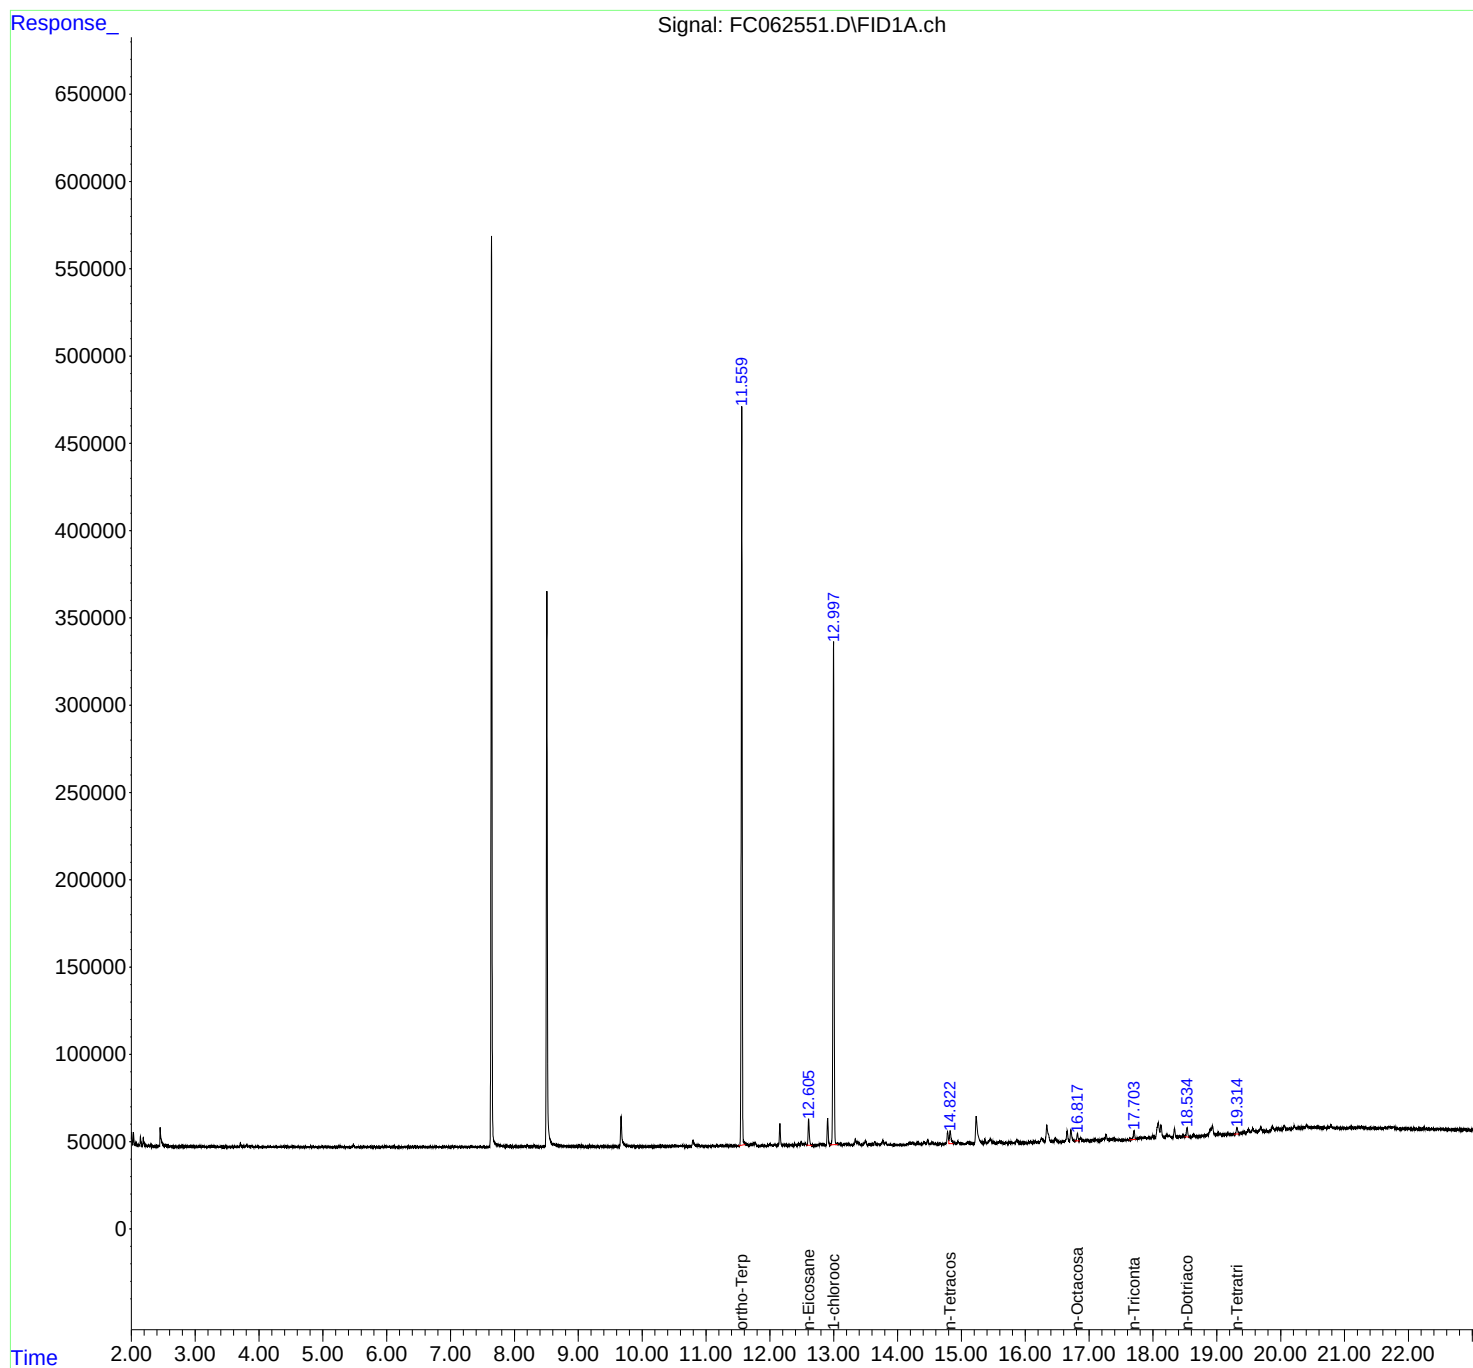


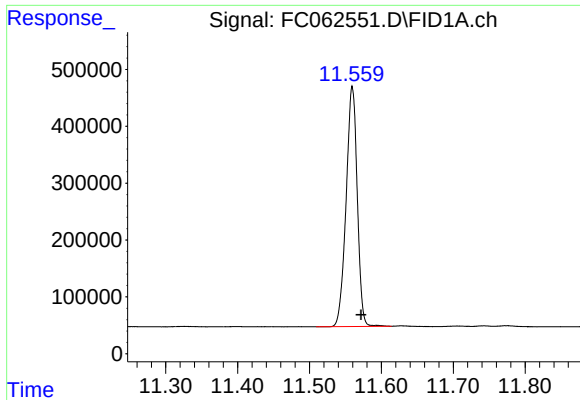

#9 ortho-Terphenyl (SURR)


R.T.: 11.560 min
Delta R.T.: -0.012 min
Response: 4528095
Conc: 32.10 ug/ml

Instrument :
FID_C
ClientSampleId :

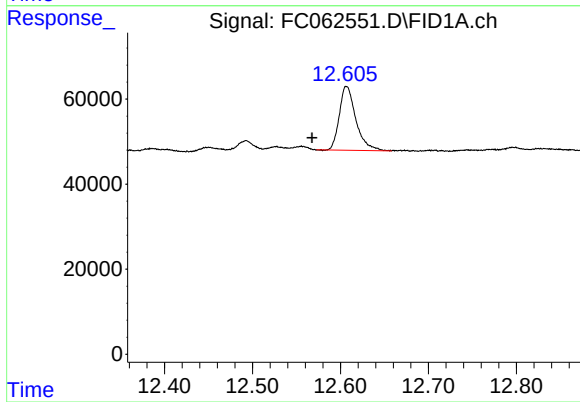


#10 n-Eicosane (C20)

R.T.: 12.607 min
Delta R.T.: 0.039 min
Response: 196429
Conc: 1.58 ug/ml

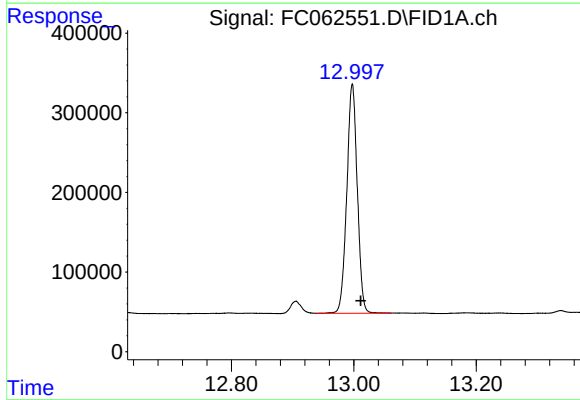


#12 1-chlorooctadecane (SURR)

R.T.: 12.998 min
Delta R.T.: -0.014 min
Response: 3429277
Conc: 32.17 ug/ml

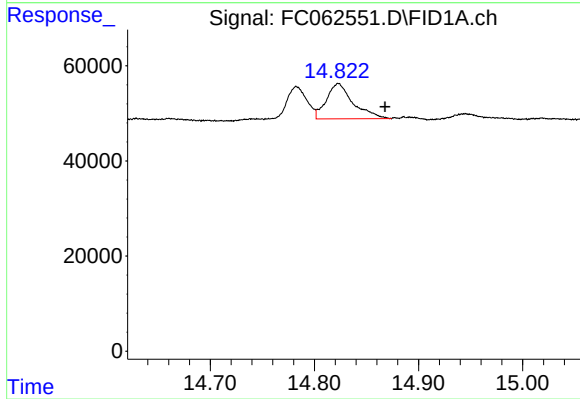

#14 n-Tetracosane (C24)


R.T.: 14.823 min
Delta R.T.: -0.045 min
Response: 132128
Conc: 1.10 ug/ml

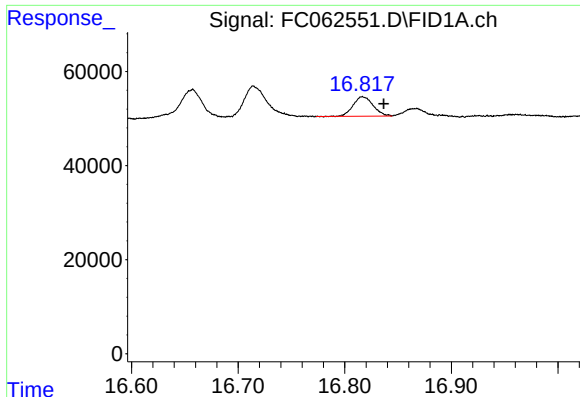

#16 n-Octacosane (C28)


R.T.: 16.817 min
Delta R.T.: -0.020 min
Response: 54059
Conc: 0.48 ug/ml

Instrument :
FID_C
ClientSampleId :

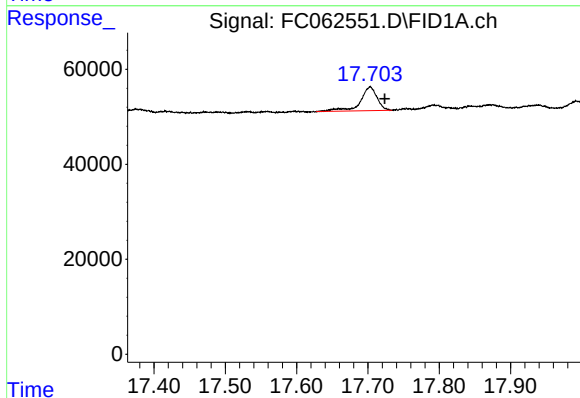


#17 n-Tricontane (C30)

R.T.: 17.703 min
Delta R.T.: -0.020 min
Response: 80758
Conc: 0.72 ug/ml

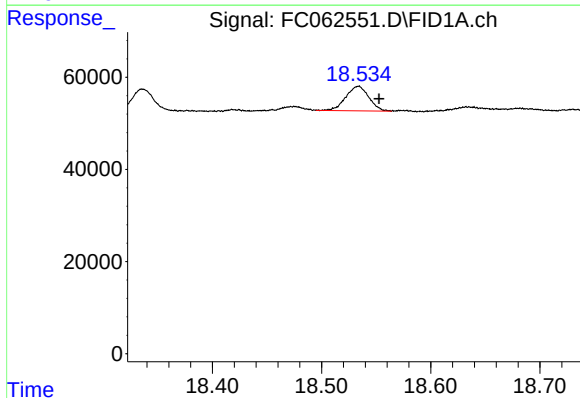

#18 n-Dotriacontane (C32)

R.T.: 18.534 min
Delta R.T.: -0.019 min
Response: 78192
Conc: 0.70 ug/ml

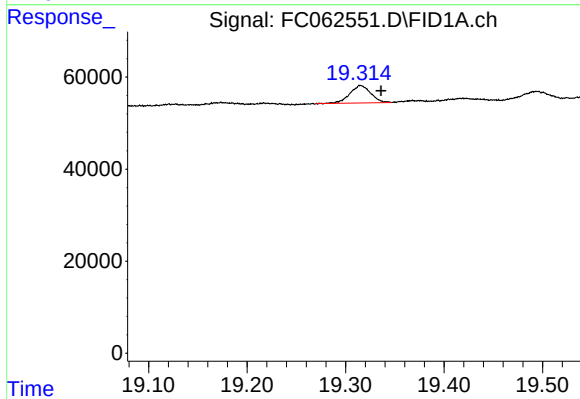

#19 n-Tetratriacontane (C34)

R.T.: 19.315 min
Delta R.T.: -0.021 min
Response: 55981
Conc: 0.52 ug/ml