

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC010522AL\
 Data File : FC057738.D
 Signal(s) : FID1A.CH
 Acq On : 06 Jan 2022 6:19
 Operator : AJ\MA
 Sample : N1016-01DL 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 06 07:47:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 12:13:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.150	948934	6.438 ug/ml
Spiked Amount 50.000		Recovery =	12.88%
Target Compounds			
16) T n-Octacosane (C28)	15.966	120816	0.738 ug/ml
17) T n-Tricontane (C30)	16.851	572864	3.669 ug/ml
18) T n-Dotriacontane (C32)	17.682	888225	6.371 ug/ml
19) T n-Tetratriacontane (C34)	18.465	863059	6.944 ug/ml
20) T n-Hexatriacontane (C36)	19.202	568225	5.111 ug/ml
21) T n-Octatriacontane (C38)	19.907	168429	1.615 ug/ml
22) T n-Tetracontane (C40)	20.728	3602992	37.628 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC010522AL\
Data File : FC057738.D
Signal(s) : FID1A.CH
Acq On : 06 Jan 2022 6:19
Operator : AJ\MA
Sample : N1016-01DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 06 07:47:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 12:13:43 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

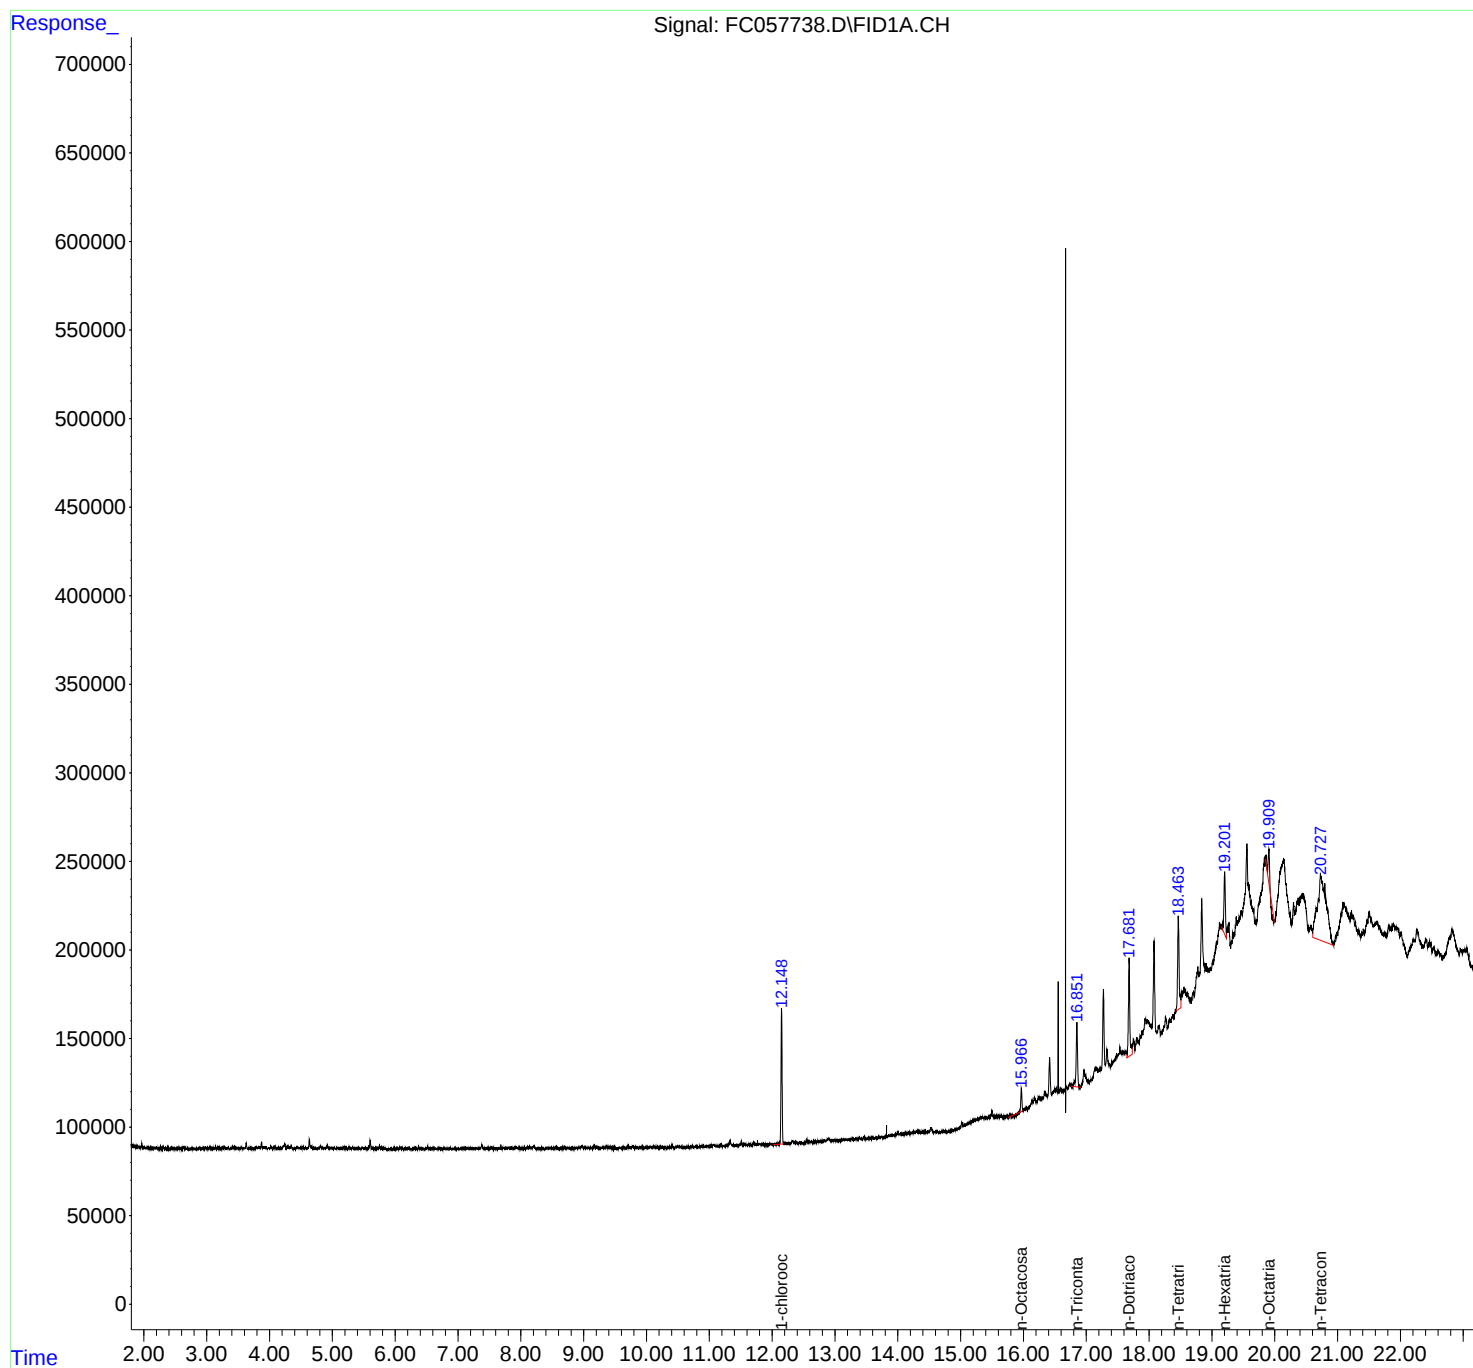


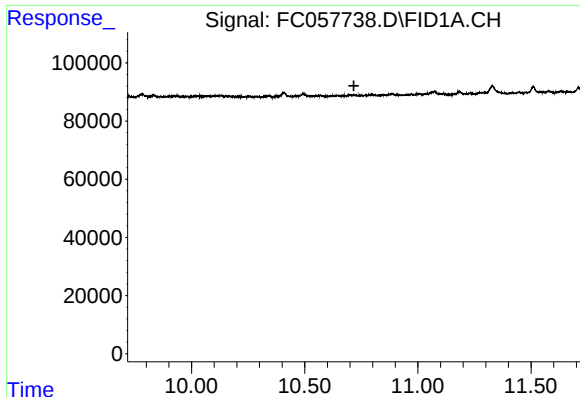

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.717 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

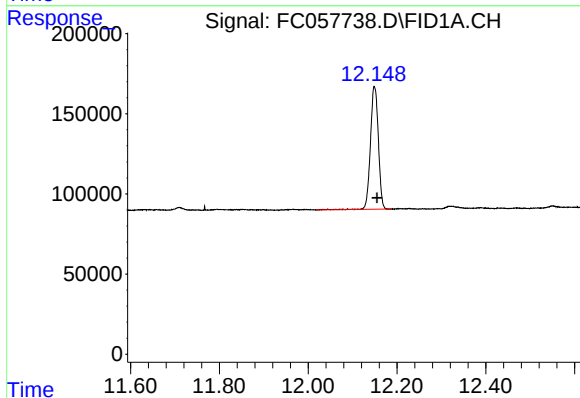


#12 1-chlorooctadecane (SURR)

R.T.: 12.150 min
Delta R.T.: -0.005 min
Response: 948934
Conc: 6.44 ug/ml

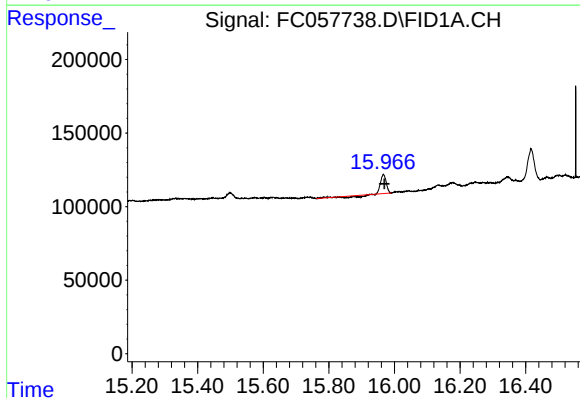


#16 n-Octacosane (C28)

R.T.: 15.966 min
Delta R.T.: -0.003 min
Response: 120816
Conc: 0.74 ug/ml

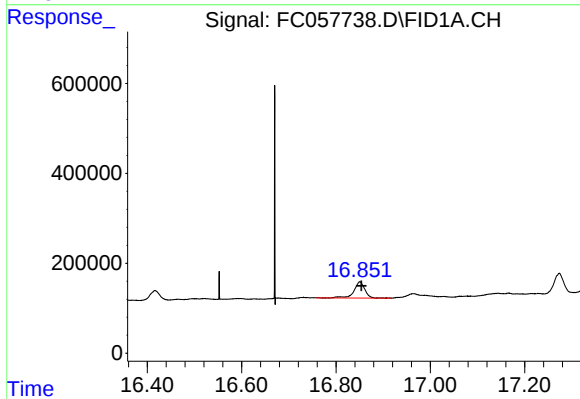

#17 n-Tricontane (C30)


R.T.: 16.851 min
Delta R.T.: -0.003 min
Response: 572864
Conc: 3.67 ug/ml

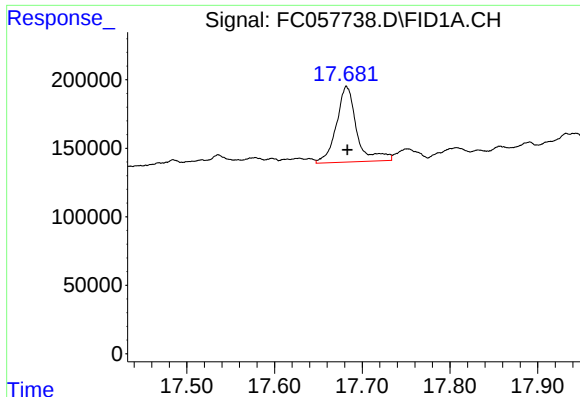

#18 n-Dotriacontane (C32)


R.T.: 17.682 min
Delta R.T.: 0.000 min
Response: 888225
Conc: 6.37 ug/ml

Instrument :
FID_C
ClientSampleId :

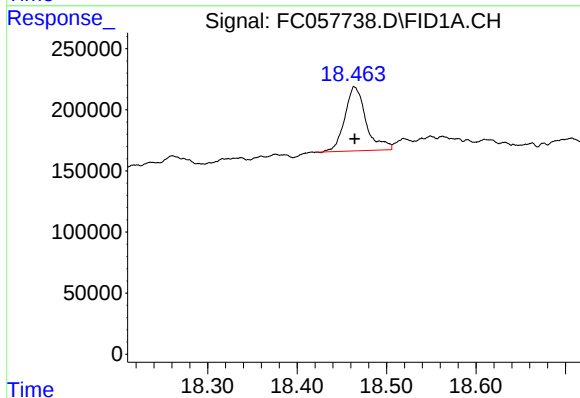


#19 n-Tetratriacontane (C34)

R.T.: 18.465 min
Delta R.T.: 0.000 min
Response: 863059
Conc: 6.94 ug/ml

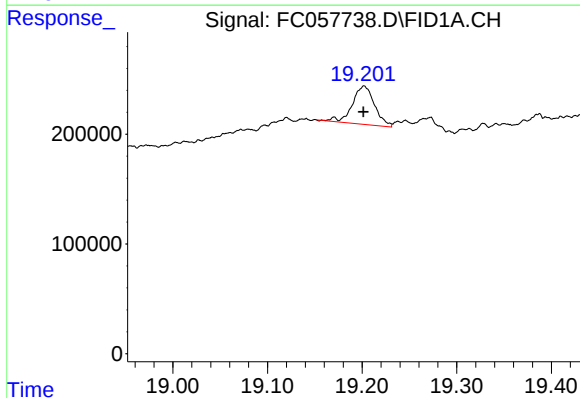


#20 n-Hexatriacontane (C36)

R.T.: 19.202 min
Delta R.T.: 0.000 min
Response: 568225
Conc: 5.11 ug/ml

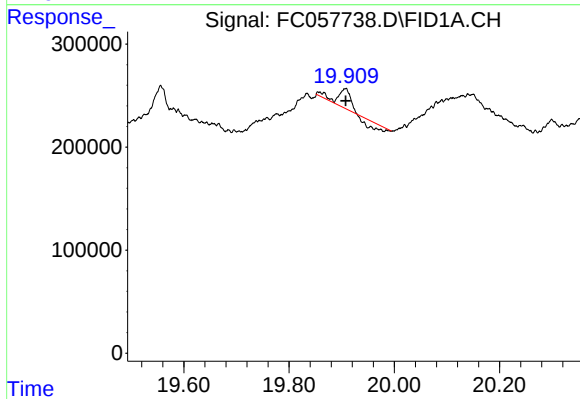

#21 n-Octatriacontane (C38)

R.T.: 19.907 min
Delta R.T.: 0.000 min
Response: 168429
Conc: 1.61 ug/ml

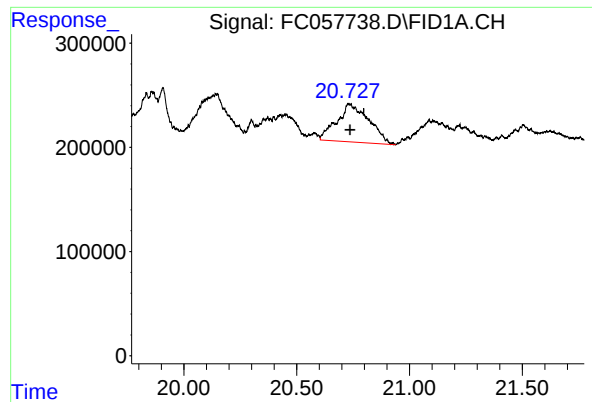

#22 n-Tetracontane (C40)

R.T.: 20.728 min
Delta R.T.: -0.009 min
Response: 3602992
Conc: 37.63 ug/ml

Instrument :

FID_C

ClientSampleId :