

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC010819AL\
 Data File : FC038508.D
 Signal(s) : FID1A.CH
 Acq On : 08 Jan 2019 23:43
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 09 04:56:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 15 05:55:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	12.961	511277	4.406 ug/ml
14) T n-Tetracosane (C24)	14.529	28648	0.250 ug/ml
15) T n-Hexacosane (C26)	15.588	54070	0.481 ug/ml
16) T n-Octacosane (C28)	16.534	62546	0.556 ug/ml
19) T n-Tetratriacontane (C34)	19.034	343622	3.899 ug/ml
20) T n-Hexatriacontane (C36)	19.708	861005	10.990 ug/ml
21) T n-Octatriacontane (C38)	20.417	4600580	59.453 ug/ml
22) T n-Tetracontane (C40)	21.281	248175	2.840 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC010819AL\
Data File : FC038508.D
Signal(s) : FID1A.CH
Acq On : 08 Jan 2019 23:43
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 09 04:56:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Sat Dec 15 05:55:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

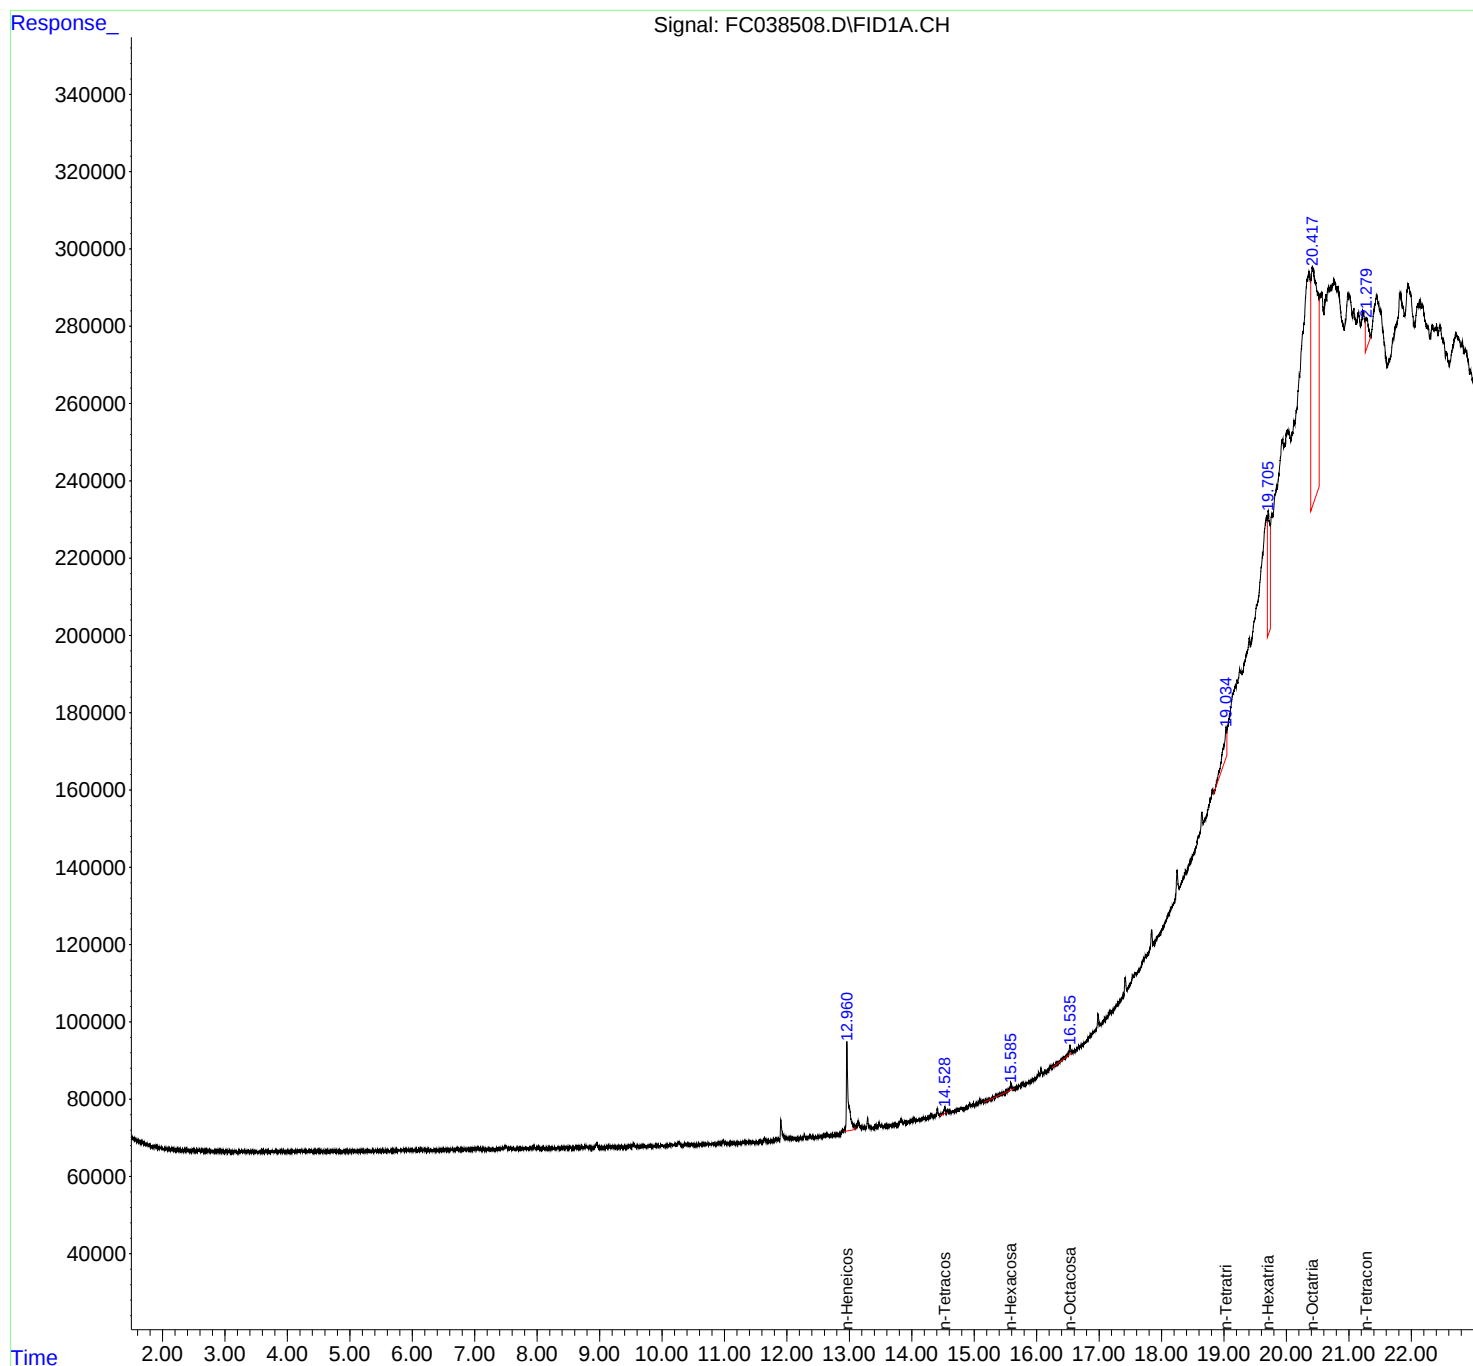

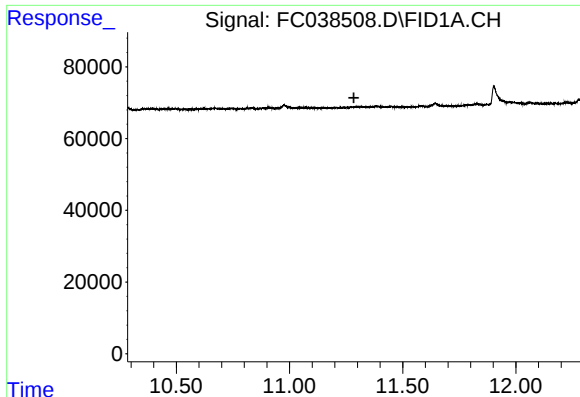


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.284 min
Response: 0
Conc: N.D.

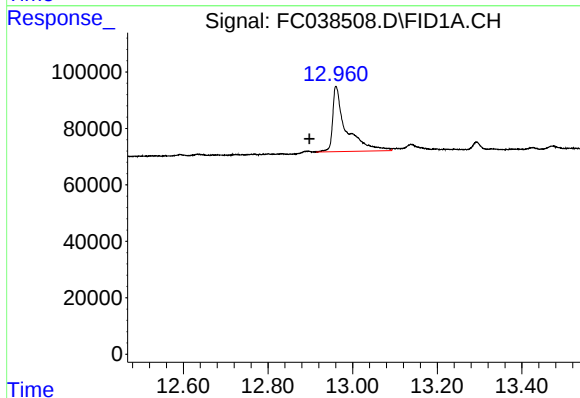


#11 n-Heneicosane (C21)

R.T.: 12.961 min
Delta R.T.: 0.064 min
Response: 511277
Conc: 4.41 ug/ml

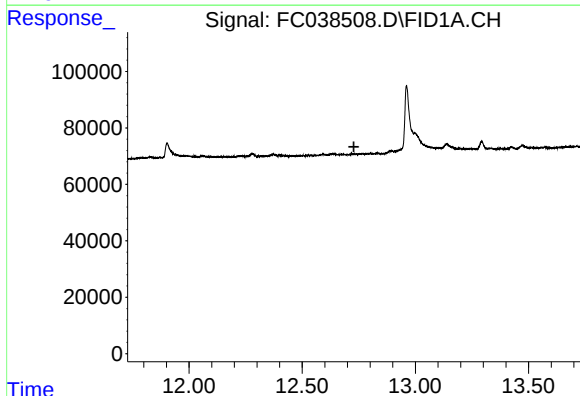


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.728 min
Response: 0
Conc: N.D.

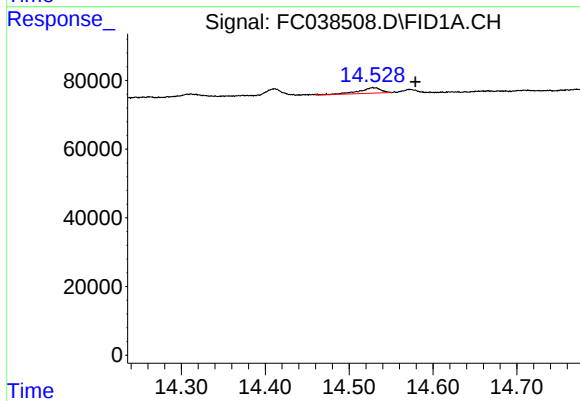


#14 n-Tetracosane (C24)

R.T.: 14.529 min
Delta R.T.: -0.050 min
Response: 28648
Conc: 0.25 ug/ml

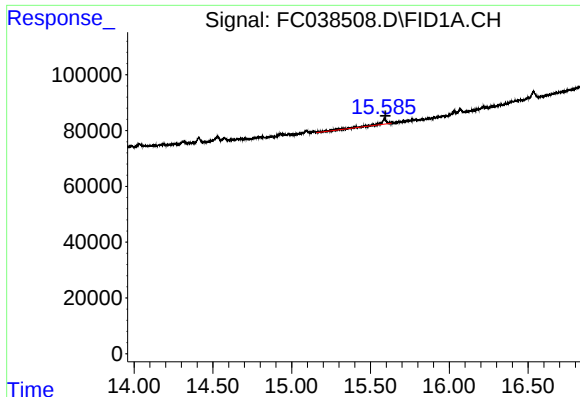


#15 n-Hexacosane (C26)

R.T.: 15.588 min
Delta R.T.: -0.006 min
Response: 54070
Conc: 0.48 ug/ml

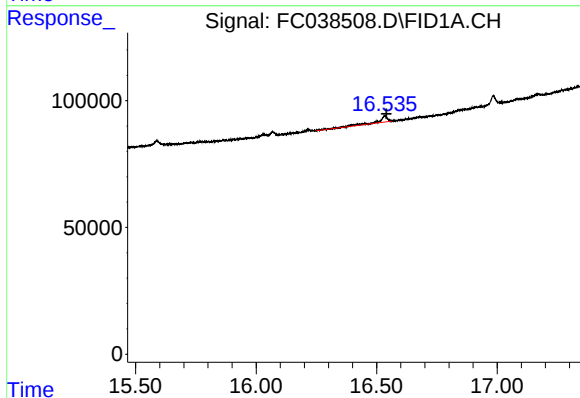


#16 n-Octacosane (C28)

R.T.: 16.534 min
Delta R.T.: -0.006 min
Response: 62546
Conc: 0.56 ug/ml

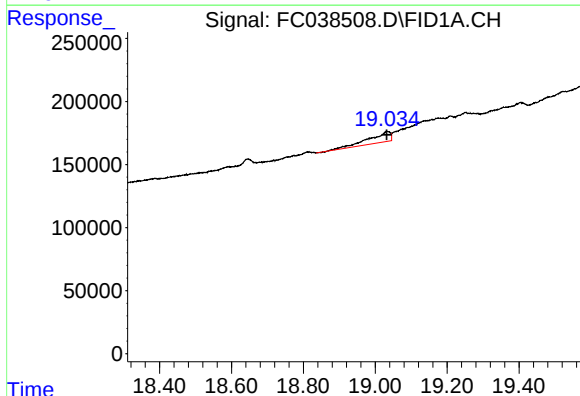


#19 n-Tetratriacontane (C34)

R.T.: 19.034 min
Delta R.T.: 0.002 min
Response: 343622
Conc: 3.90 ug/ml

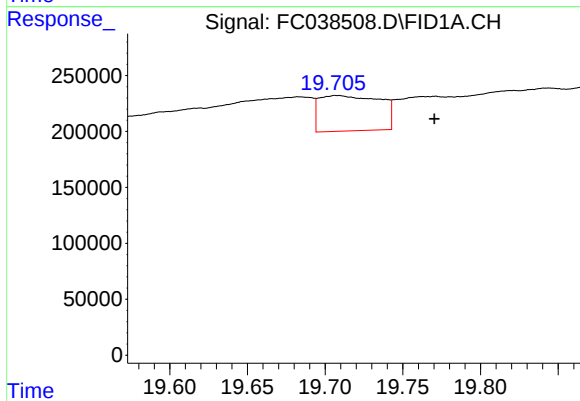


#20 n-Hexatriacontane (C36)

R.T.: 19.708 min
Delta R.T.: -0.063 min
Response: 861005
Conc: 10.99 ug/ml

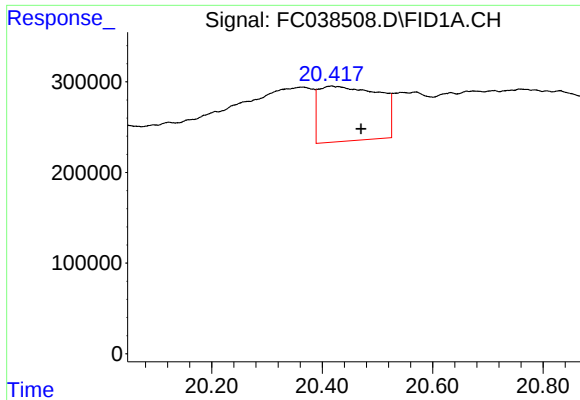

#21 n-Octatriacontane (C38)

R.T.: 20.417 min
Delta R.T.: -0.053 min
Response: 4600580
Conc: 59.45 ug/ml

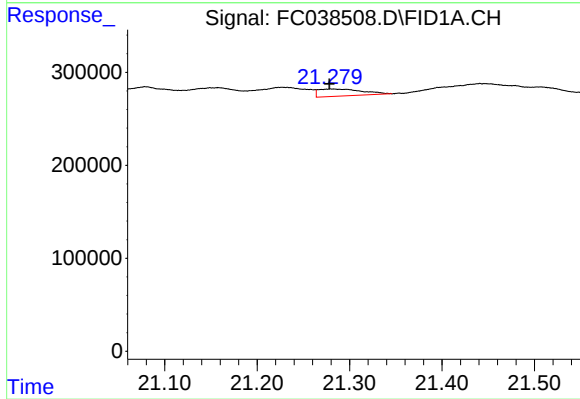

#22 n-Tetracontane (C40)

R.T.: 21.281 min
Delta R.T.: 0.003 min
Response: 248175
Conc: 2.84 ug/ml