

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011022AL\
 Data File : FC057785.D
 Signal(s) : FID1A.CH
 Acq On : 10 Jan 2022 9:00
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 00:09:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 12:13:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	12.870	270181	1.562 ug/ml
14) T n-Tetracosane (C24)	13.991	117139	0.677 ug/ml
15) T n-Hexacosane (C26)	15.013	175042	1.040 ug/ml
16) T n-Octacosane (C28)	15.958	183657	1.122 ug/ml
17) T n-Tricontane (C30)	16.843	301481	1.931 ug/ml
18) T n-Dotriacontane (C32)	17.672	225001	1.614 ug/ml
19) T n-Tetratriacontane (C34)	18.455	216934	1.745 ug/ml
20) T n-Hexatriacontane (C36)	19.192	325099	2.924 ug/ml
21) T n-Octatriacontane (C38)	19.888	488471	4.683 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011022AL\
Data File : FC057785.D
Signal(s) : FID1A.CH
Acq On : 10 Jan 2022 9:00
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 00:09:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 12:13:43 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

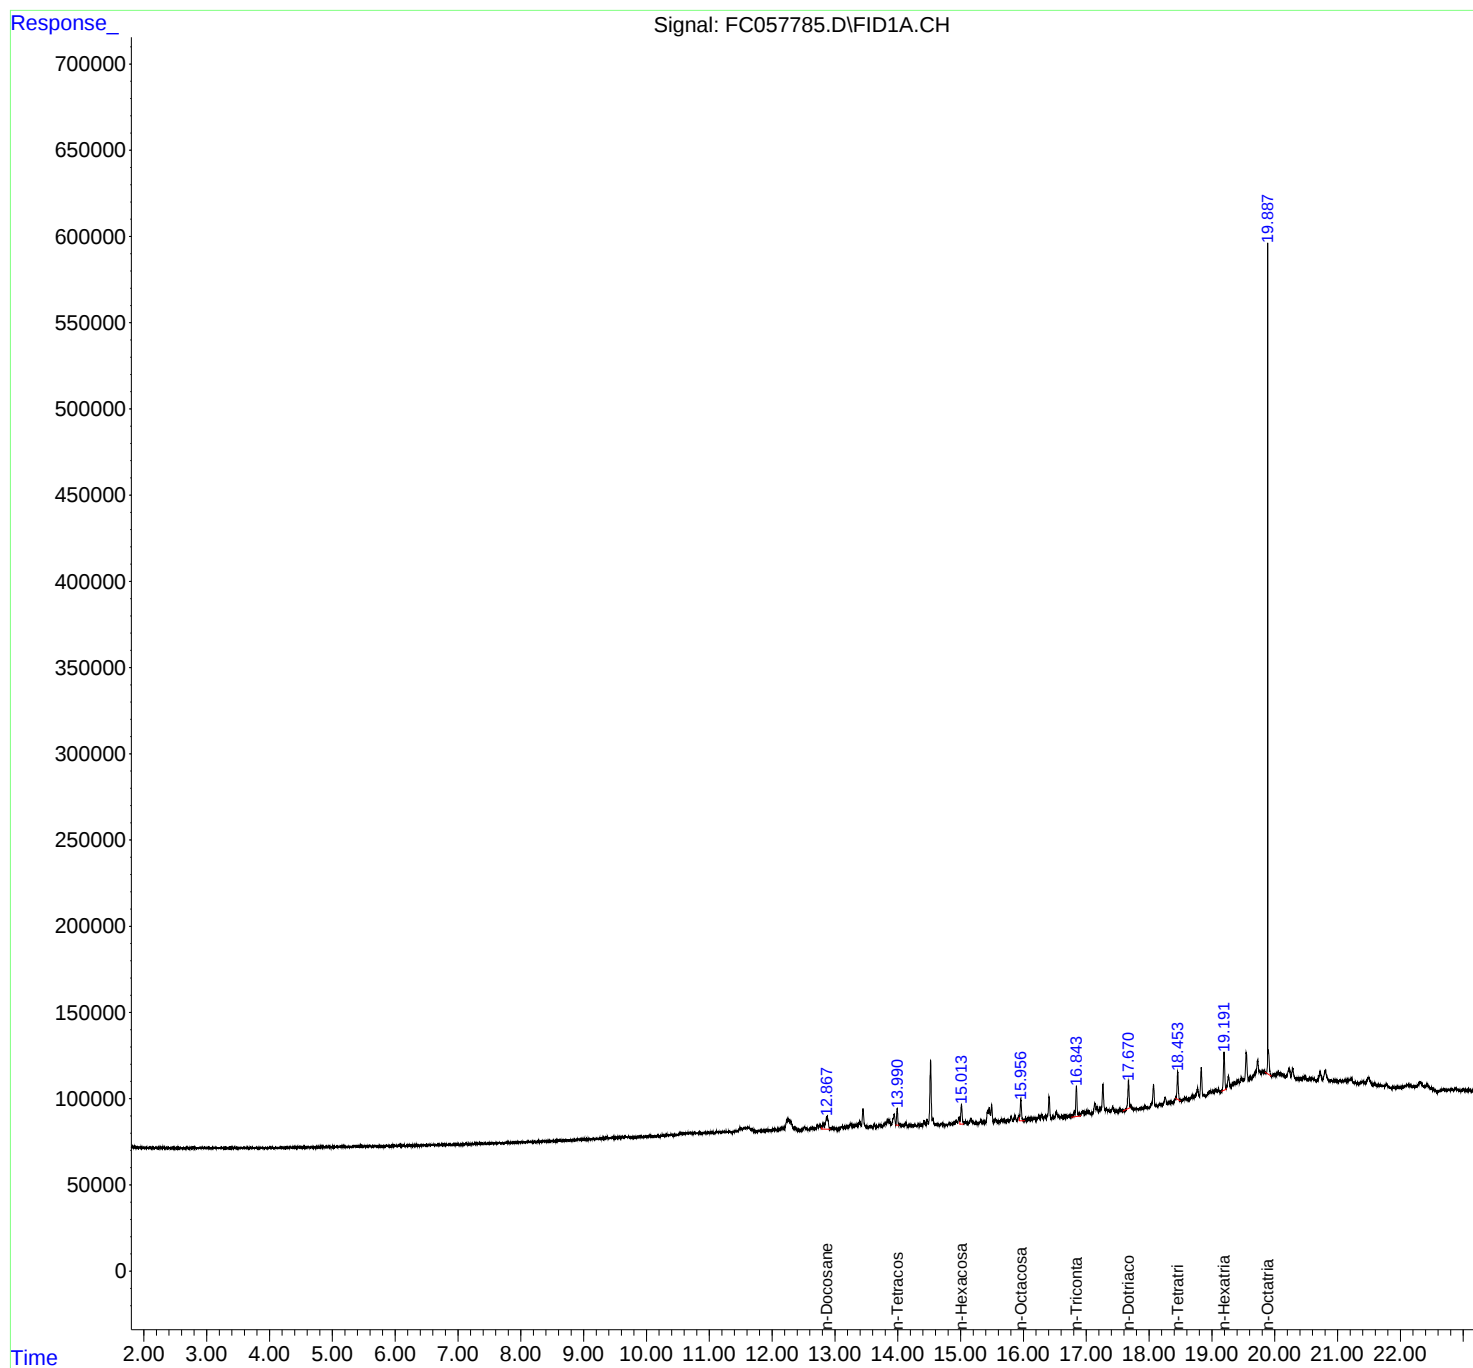


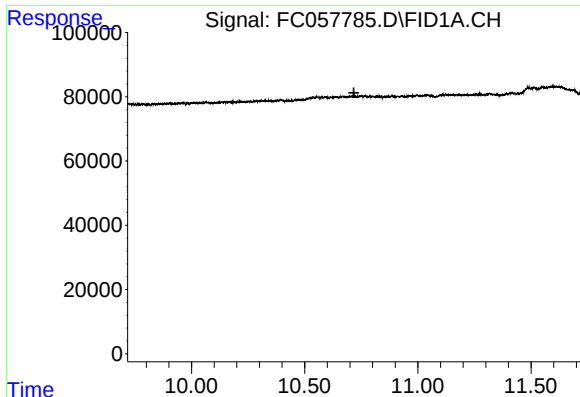

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.717 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

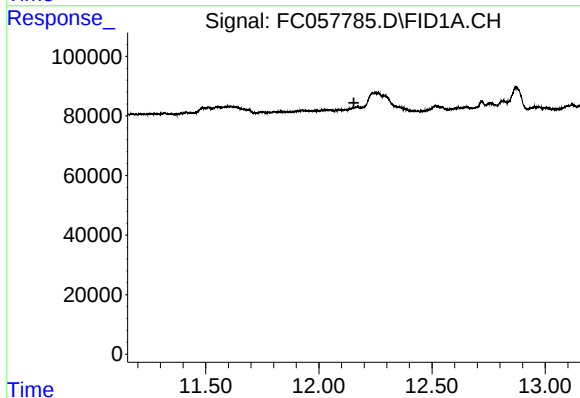


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.155 min
Response: 0
Conc: N.D.

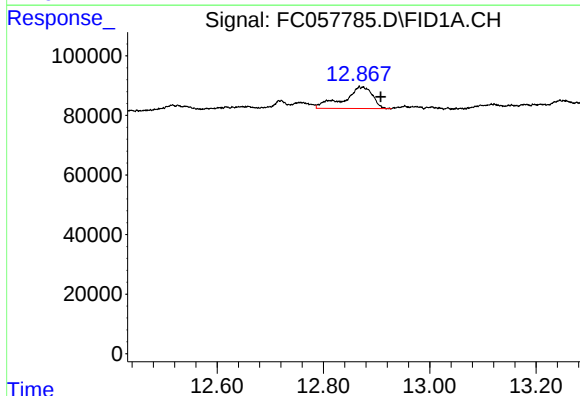


#13 n-Docosane (C22)

R.T.: 12.870 min
Delta R.T.: -0.038 min
Response: 270181
Conc: 1.56 ug/ml

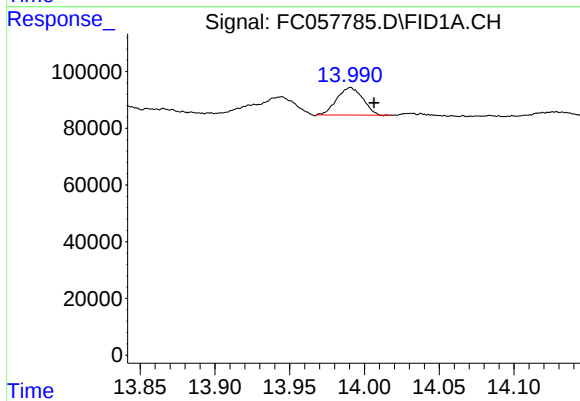

#14 n-Tetracosane (C24)


R.T.: 13.991 min
Delta R.T.: -0.016 min
Response: 117139
Conc: 0.68 ug/ml

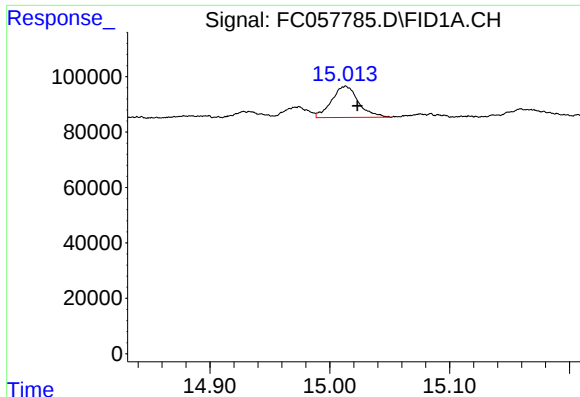

#15 n-Hexacosane (C26)


R.T.: 15.013 min
Delta R.T.: -0.010 min
Response: 175042
Conc: 1.04 ug/ml

Instrument :
FID_C
ClientSampleId :

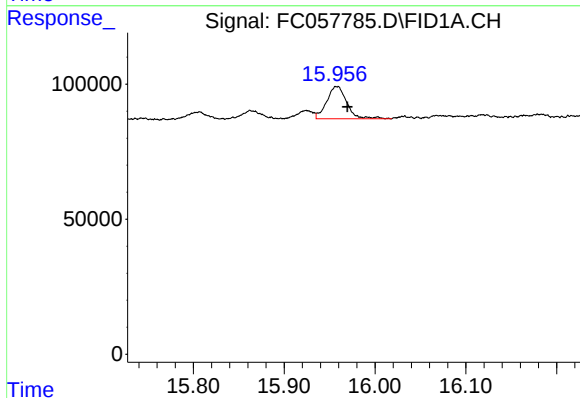


#16 n-Octacosane (C28)

R.T.: 15.958 min
Delta R.T.: -0.012 min
Response: 183657
Conc: 1.12 ug/ml

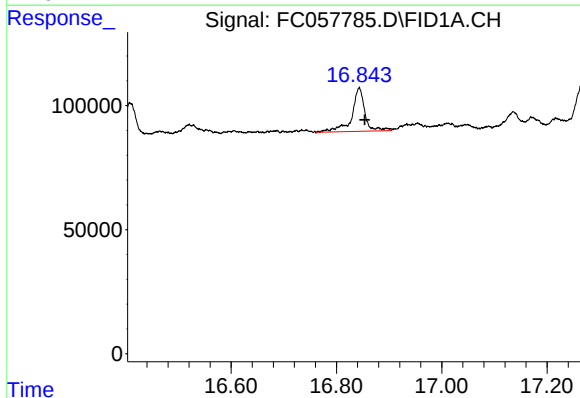


#17 n-Tricontane (C30)

R.T.: 16.843 min
Delta R.T.: -0.011 min
Response: 301481
Conc: 1.93 ug/ml

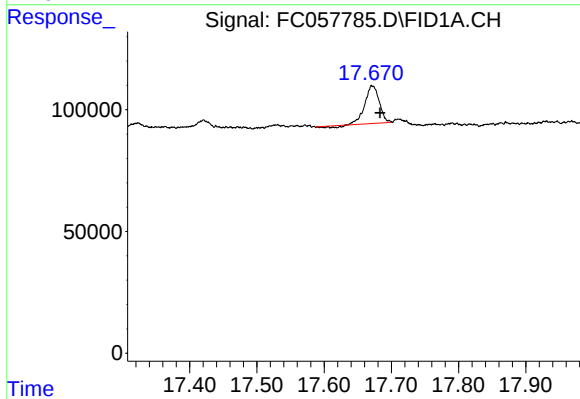

#18 n-Dotriacontane (C32)


R.T.: 17.672 min
Delta R.T.: -0.011 min
Response: 225001
Conc: 1.61 ug/ml

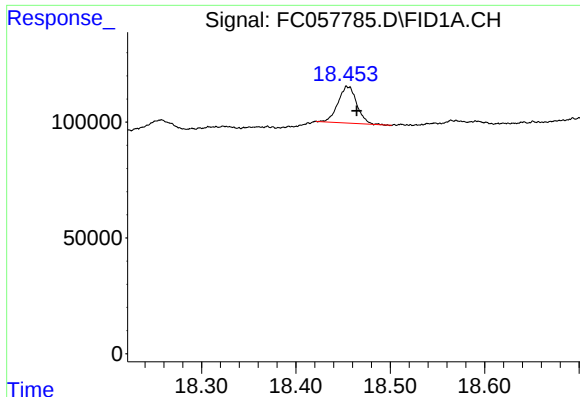

#19 n-Tetratriacontane (C34)


R.T.: 18.455 min
Delta R.T.: -0.009 min
Response: 216934
Conc: 1.75 ug/ml

Instrument :
FID_C
ClientSampleId :

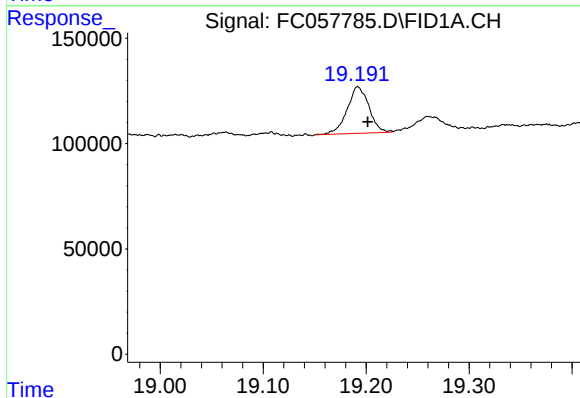

#20 n-Hexatriacontane (C36)

R.T.: 19.192 min
Delta R.T.: -0.009 min
Response: 325099
Conc: 2.92 ug/ml

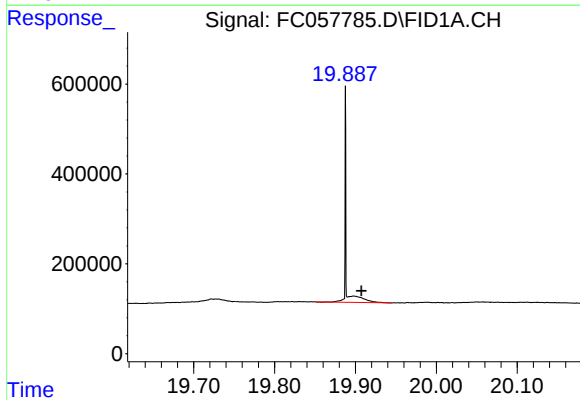

#21 n-Octatriacontane (C38)

R.T.: 19.888 min
Delta R.T.: -0.019 min
Response: 488471
Conc: 4.68 ug/ml