

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011023AL\
Data File : FC062601.D
Signal(s) : FID1A.ch
Acq On : 10 Jan 2023 09:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 05:47:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.703	63408	0.586 ug/ml
18) T	n-Dotriacontane (C32)	18.532	80311	0.736 ug/ml
19) T	n-Tetratriacontane (C34)	19.312	61710	0.568 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011023AL\
Data File : FC062601.D
Signal(s) : FID1A.ch
Acq On : 10 Jan 2023 09:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 05:47:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

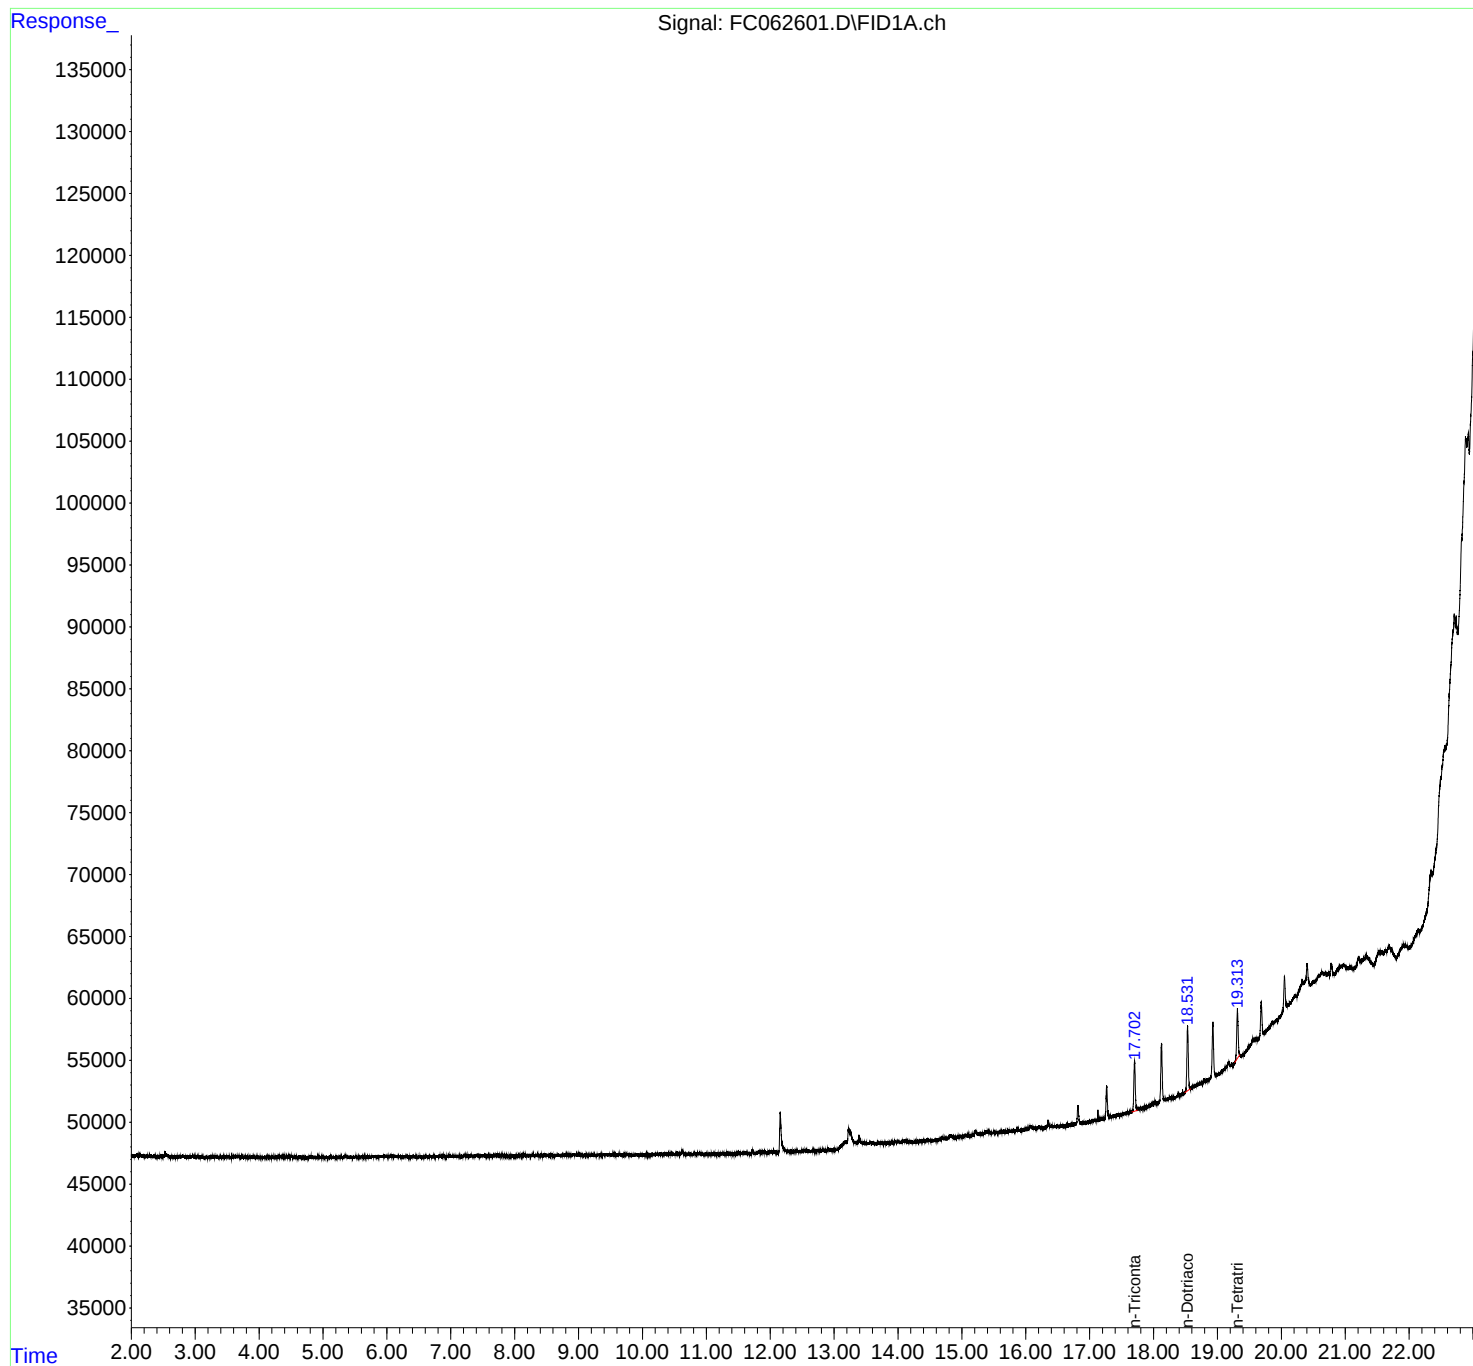


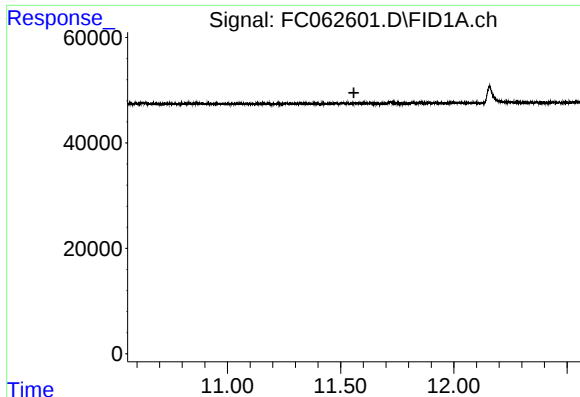

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.558 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

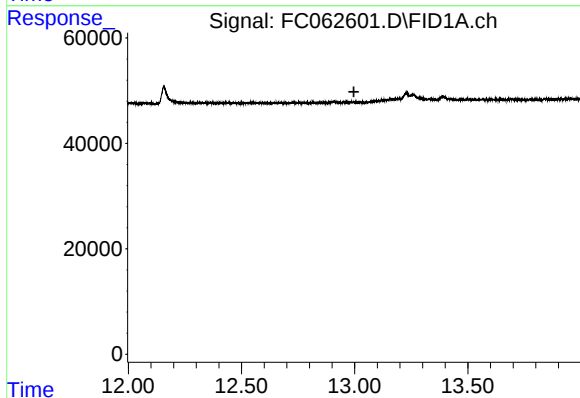


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.997 min
Response: 0
Conc: N.D.

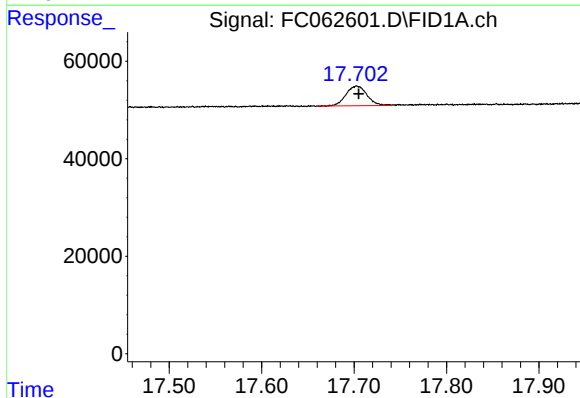


#17 n-Tricontane (C30)

R.T.: 17.703 min
Delta R.T.: -0.002 min
Response: 63408
Conc: 0.59 ug/ml

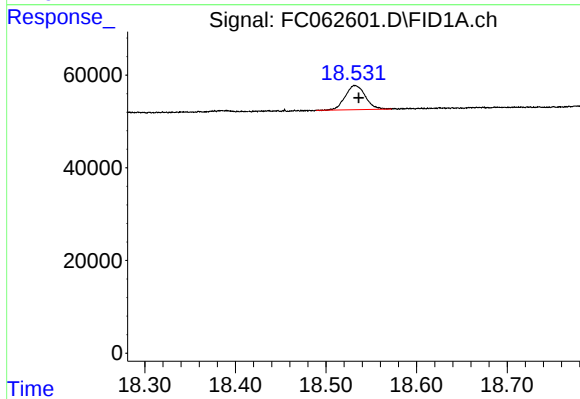

#18 n-Dotriacontane (C32)

R.T.: 18.532 min
Delta R.T.: -0.004 min
Response: 80311
Conc: 0.74 ug/ml

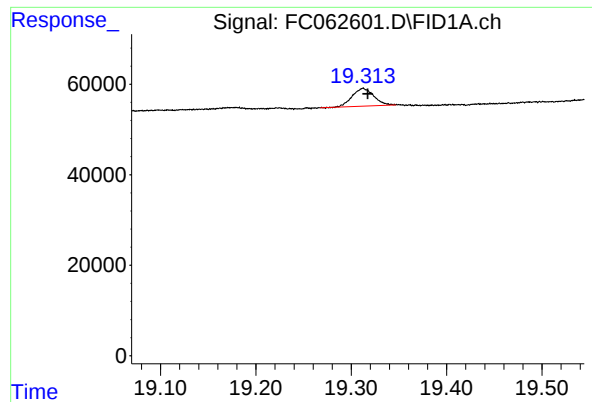

#19 n-Tetratriacontane (C34)

R.T.: 19.312 min
Delta R.T.: -0.005 min
Response: 61710
Conc: 0.57 ug/ml

Instrument :

FID_C

ClientSampleId :