

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011023AL\
 Data File : FC062604.D
 Signal(s) : FID1A.ch
 Acq On : 10 Jan 2023 12:17
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 05:47:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 04:54:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.180	187290	1.528 ug/ml
14) T	n-Tetracosane (C24)	14.797f	53450	0.459 ug/ml
17) T	n-Tricontane (C30)	17.705	103854	0.959 ug/ml
18) T	n-Dotriacontane (C32)	18.533	135706	1.243 ug/ml
19) T	n-Tetratriacontane (C34)	19.314	147954	1.361 ug/ml
20) T	n-Hexatriacontane (C36)	20.052	168680	1.516 ug/ml
21) T	n-Octatriacontane (C38)	20.785	2389758	22.565 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011023AL\
Data File : FC062604.D
Signal(s) : FID1A.ch
Acq On : 10 Jan 2023 12:17
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 05:47:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

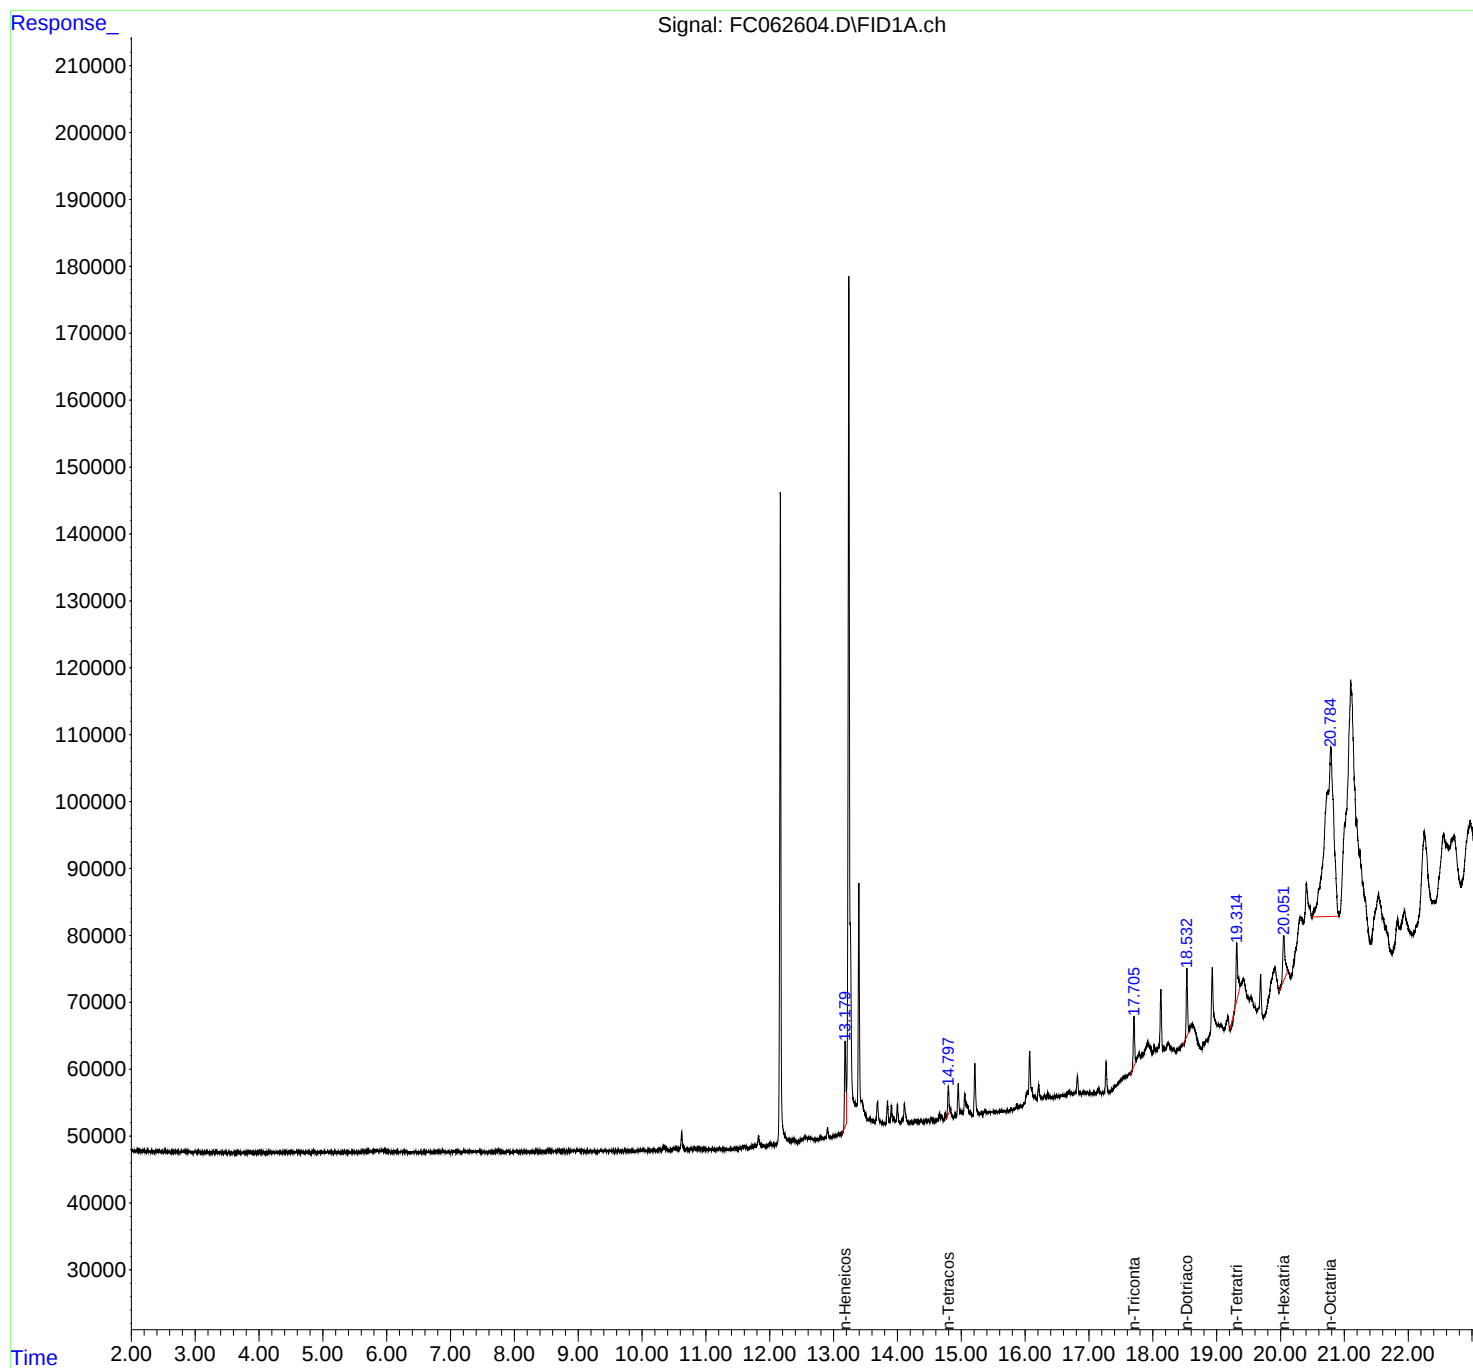


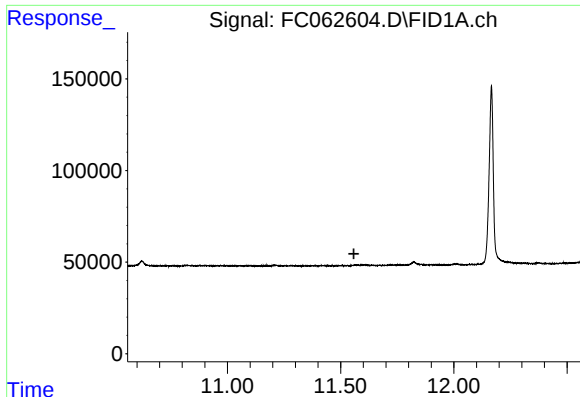

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.558 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

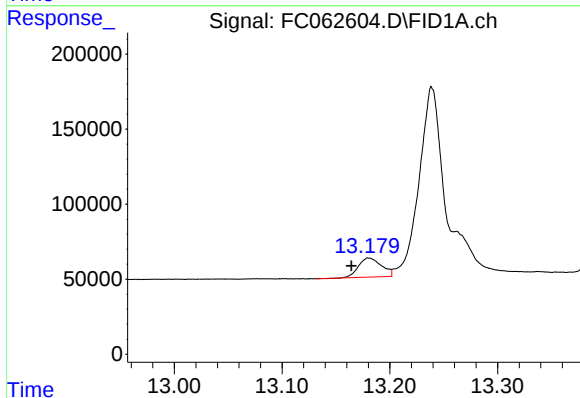


#11 n-Heneicosane (C21)

R.T.: 13.180 min
Delta R.T.: 0.016 min
Response: 187290
Conc: 1.53 ug/ml

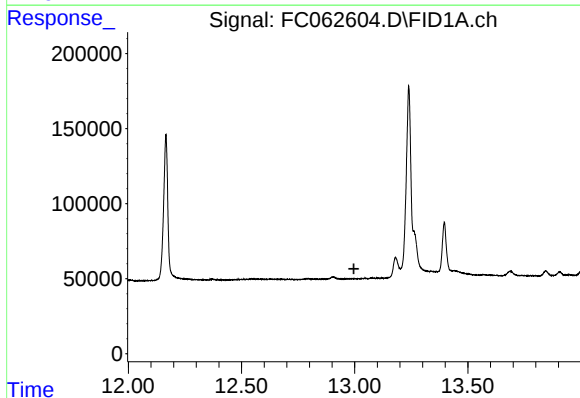


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.997 min
Response: 0
Conc: N.D.

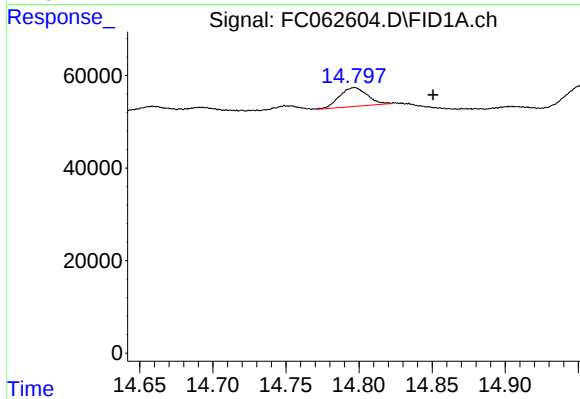

#14 n-Tetracosane (C24)


R.T.: 14.797 min
Delta R.T.: -0.054 min
Response: 53450
Conc: 0.46 ug/ml

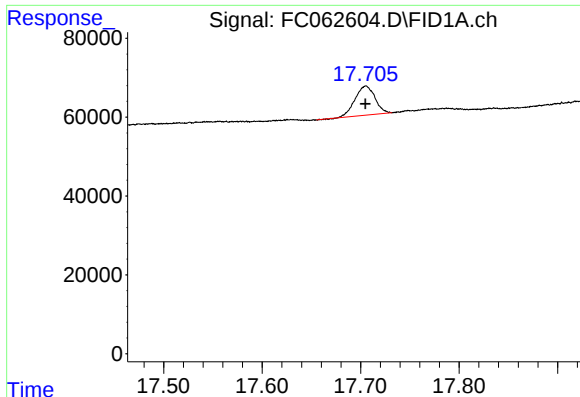

#17 n-Tricontane (C30)


R.T.: 17.705 min
Delta R.T.: 0.000 min
Response: 103854
Conc: 0.96 ug/ml

Instrument :
FID_C
ClientSampleId :

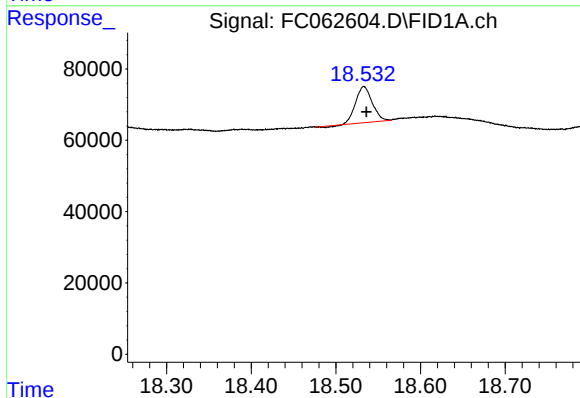


#18 n-Dotriacontane (C32)

R.T.: 18.533 min
Delta R.T.: -0.003 min
Response: 135706
Conc: 1.24 ug/ml

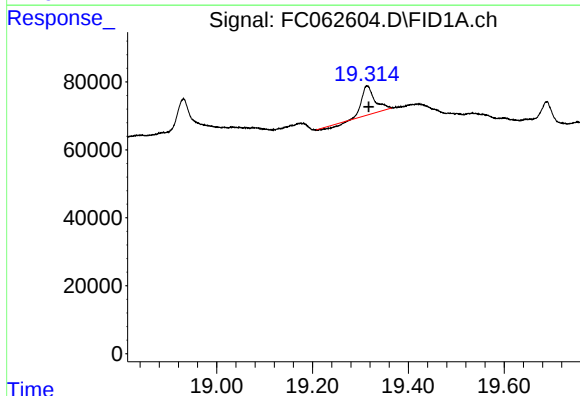


#19 n-Tetratriacontane (C34)

R.T.: 19.314 min
Delta R.T.: -0.003 min
Response: 147954
Conc: 1.36 ug/ml

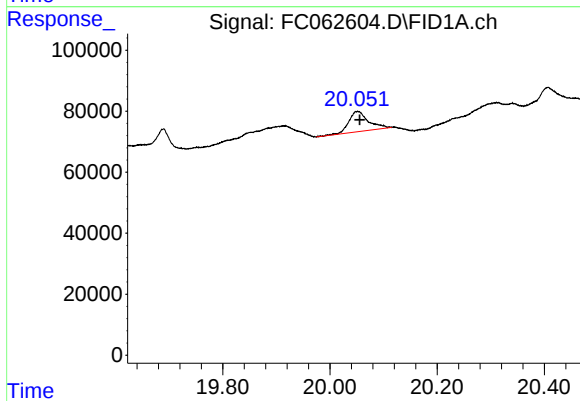

#20 n-Hexatriacontane (C36)

R.T.: 20.052 min
Delta R.T.: -0.004 min
Response: 168680
Conc: 1.52 ug/ml

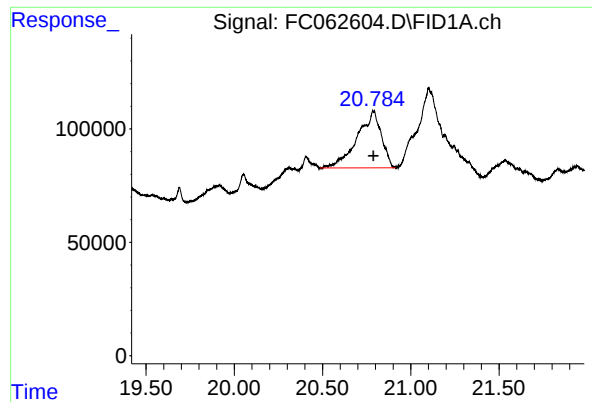

#21 n-Octatriacontane (C38)

R.T.: 20.785 min
Delta R.T.: -0.003 min
Response: 2389758
Conc: 22.57 ug/ml

Instrument :

FID_C

ClientSampleId :