

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011023AL\
 Data File : FC062611.D
 Signal(s) : FID1A.ch
 Acq On : 10 Jan 2023 20:27
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 11 05:48:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 04:54:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.226f	31433	0.256 ug/ml
17) T n-Tricontane (C30)	17.701	121565	1.123 ug/ml
18) T n-Dotriacontane (C32)	18.531	127394	1.167 ug/ml
19) T n-Tetratriacontane (C34)	19.313	323396	2.975 ug/ml
20) T n-Hexatriacontane (C36)	20.053	341830	3.073 ug/ml
21) T n-Octatriacontane (C38)	20.784	270786	2.557 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011023AL\
Data File : FC062611.D
Signal(s) : FID1A.ch
Acq On : 10 Jan 2023 20:27
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 11 05:48:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

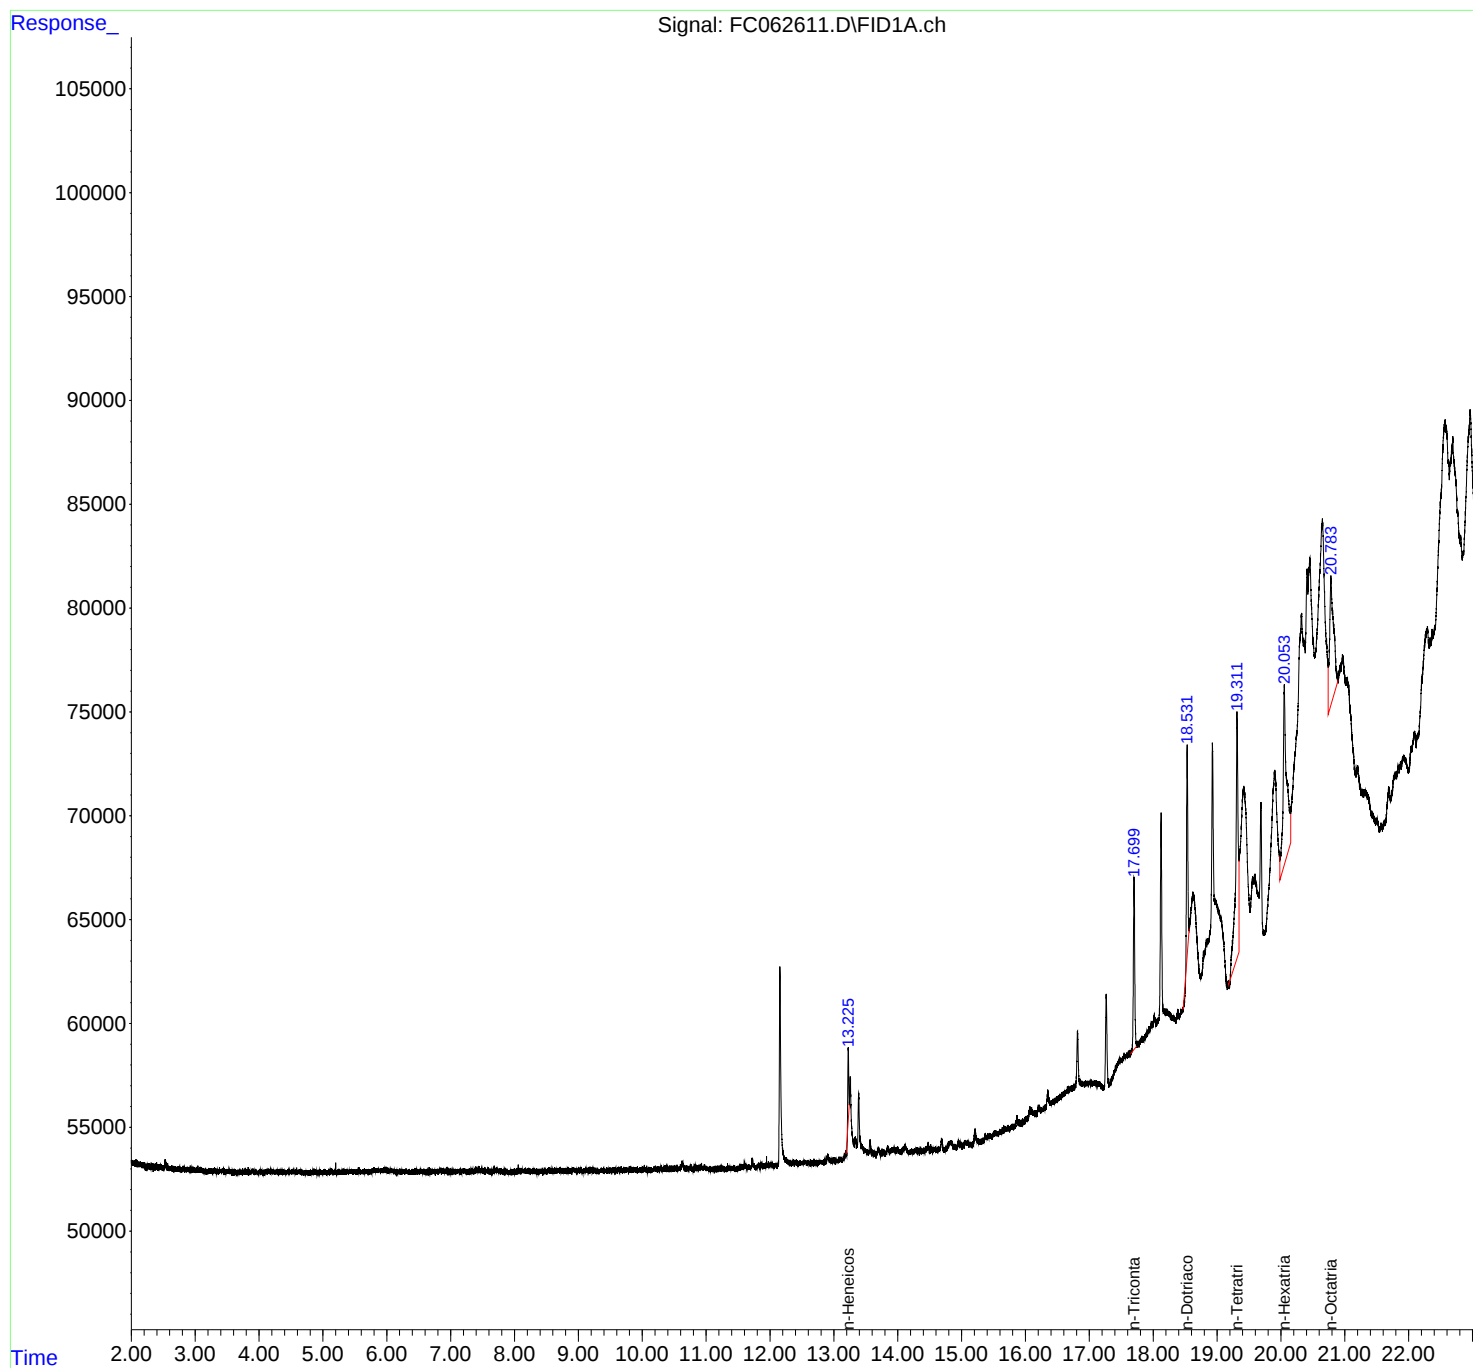


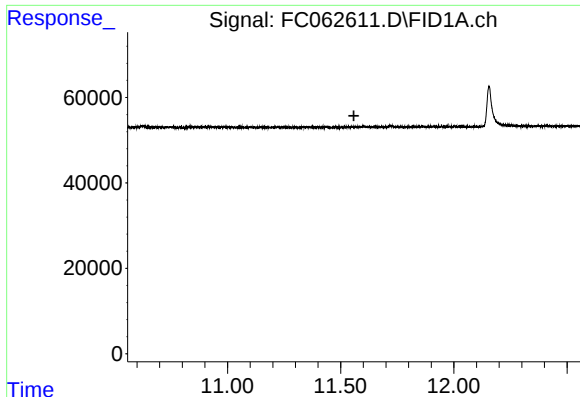

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.558 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

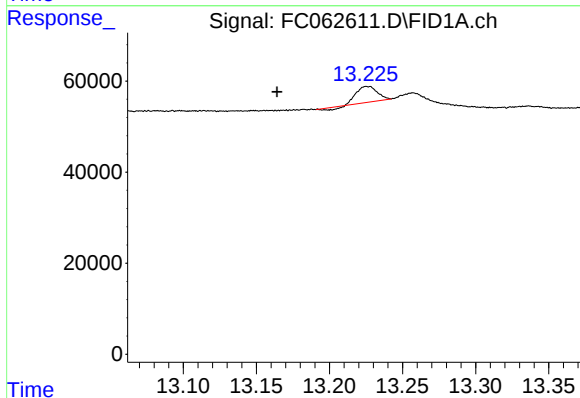


#11 n-Heneicosane (C21)

R.T.: 13.226 min
Delta R.T.: 0.062 min
Response: 31433
Conc: 0.26 ug/ml

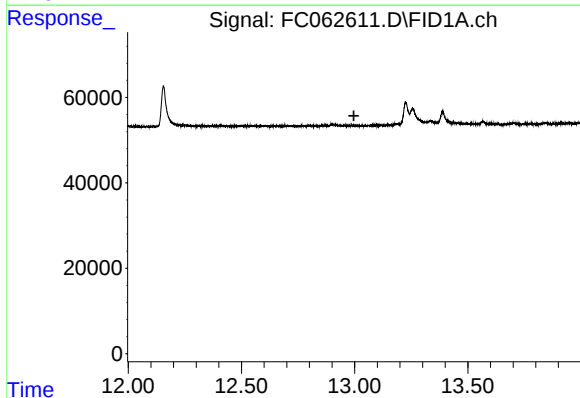


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.997 min
Response: 0
Conc: N.D.

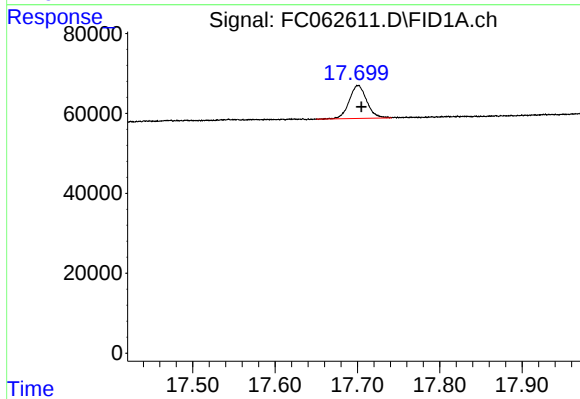

#17 n-Tricontane (C30)


R.T.: 17.701 min
Delta R.T.: -0.004 min
Response: 121565
Conc: 1.12 ug/ml

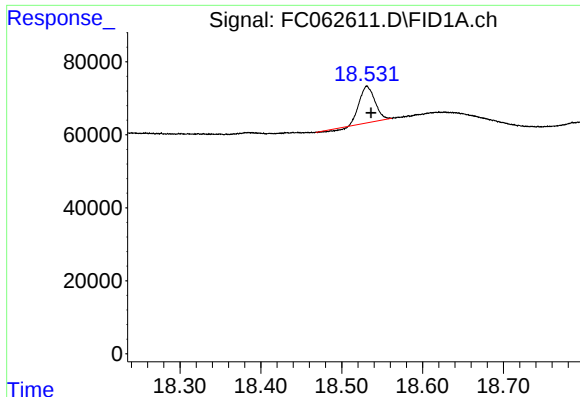

#18 n-Dotriacontane (C32)


R.T.: 18.531 min
Delta R.T.: -0.005 min
Response: 127394
Conc: 1.17 ug/ml

Instrument :
FID_C
ClientSampleId :

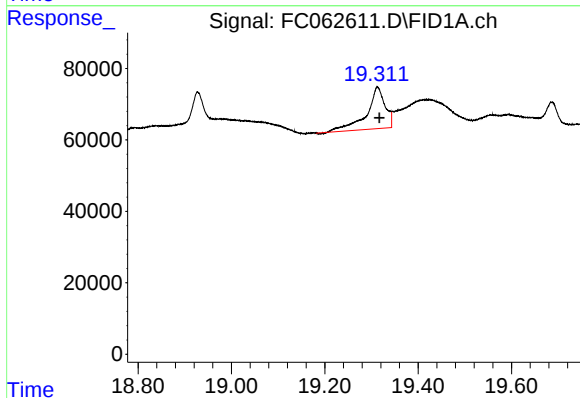


#19 n-Tetratriacontane (C34)

R.T.: 19.313 min
Delta R.T.: -0.005 min
Response: 323396
Conc: 2.97 ug/ml

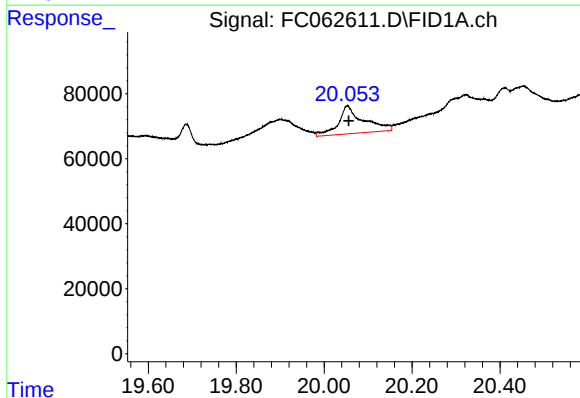

#20 n-Hexatriacontane (C36)

R.T.: 20.053 min
Delta R.T.: -0.003 min
Response: 341830
Conc: 3.07 ug/ml

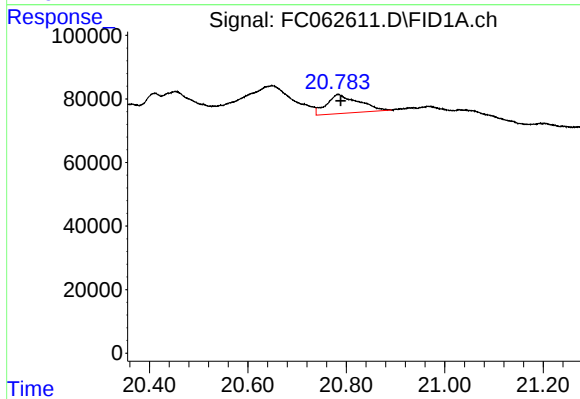

#21 n-Octatriacontane (C38)

R.T.: 20.784 min
Delta R.T.: -0.005 min
Response: 270786
Conc: 2.56 ug/ml