

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011623AL\
Data File : FC062666.D
Signal(s) : FID1A.ch
Acq On : 16 Jan 2023 08:15
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 02:01:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.157	206585	1.686 ug/ml
14) T	n-Tetracosane (C24)	14.846	54275	0.466 ug/ml
17) T	n-Tricontane (C30)	17.701	79242	0.732 ug/ml
18) T	n-Dotriacontane (C32)	18.533	190795	1.748 ug/ml
19) T	n-Tetratriacontane (C34)	19.312	149821	1.378 ug/ml
20) T	n-Hexatriacontane (C36)	20.051	150239	1.351 ug/ml
22) T	n-Tetracontane (C40)	21.746	218066	2.048 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011623AL\
Data File : FC062666.D
Signal(s) : FID1A.ch
Acq On : 16 Jan 2023 08:15
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 02:01:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010523.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

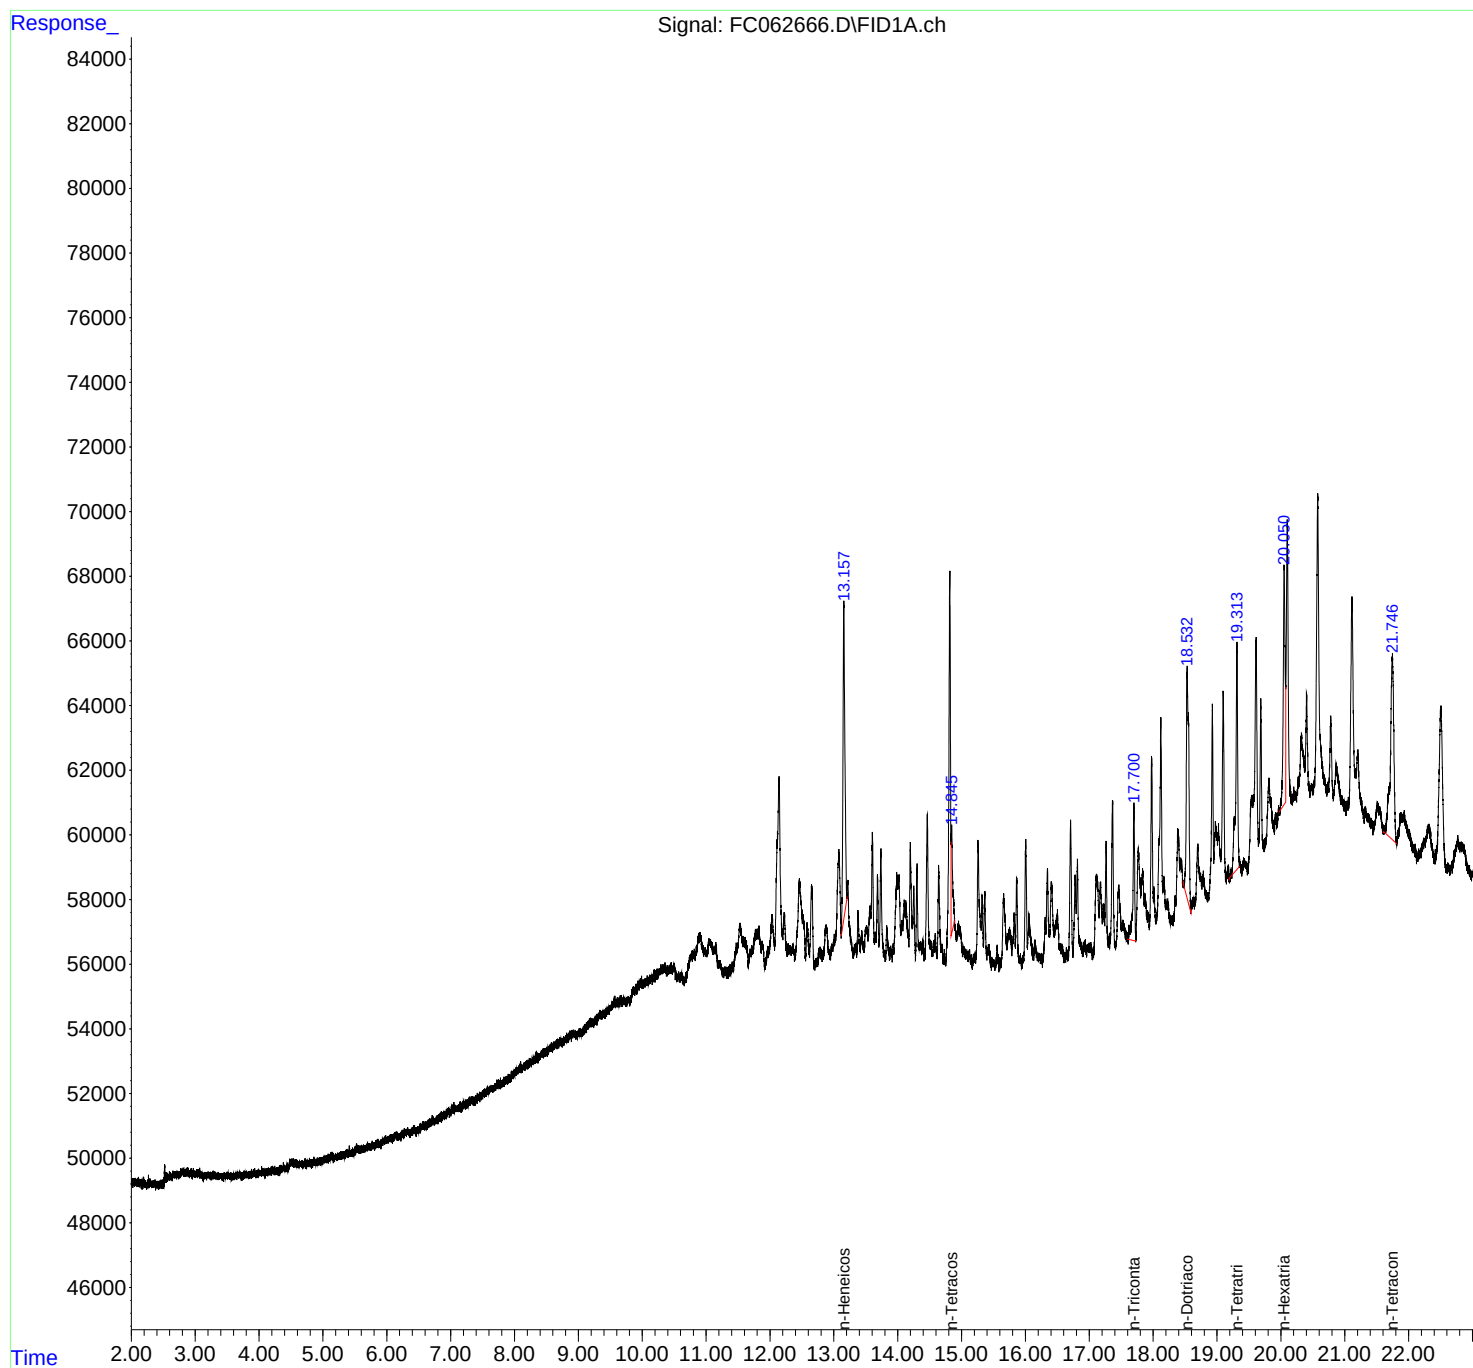


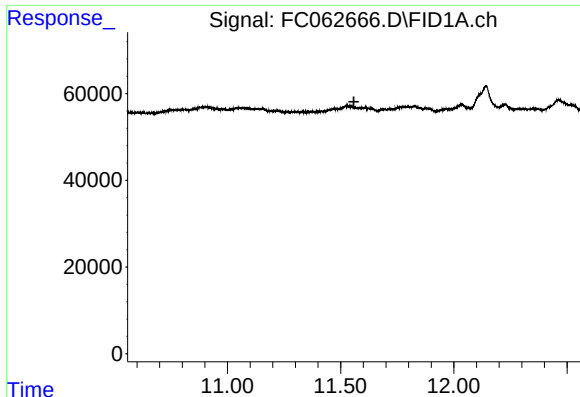

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.558 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

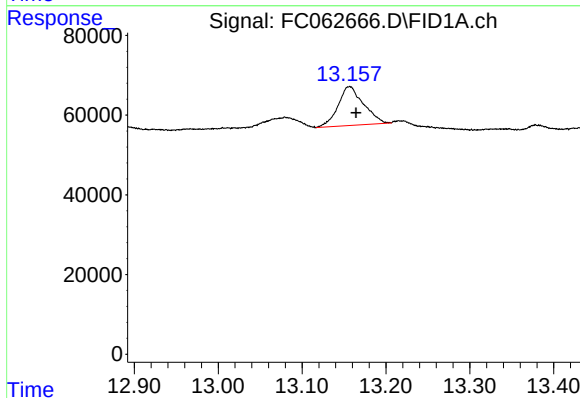


#11 n-Heneicosane (C21)

R.T.: 13.157 min
Delta R.T.: -0.008 min
Response: 206585
Conc: 1.69 ug/ml

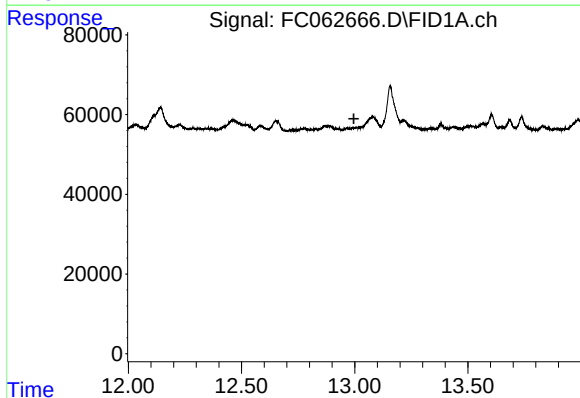


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.997 min
Response: 0
Conc: N.D.

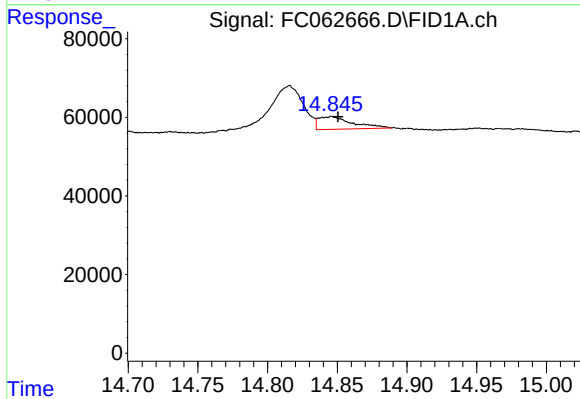

#14 n-Tetracosane (C24)


R.T.: 14.846 min
Delta R.T.: -0.005 min
Response: 54275
Conc: 0.47 ug/ml

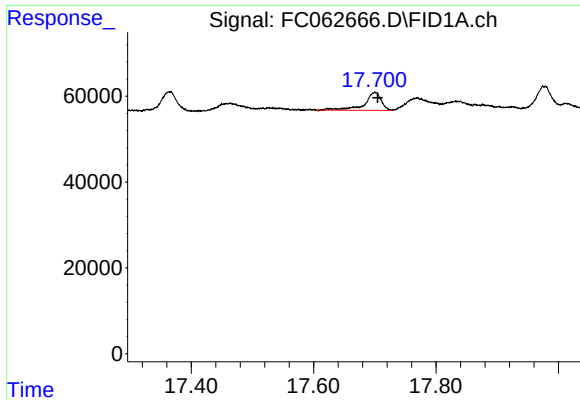

#17 n-Tricontane (C30)


R.T.: 17.701 min
Delta R.T.: -0.004 min
Response: 79242
Conc: 0.73 ug/ml

Instrument :
FID_C
ClientSampleId :

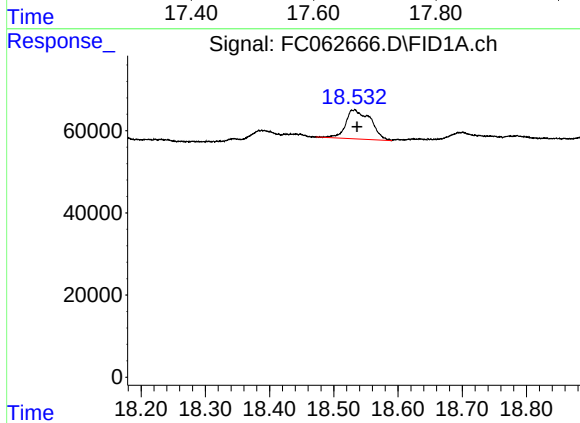


#18 n-Dotriacontane (C32)

R.T.: 18.533 min
Delta R.T.: -0.003 min
Response: 190795
Conc: 1.75 ug/ml

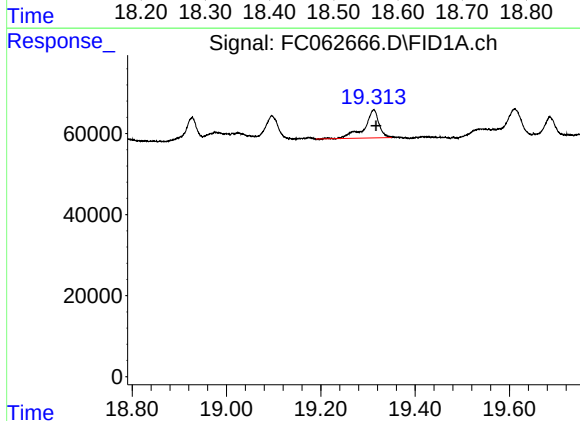


#19 n-Tetratriacontane (C34)

R.T.: 19.312 min
Delta R.T.: -0.005 min
Response: 149821
Conc: 1.38 ug/ml

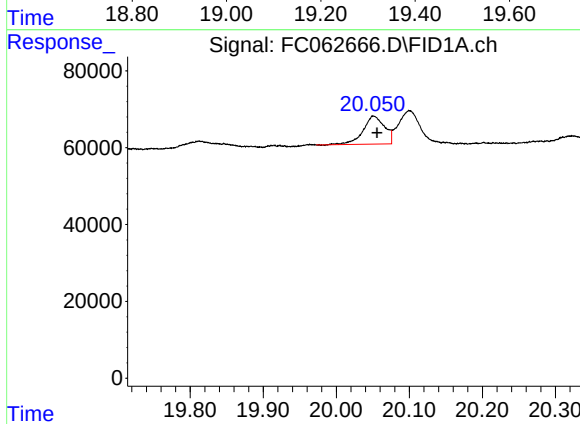

#20 n-Hexatriacontane (C36)

R.T.: 20.051 min
Delta R.T.: -0.005 min
Response: 150239
Conc: 1.35 ug/ml

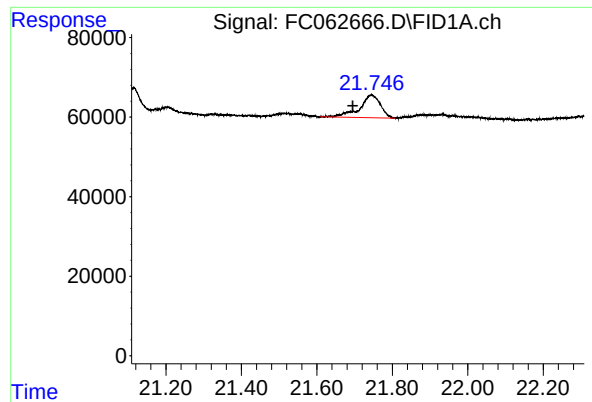

#22 n-Tetracontane (C40)

R.T.: 21.746 min
Delta R.T.: 0.051 min
Response: 218066
Conc: 2.05 ug/ml

Instrument :
FID_C
ClientSampleId :