

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011722AL\
 Data File : FC057939.D
 Signal(s) : FID1A.CH
 Acq On : 17 Jan 2022 9:26
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 18 00:49:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 12:13:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	12.874	769632	4.449 ug/ml
14) T n-Tetracosane (C24)	13.997	332044	1.918 ug/ml
15) T n-Hexacosane (C26)	15.019	405651	2.410 ug/ml
16) T n-Octacosane (C28)	15.967	309002	1.888 ug/ml
17) T n-Tricontane (C30)	16.853	315881	2.023 ug/ml
18) T n-Dotriacontane (C32)	17.680	377740	2.709 ug/ml
19) T n-Tetratriacontane (C34)	18.468	197417	1.588 ug/ml
20) T n-Hexatriacontane (C36)	19.206	249826	2.247 ug/ml
21) T n-Octatriacontane (C38)	19.914	190014	1.822 ug/ml
22) T n-Tetracontane (C40)	20.742	204659	2.137 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011722AL\
Data File : FC057939.D
Signal(s) : FID1A.CH
Acq On : 17 Jan 2022 9:26
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 18 00:49:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 12:13:43 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

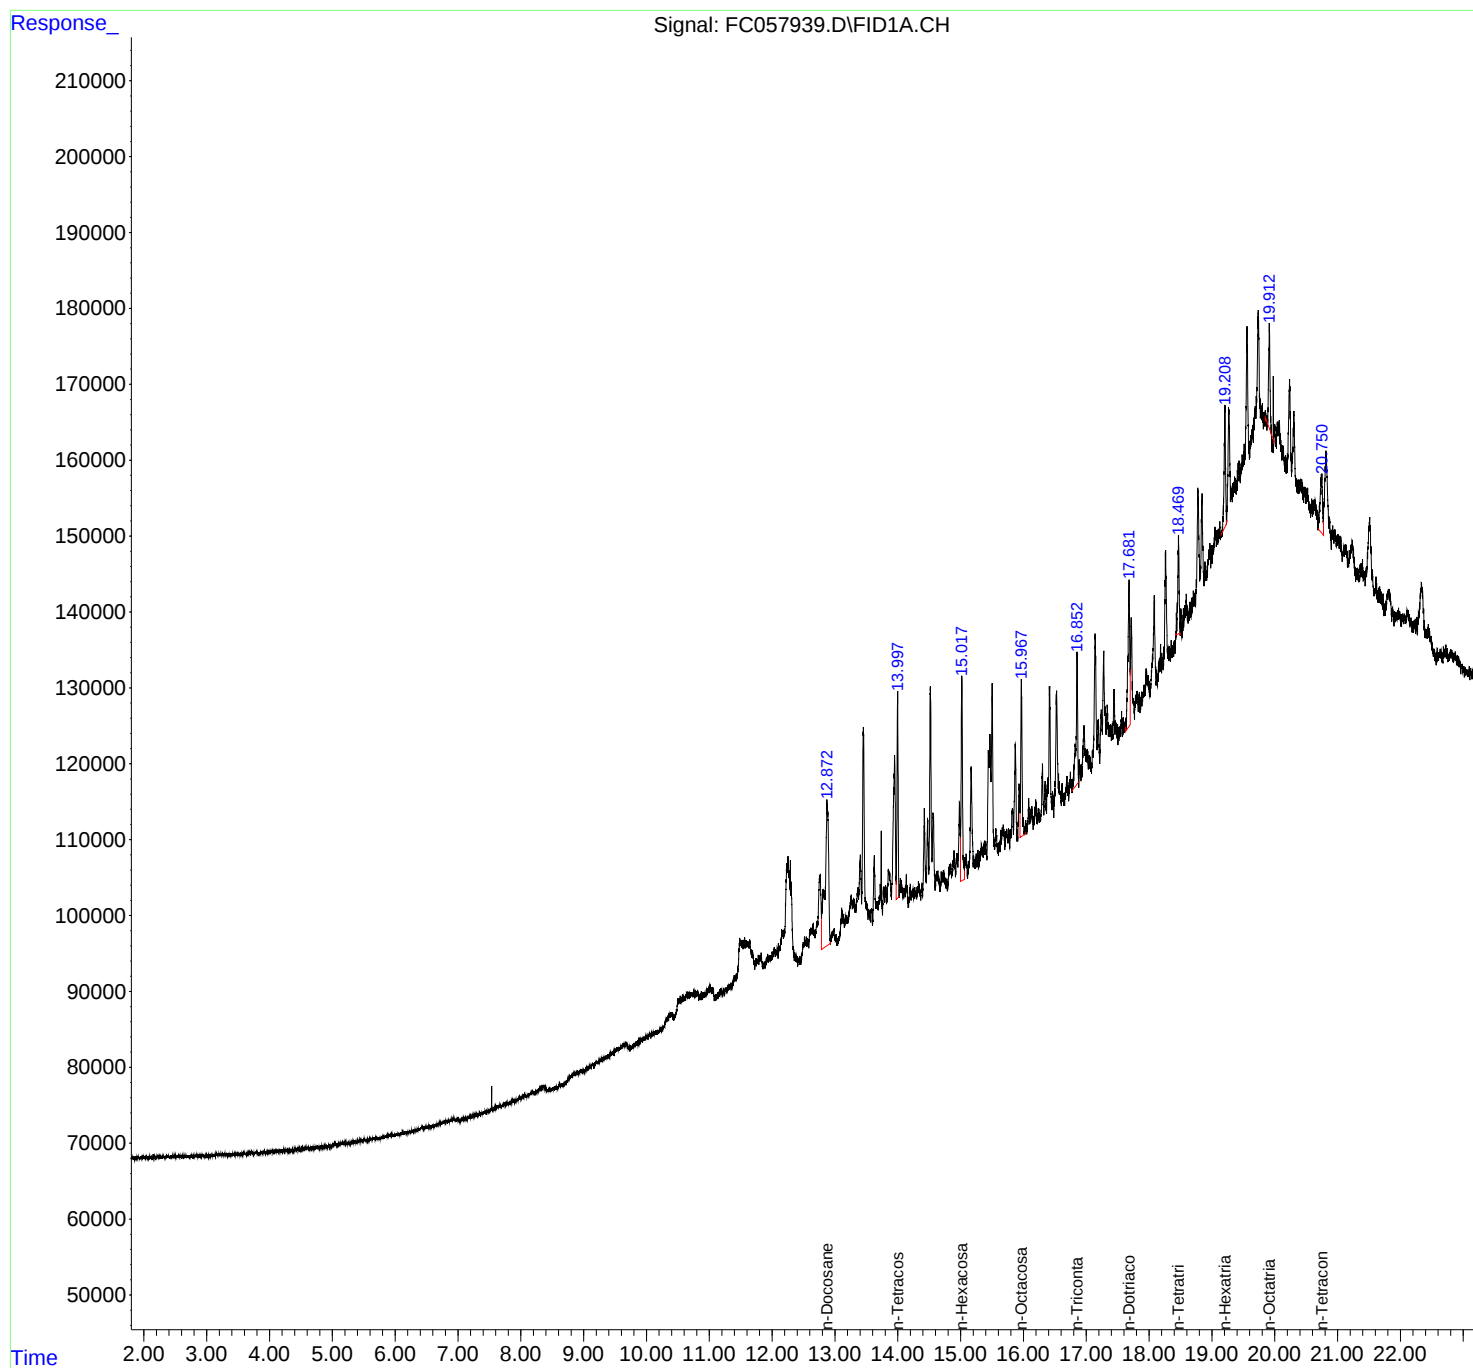


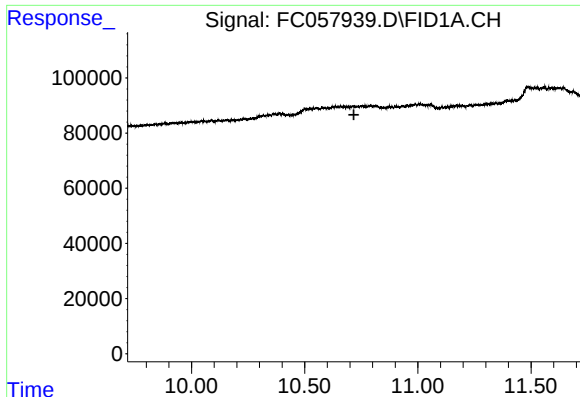

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.717 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

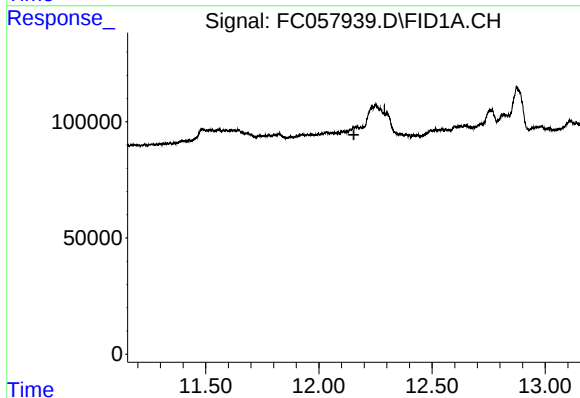


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.155 min
Response: 0
Conc: N.D.

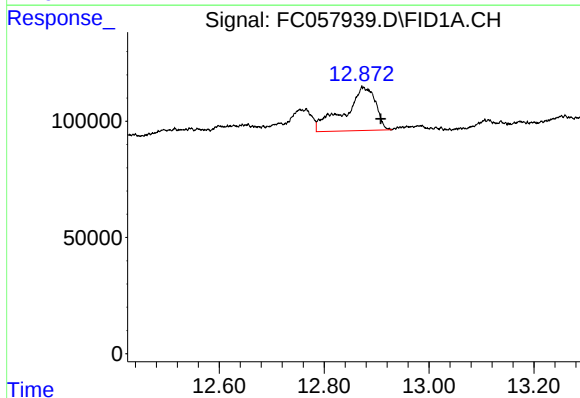


#13 n-Docosane (C22)

R.T.: 12.874 min
Delta R.T.: -0.034 min
Response: 769632
Conc: 4.45 ug/ml

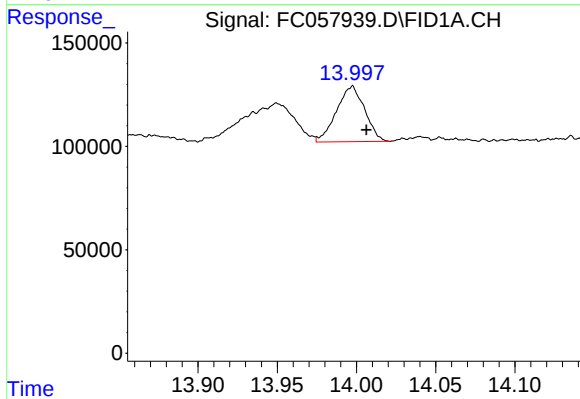

#14 n-Tetracosane (C24)


R.T.: 13.997 min
Delta R.T.: -0.009 min
Response: 332044
Conc: 1.92 ug/ml

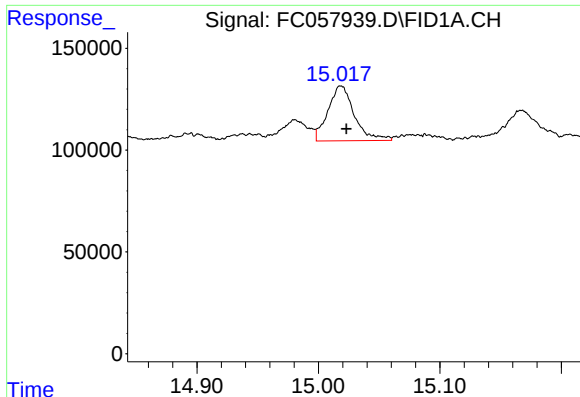

#15 n-Hexacosane (C26)


R.T.: 15.019 min
Delta R.T.: -0.005 min
Response: 405651
Conc: 2.41 ug/ml

Instrument :
FID_C
ClientSampleId :

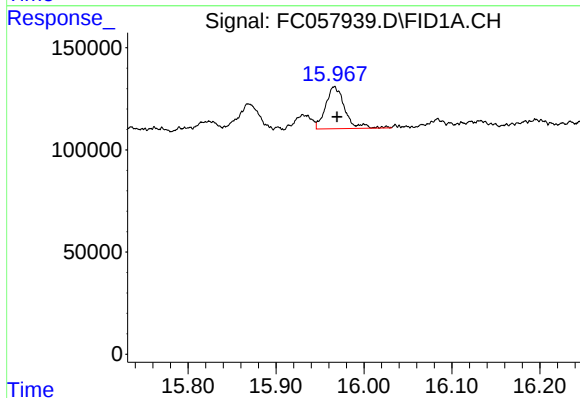


#16 n-Octacosane (C28)

R.T.: 15.967 min
Delta R.T.: -0.003 min
Response: 309002
Conc: 1.89 ug/ml

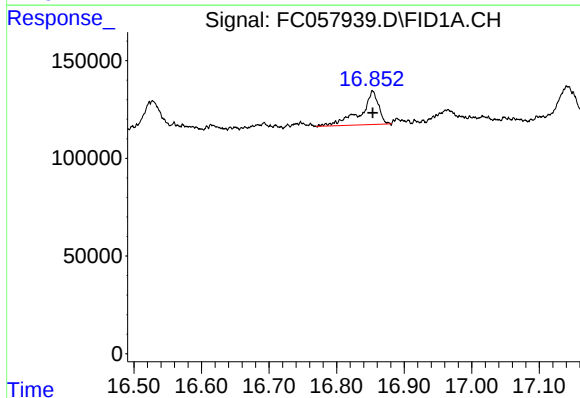


#17 n-Tricontane (C30)

R.T.: 16.853 min
Delta R.T.: 0.000 min
Response: 315881
Conc: 2.02 ug/ml

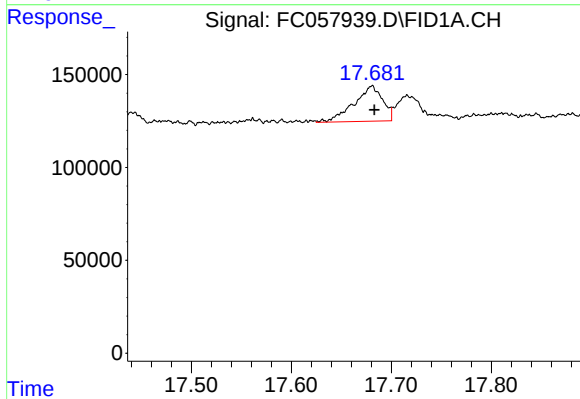

#18 n-Dotriacontane (C32)


R.T.: 17.680 min
Delta R.T.: -0.003 min
Response: 377740
Conc: 2.71 ug/ml

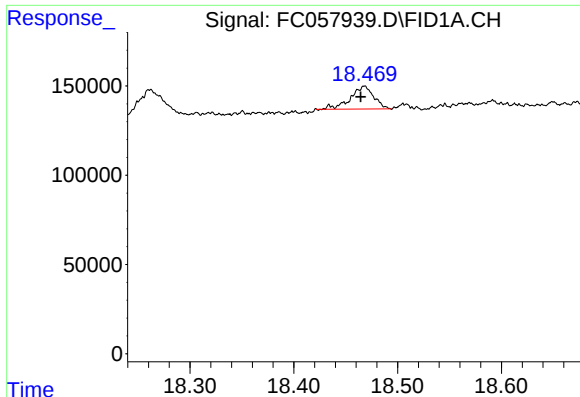

#19 n-Tetratriacontane (C34)


R.T.: 18.468 min
Delta R.T.: 0.003 min
Response: 197417
Conc: 1.59 ug/ml

Instrument :
FID_C
ClientSampleId :

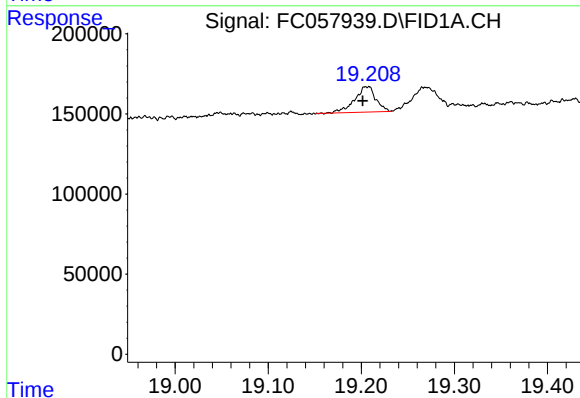


#20 n-Hexatriacontane (C36)

R.T.: 19.206 min
Delta R.T.: 0.005 min
Response: 249826
Conc: 2.25 ug/ml

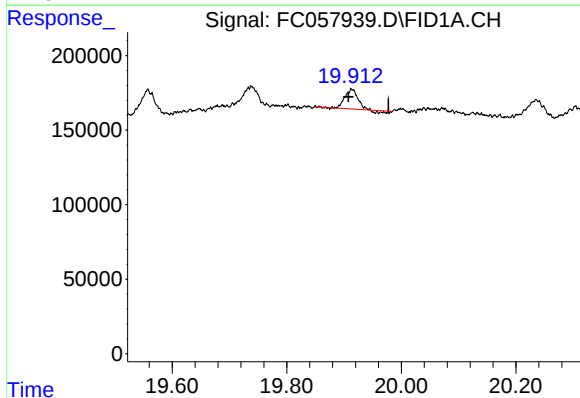

#21 n-Octatriacontane (C38)

R.T.: 19.914 min
Delta R.T.: 0.006 min
Response: 190014
Conc: 1.82 ug/ml

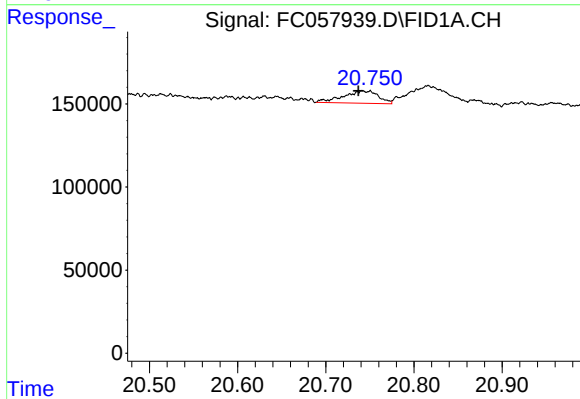

#22 n-Tetracontane (C40)

R.T.: 20.742 min
Delta R.T.: 0.005 min
Response: 204659
Conc: 2.14 ug/ml