

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011722AL\
 Data File : FC057948.D
 Signal(s) : FID1A.CH
 Acq On : 17 Jan 2022 15:01
 Operator : AJ\MA
 Sample : N1097-13DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-3SDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/18/2022
 Supervised By :Ankita Jodhani 01/18/2022

Integration File: autoint1.e
 Quant Time: Jan 18 00:51:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 12:13:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.709	1067677	5.522 ug/mlm
Spiked Amount 50.000		Recovery =	11.04%
12) S 1-chlorooctadecane (S...	12.148	956172	6.487 ug/mlm
Spiked Amount 50.000		Recovery =	12.97%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011722AL\
Data File : FC057948.D
Signal(s) : FID1A.CH
Acq On : 17 Jan 2022 15:01
Operator : AJ\MA
Sample : N1097-13DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
TP-3SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/18/2022
Supervised By :Ankita Jodhani 01/18/2022

Integration File: autoint1.e
Quant Time: Jan 18 00:51:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 12:13:43 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

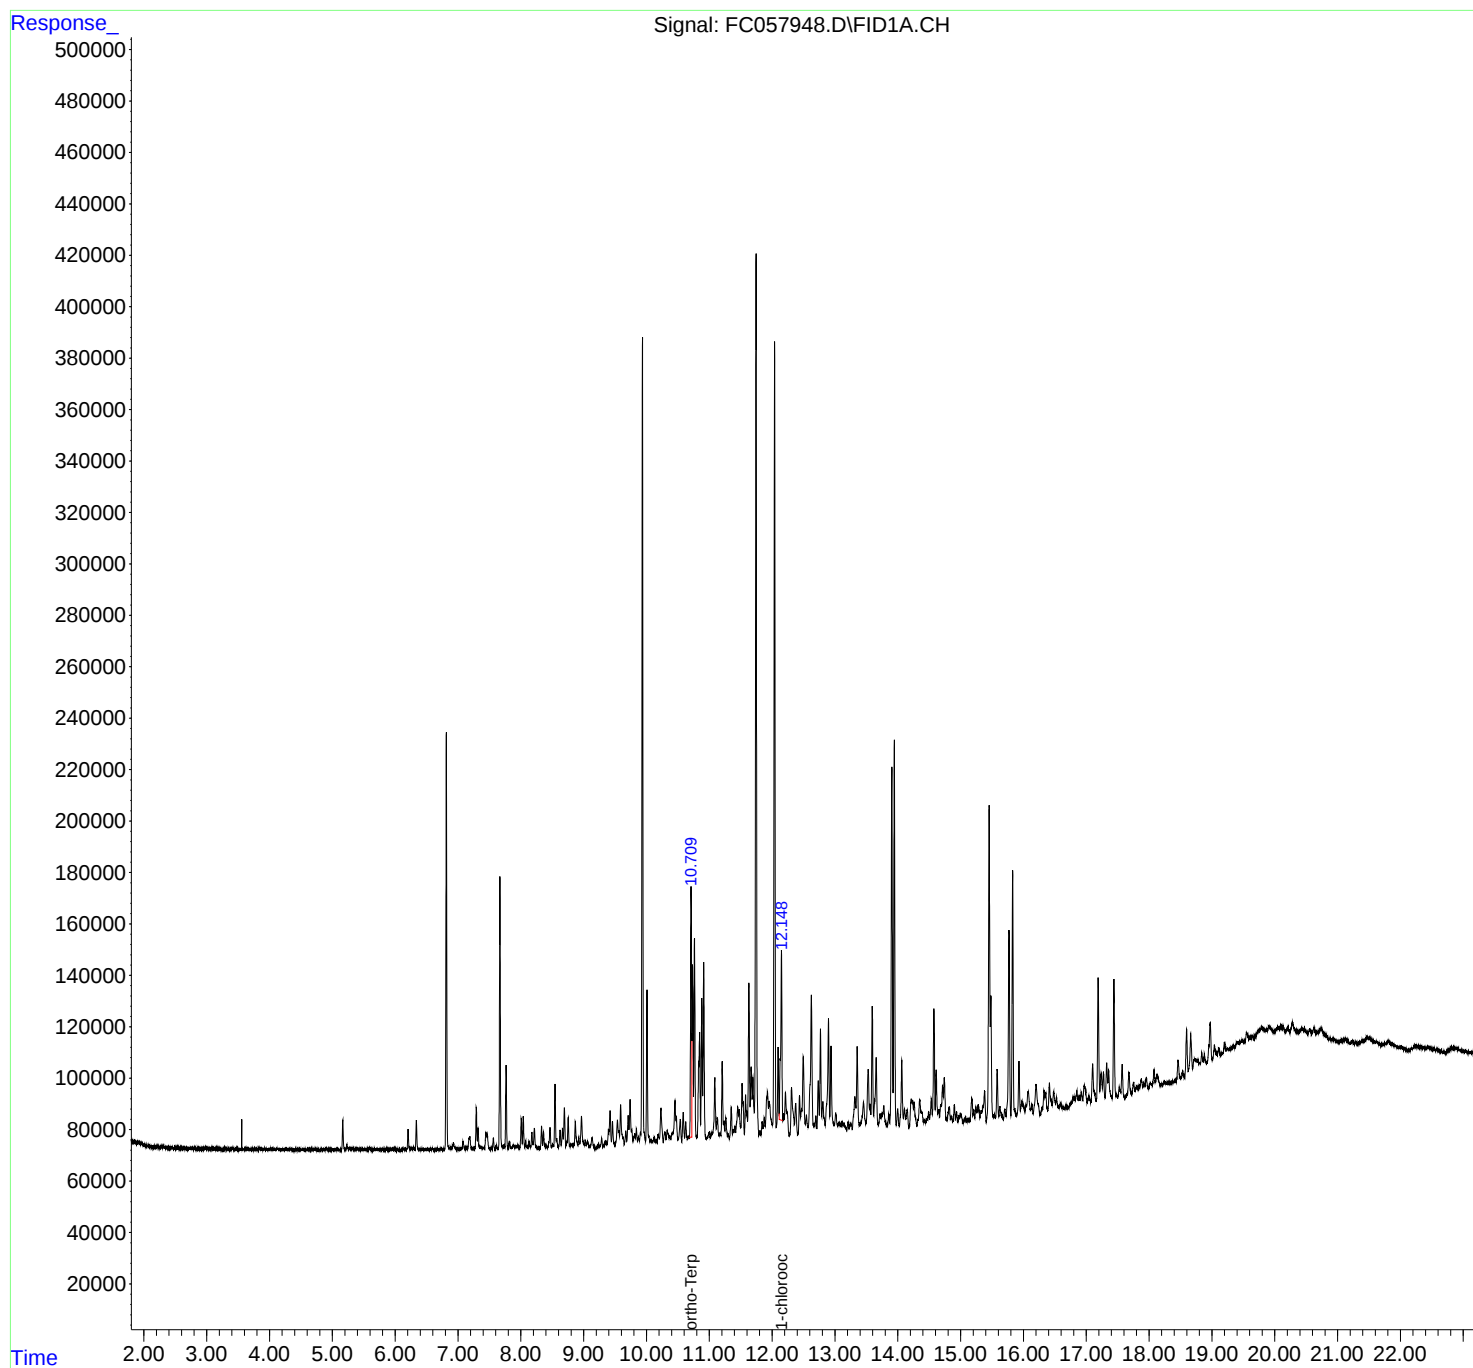

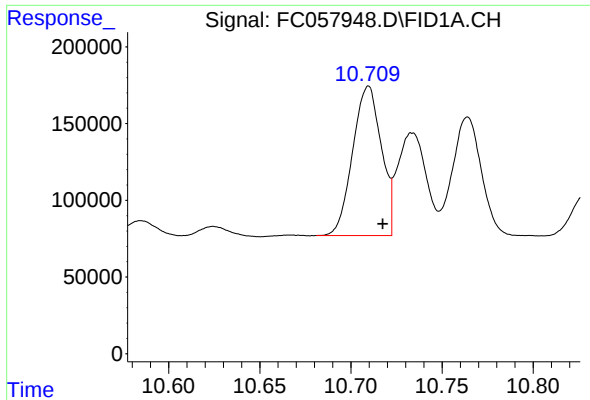


#9 ortho-Terphenyl (SURR)

R.T.: 10.709 min
Delta R.T.: -0.008 min
Response: 1067677
Conc: 5.52 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-3SDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/18/2022
Supervised By :Ankita Jodhani 01/18/2022

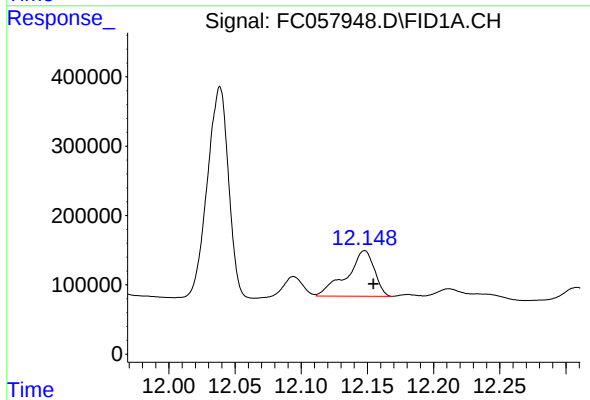

#12 1-chlorooctadecane (SURR)

R.T.: 12.148 min
Delta R.T.: -0.007 min
Response: 956172
Conc: 6.49 ug/ml m