

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011822AL\
 Data File : FC057996.D
 Signal(s) : FID1A.CH
 Acq On : 19 Jan 2022 8:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 08:40:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 12:13:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.137	163276	1.108 ug/ml
Spiked Amount 50.000		Recovery =	2.22%
Target Compounds			
15) T n-Hexacosane (C26)	15.019	14628	0.087 ug/ml
16) T n-Octacosane (C28)	15.971	6508	0.040 ug/ml
17) T n-Tricontane (C30)	16.856	82208	0.527 ug/ml
18) T n-Dotriacontane (C32)	17.688	152834	1.096 ug/ml
19) T n-Tetratriacontane (C34)	18.481	209249	1.684 ug/ml
22) T n-Tetracontane (C40)	20.758	1806677	18.868 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC011822AL\
Data File : FC057996.D
Signal(s) : FID1A.CH
Acq On : 19 Jan 2022 8:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 08:40:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 12:13:43 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

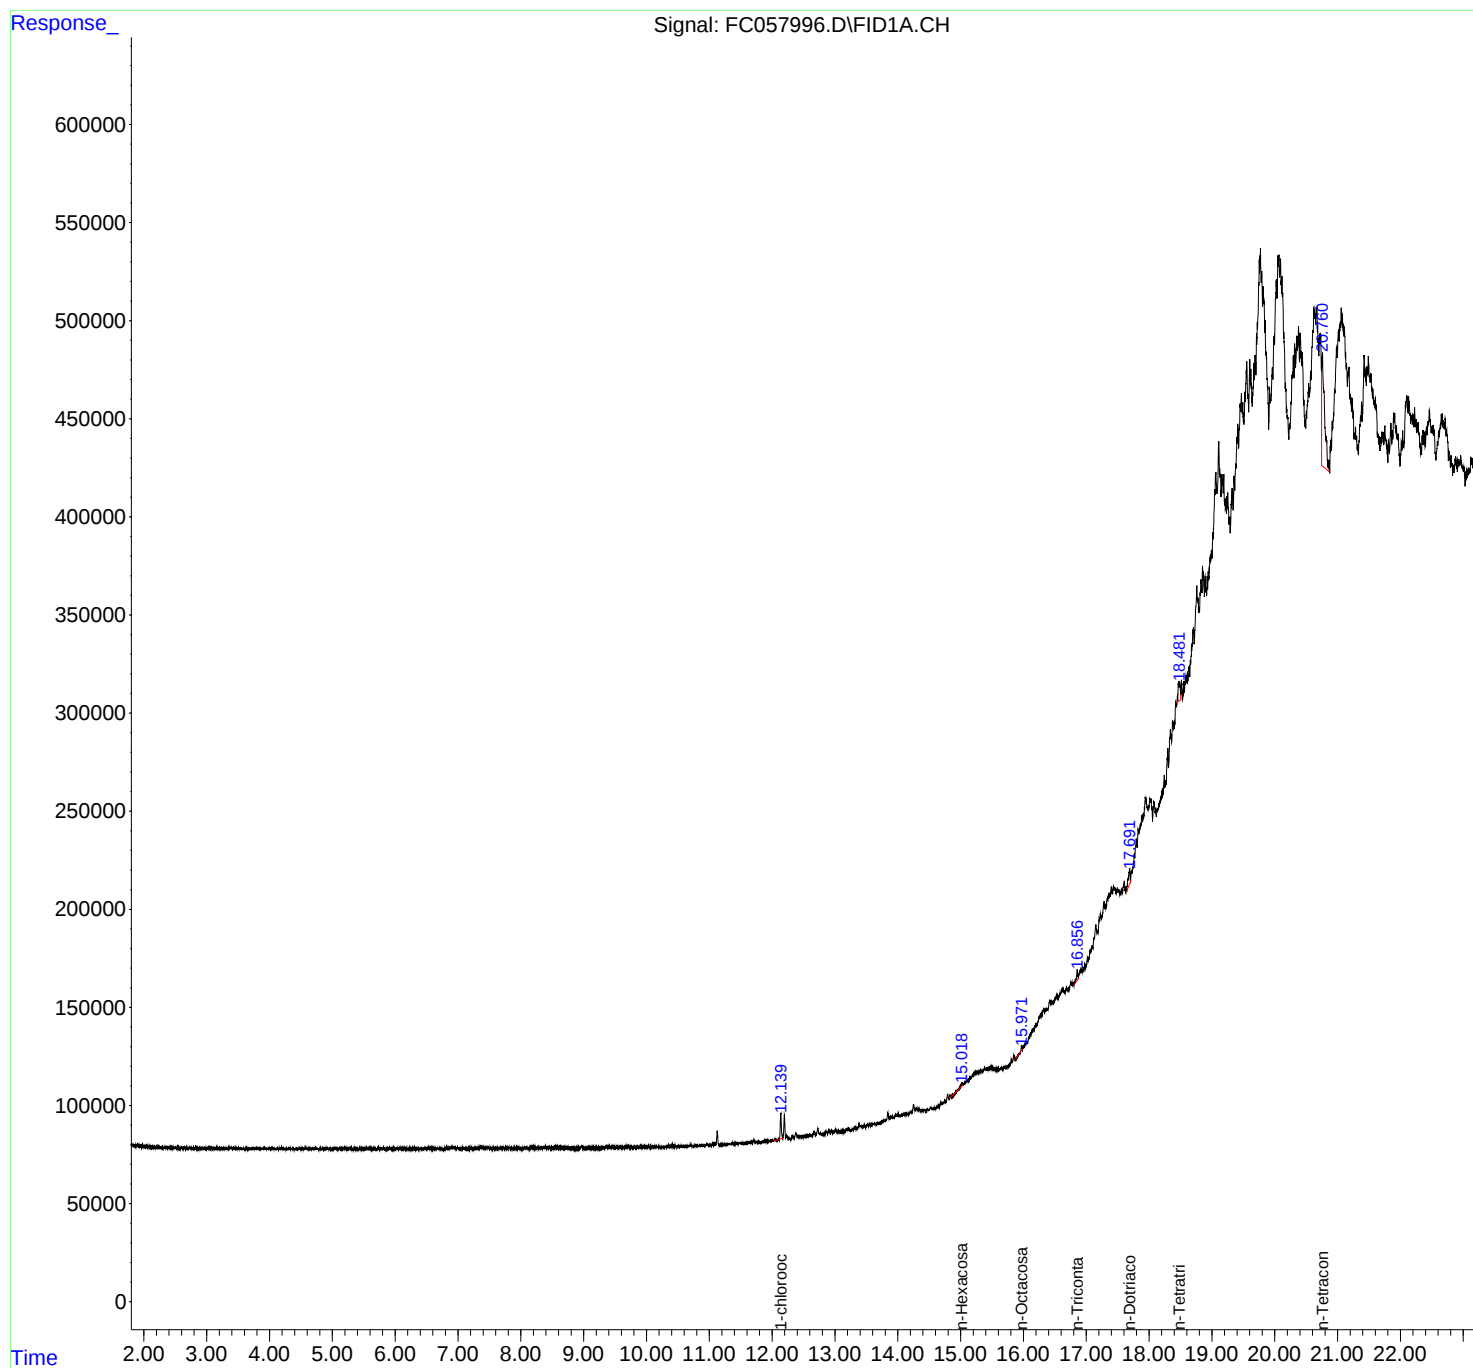


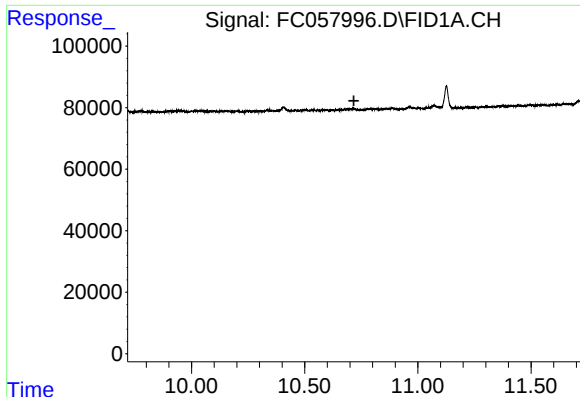

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.717 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

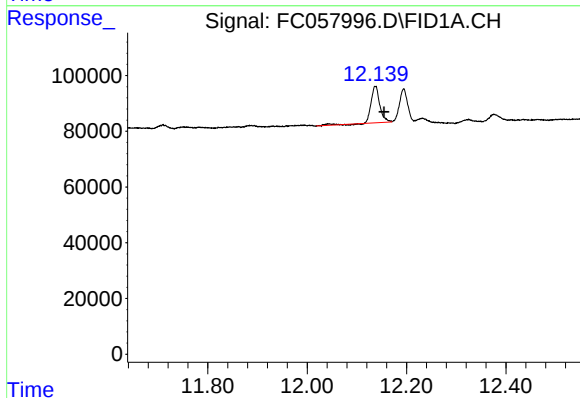


#12 1-chlorooctadecane (SURR)

R.T.: 12.137 min
Delta R.T.: -0.017 min
Response: 163276
Conc: 1.11 ug/ml

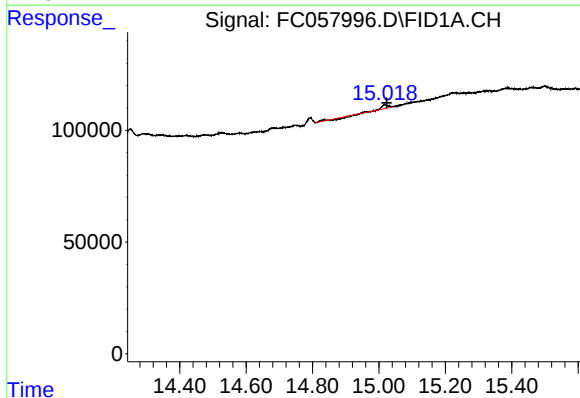


#15 n-Hexacosane (C26)

R.T.: 15.019 min
Delta R.T.: -0.004 min
Response: 14628
Conc: 0.09 ug/ml

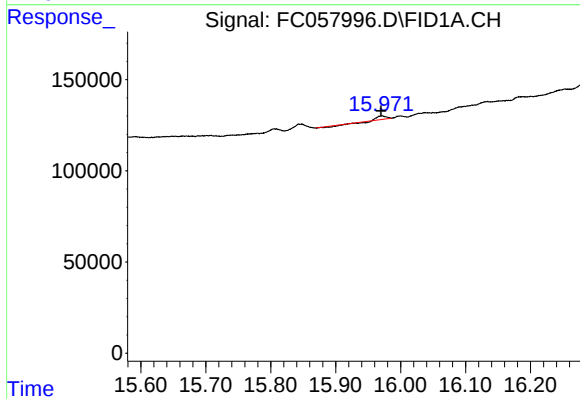

#16 n-Octacosane (C28)


R.T.: 15.971 min
Delta R.T.: 0.002 min
Response: 6508
Conc: 0.04 ug/ml

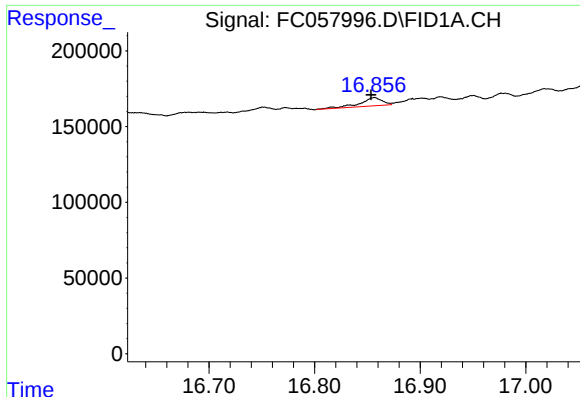

#17 n-Tricontane (C30)


R.T.: 16.856 min
Delta R.T.: 0.003 min
Response: 82208
Conc: 0.53 ug/ml

Instrument :
FID_C
ClientSampleId :

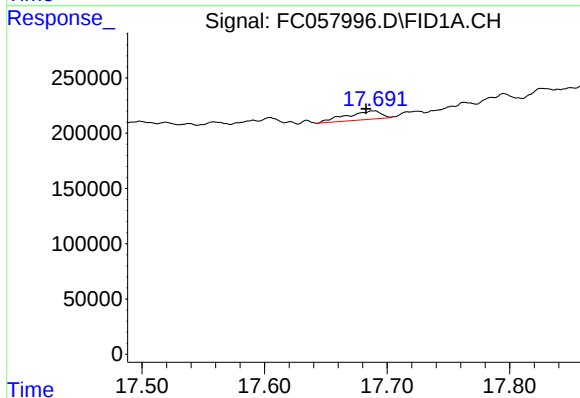


#18 n-Dotriacontane (C32)

R.T.: 17.688 min
Delta R.T.: 0.005 min
Response: 152834
Conc: 1.10 ug/ml

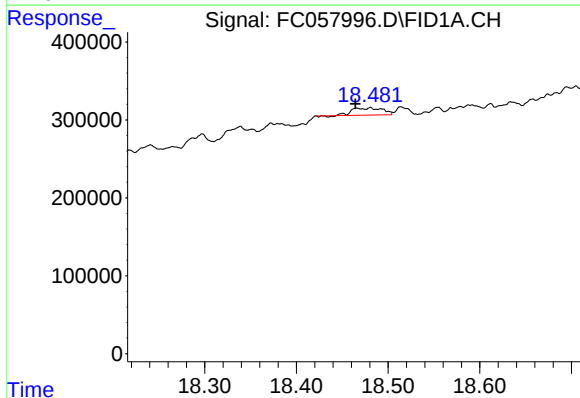

#19 n-Tetratriacontane (C34)

R.T.: 18.481 min
Delta R.T.: 0.016 min
Response: 209249
Conc: 1.68 ug/ml

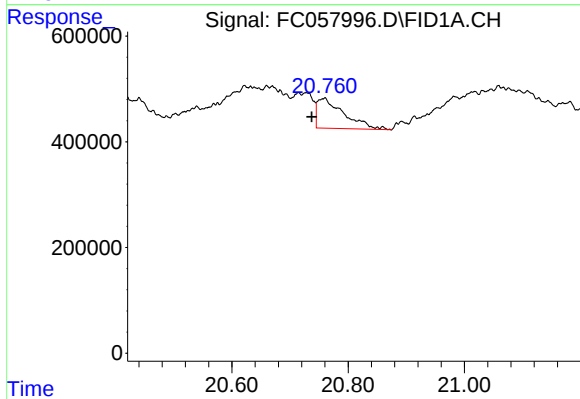

#22 n-Tetracontane (C40)

R.T.: 20.758 min
Delta R.T.: 0.021 min
Response: 1806677
Conc: 18.87 ug/ml