

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC012419AL\
 Data File : FC038771.D
 Signal(s) : FID1A.CH
 Acq On : 24 Jan 2019 21:43
 Operator : AJ\SJ
 Sample : K1016-03DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TR-05-RO-1-012319DL

Integration File: autoint1.e
 Quant Time: Jan 25 02:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 010919.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 05:47:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.247	694037	6.429 ug/ml
Spiked Amount 50.000		Recovery =	12.86%
12) S 1-chlorooctadecane (S...	12.686	10324120	130.776 ug/ml
Spiked Amount 50.000		Recovery =	261.55%
Target Compounds			
10) T n-Eicosane (C20)	12.289	403241	4.411 ug/ml
11) T n-Heneicosane (C21)	12.917	1298687	14.517 ug/ml
14) T n-Tetracosane (C24)	14.501	205629	2.329 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC012419AL\
Data File : FC038771.D
Signal(s) : FID1A.CH
Acq On : 24 Jan 2019 21:43
Operator : AJ\SJ
Sample : K1016-03DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleID :
TR-05-RO-1-012319DL

Integration File: autoint1.e
Quant Time: Jan 25 02:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 010919.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 05:47:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

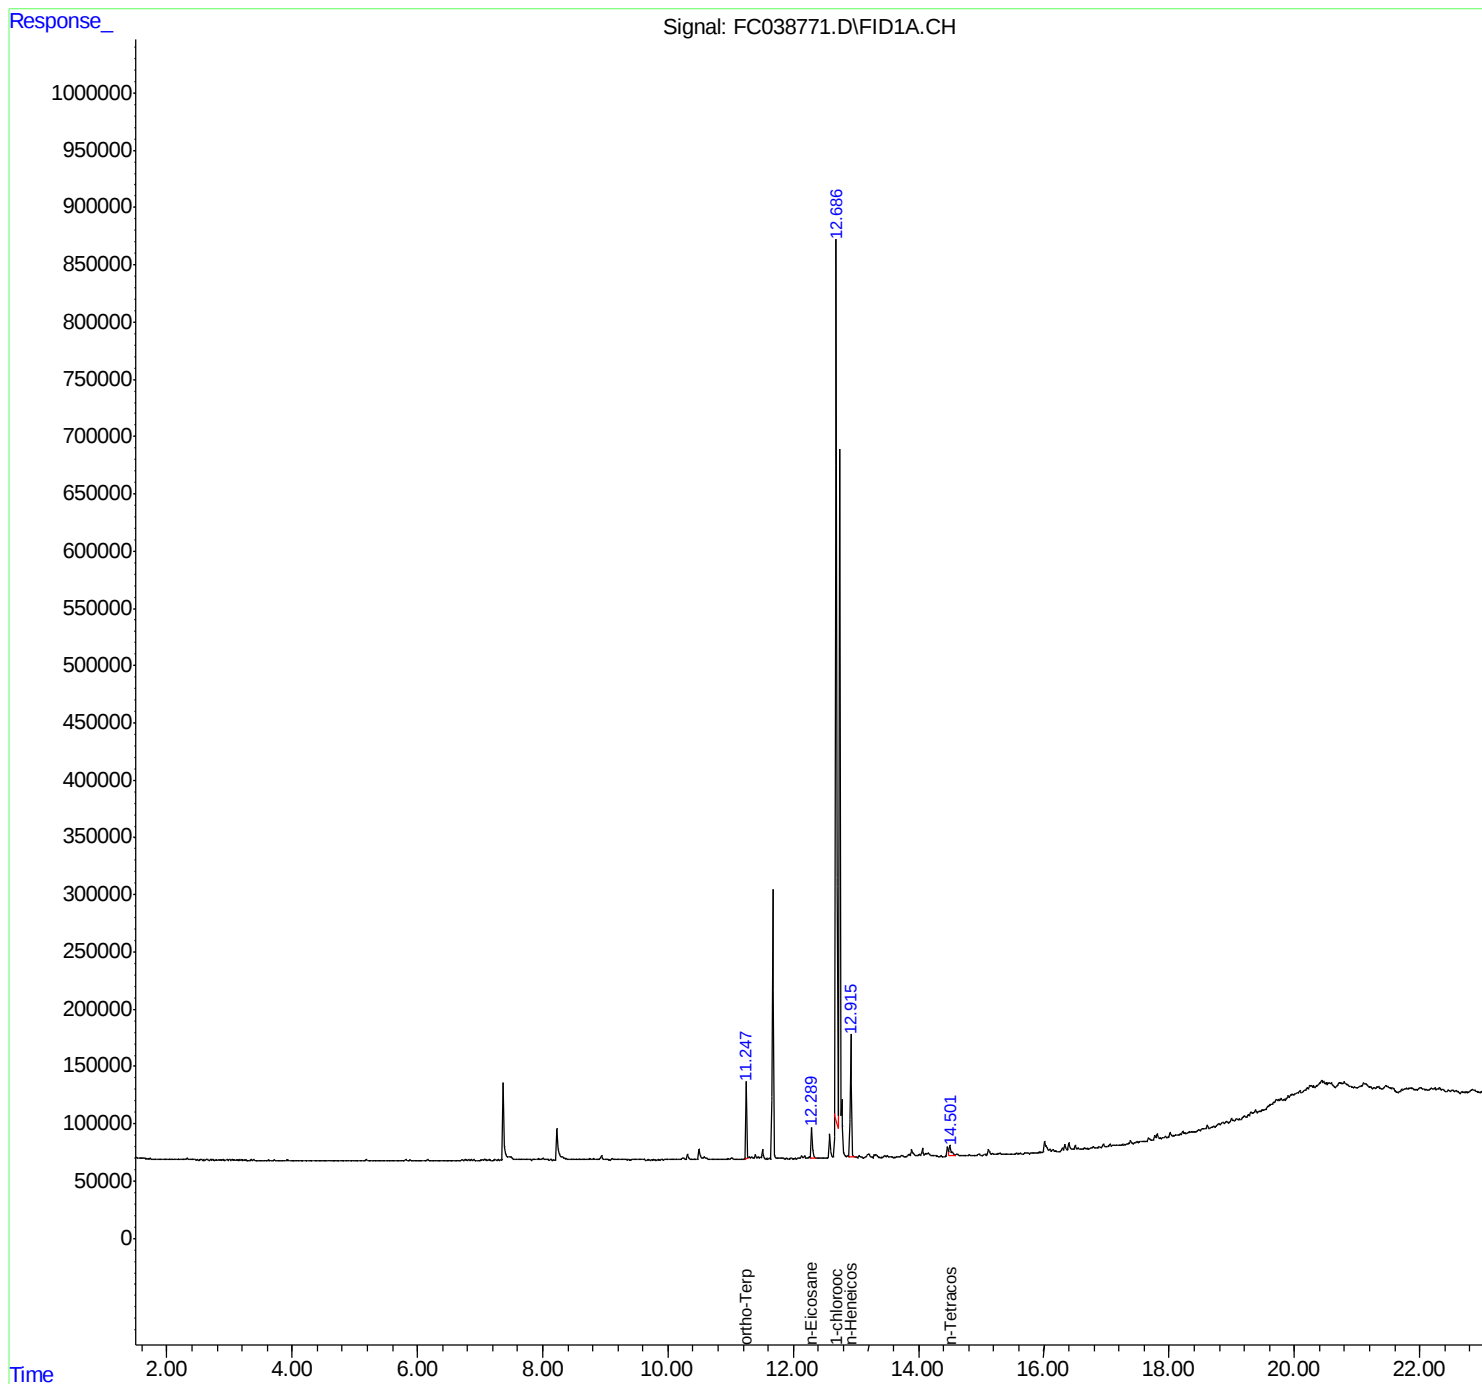


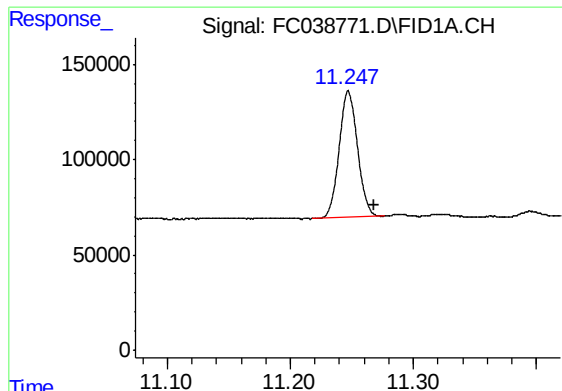

#9 ortho-Terphenyl (SURR)


R.T.: 11.247 min
Delta R.T.: -0.021 min
Response: 694037
Conc: 6.43 ug/ml

Instrument :
FID_C
ClientSampleId :
TR-05-RO-1-012319DL

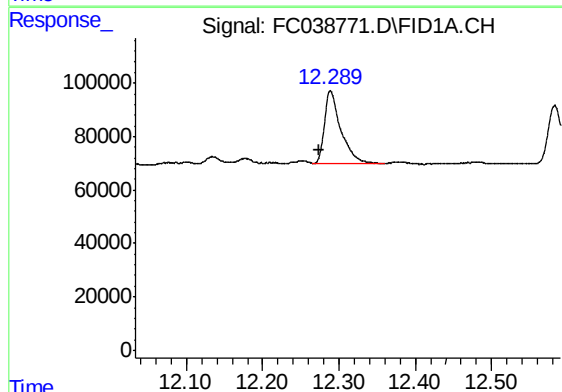


#10 n-Eicosane (C20)

R.T.: 12.289 min
Delta R.T.: 0.015 min
Response: 403241
Conc: 4.41 ug/ml

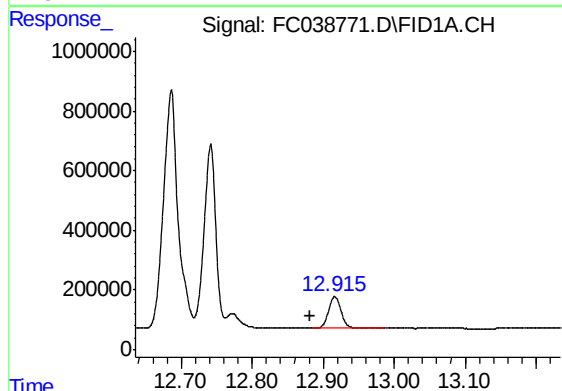


#11 n-Heneicosane (C21)

R.T.: 12.917 min
Delta R.T.: 0.035 min
Response: 1298687
Conc: 14.52 ug/ml

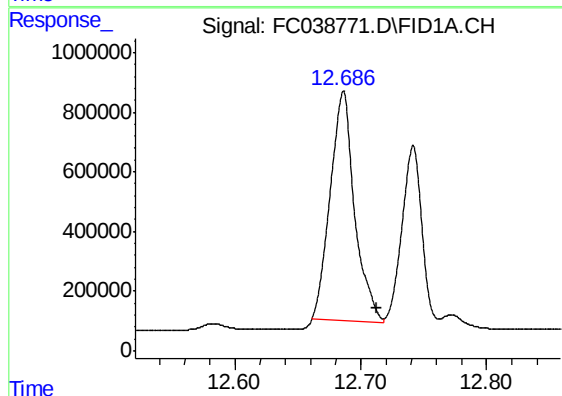

#12 1-chlorooctadecane (SURR)

R.T.: 12.686 min
Delta R.T.: -0.027 min
Response: 10324120
Conc: 130.78 ug/ml

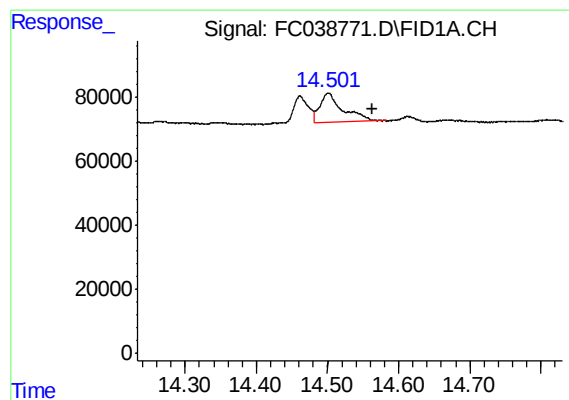

#14 n-Tetracosane (C24)

R.T.: 14.501 min
Delta R.T.: -0.063 min
Response: 205629
Conc: 2.33 ug/ml

Instrument :
FID_C
ClientSampleId :
TR-05-RO-1-012319DL