

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC012622AL\
 Data File : FC058135.D
 Signal(s) : FID1A.CH
 Acq On : 26 Jan 2022 20:45
 Operator : AJ\MA
 Sample : N1267-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 2ND-3RD-FLOOR-WALLS-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/27/2022
 Supervised By :mohammad ahmed 01/27/2022

Integration File: autoint1.e
 Quant Time: Jan 27 02:35:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 12:13:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.696	6865031	35.503 ug/ml
Spiked Amount 50.000		Recovery =	71.01%
12) S 1-chlorooctadecane (S...	12.133	5433514	36.866 ug/mlm
Spiked Amount 50.000		Recovery =	73.73%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC012622AL\
Data File : FC058135.D
Signal(s) : FID1A.CH
Acq On : 26 Jan 2022 20:45
Operator : AJ\MA
Sample : N1267-19
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
2ND-3RD-FLOOR-WALLS-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/27/2022
Supervised By :mohammad ahmed 01/27/2022

Integration File: autoint1.e
Quant Time: Jan 27 02:35:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 010522.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 12:13:43 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

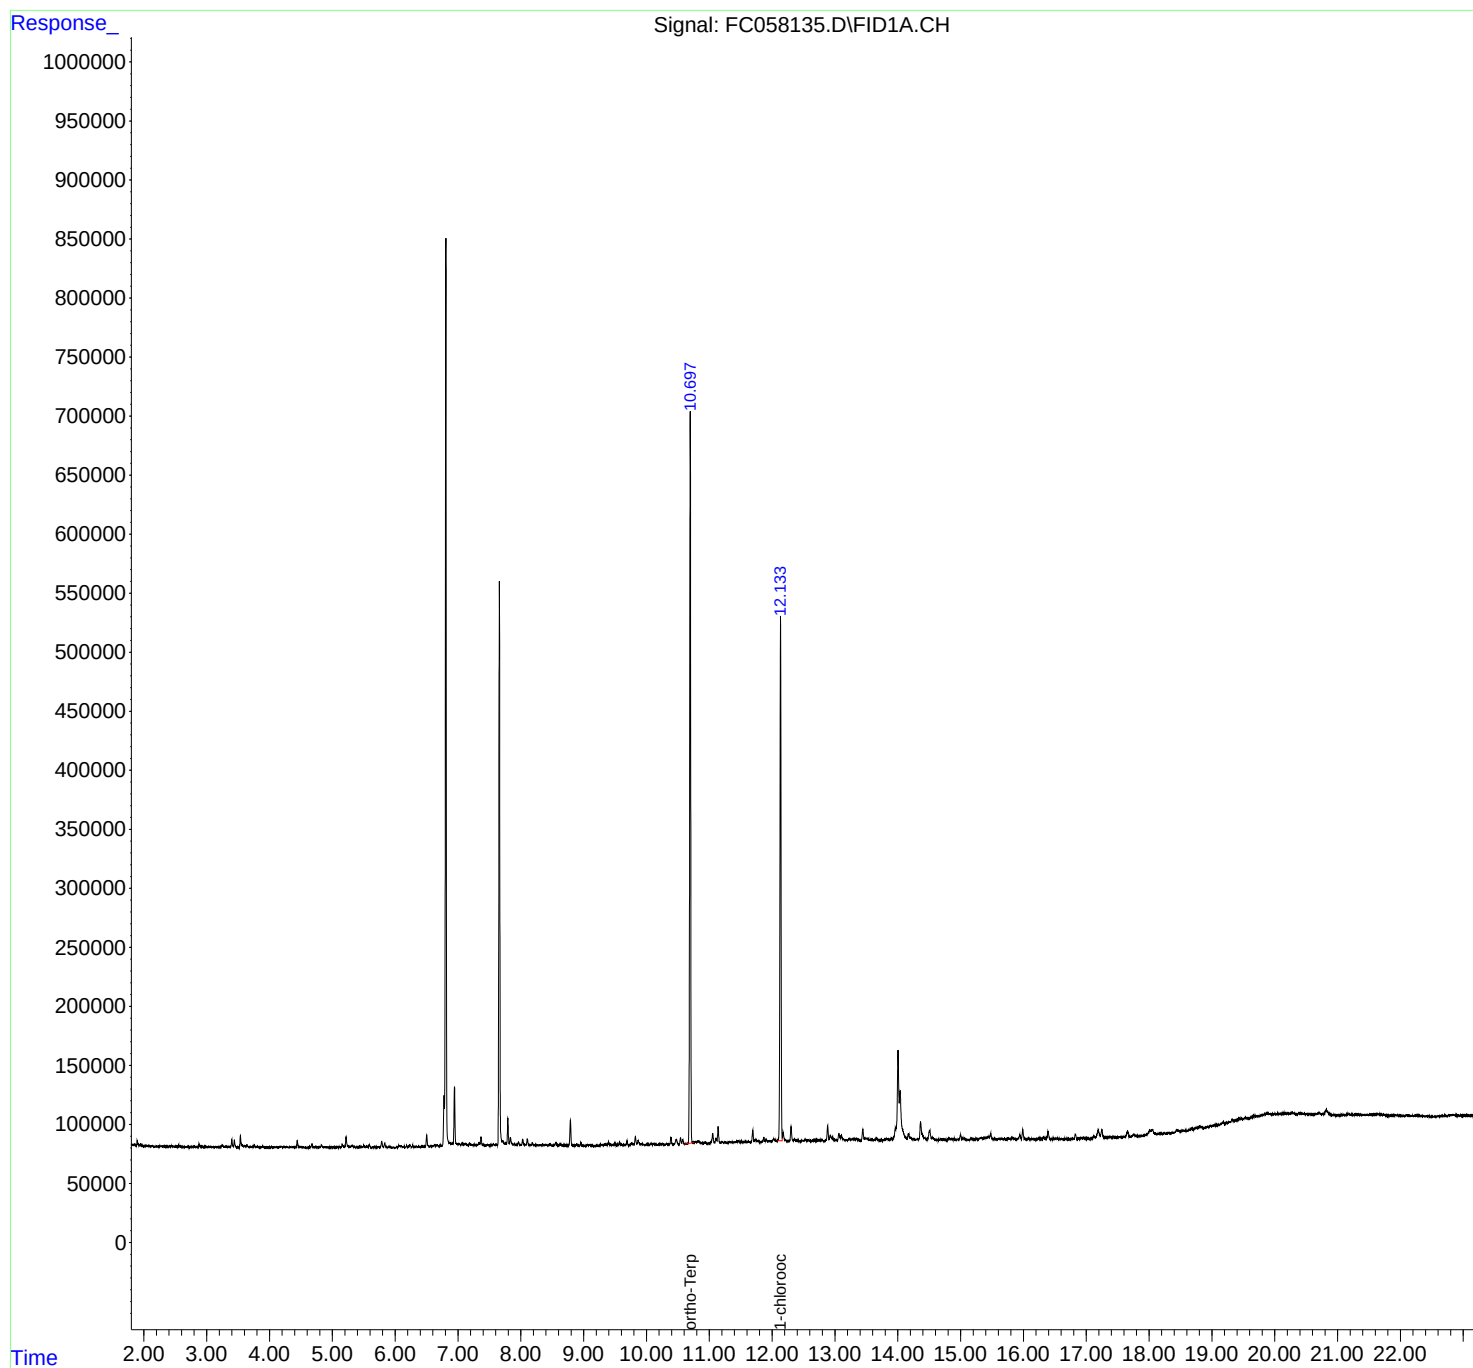

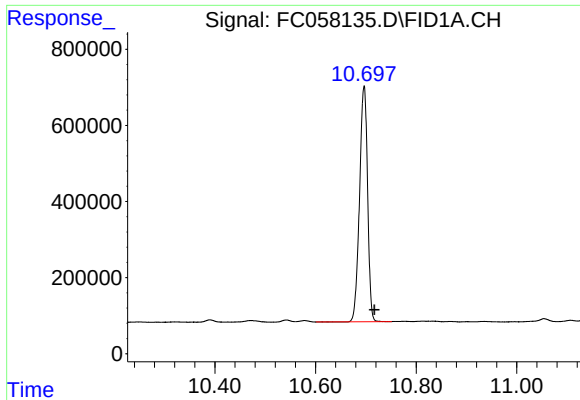

#9 ortho-Terphenyl (SURR)

R.T.: 10.696 min
Delta R.T.: -0.021 min
Response: 6865031
Conc: 35.50 ug/ml

Instrument :

FID_C

ClientSampleId :


2ND-3RD-FLOOR-WALLS-1

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 01/27/2022

Supervised By :mohammad ahmed 01/27/2022

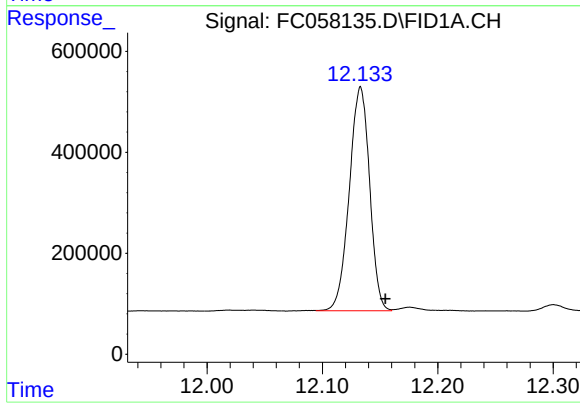

#12 1-chlorooctadecane (SURR)

R.T.: 12.133 min
Delta R.T.: -0.022 min
Response: 5433514
Conc: 36.87 ug/ml m