

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC013120AL\
 Data File : FC045604.D
 Signal(s) : FID1A.CH
 Acq On : 01 Feb 2020 2:45
 Operator : DD\AJ
 Sample : L1274-02D
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 01 06:04:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 012120.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 22 04:15:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.186	2701953	31.077 ug/ml
Spiked Amount 50.000		Recovery =	62.15%
Target Compounds			
16) T n-Octacosane (C28)	16.998	179592	1.757 ug/ml
17) T n-Tricontane (C30)	17.882	302665	3.083 ug/ml
18) T n-Dotriacontane (C32)	18.713	253681	3.049 ug/ml
19) T n-Tetratriacontane (C34)	19.495	201351	2.845 ug/ml
20) T n-Hexatriacontane (C36)	20.233	679341	10.595 ug/ml
21) T n-Octatriacontane (C38)	21.007	193763	3.313 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC013120AL\
Data File : FC045604.D
Signal(s) : FID1A.CH
Acq On : 01 Feb 2020 2:45
Operator : DD\AJ
Sample : L1274-02D
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 01 06:04:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 012120.M
Quant Title : GC Extractables
QLast Update : Wed Jan 22 04:15:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

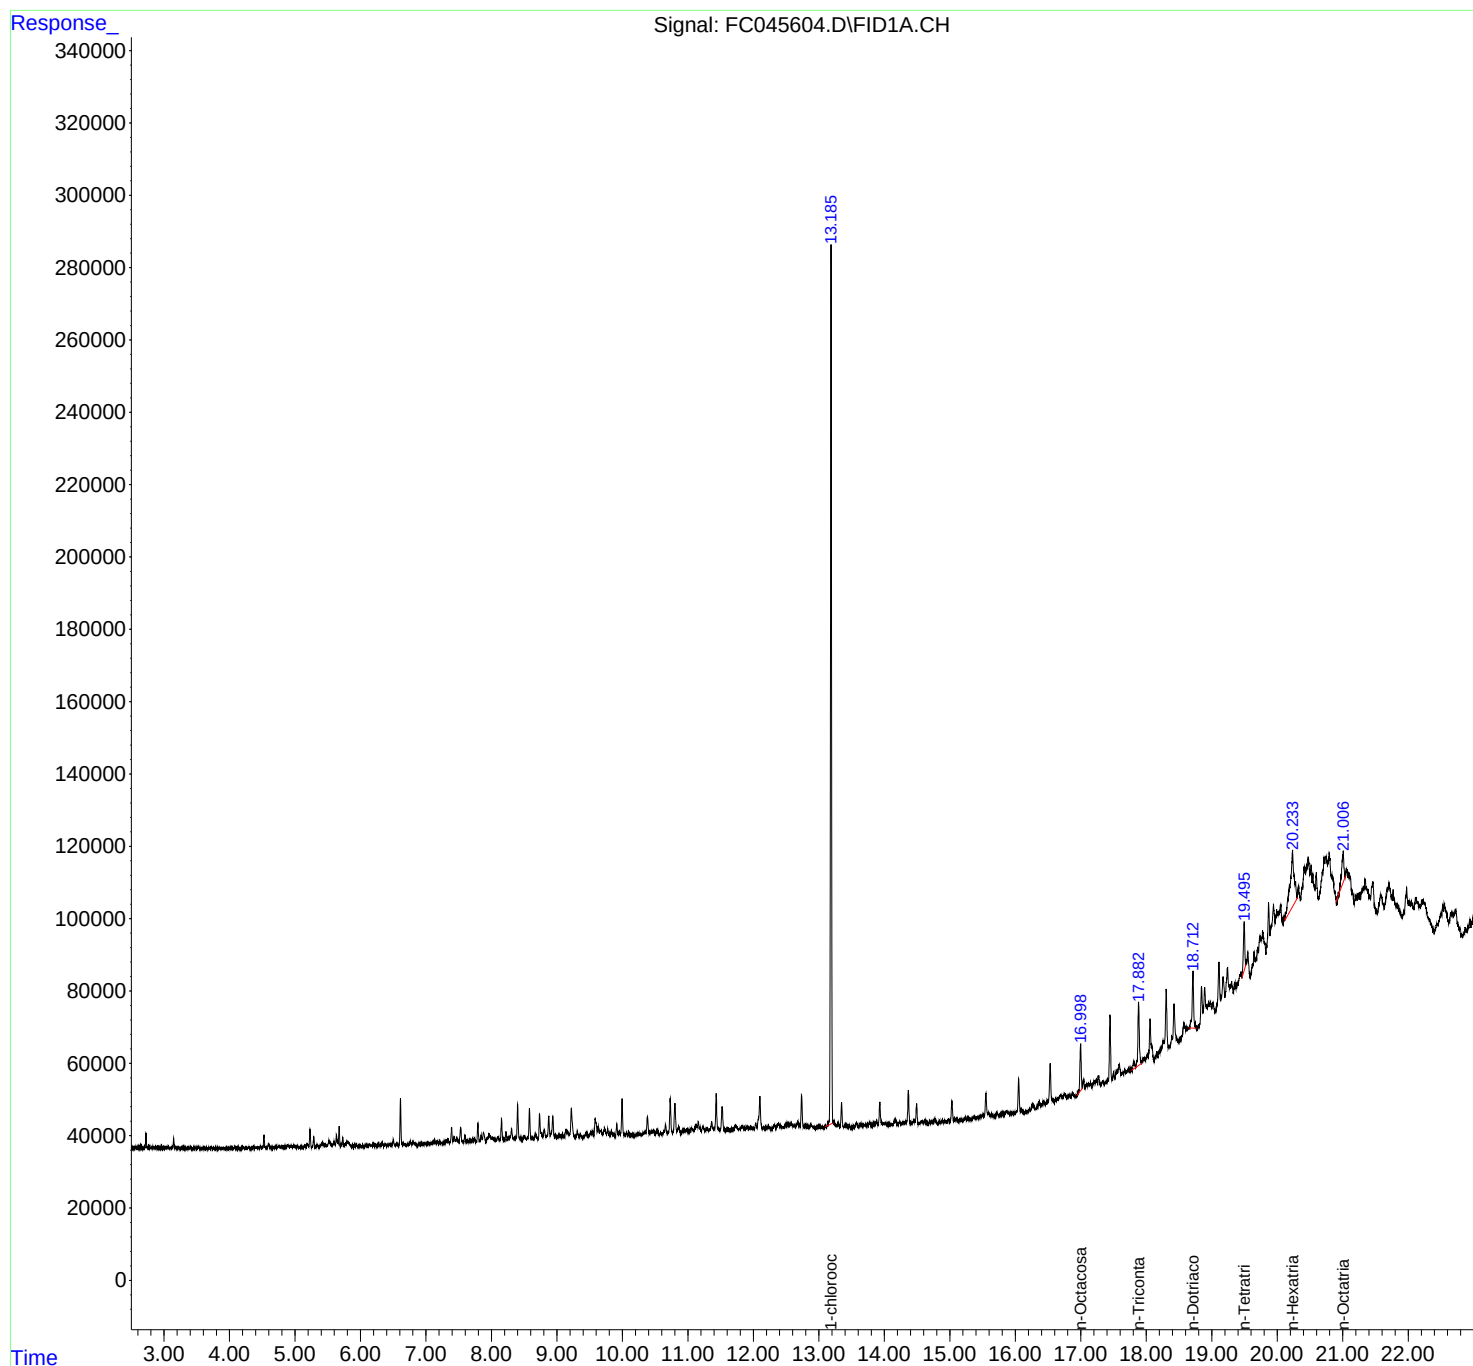


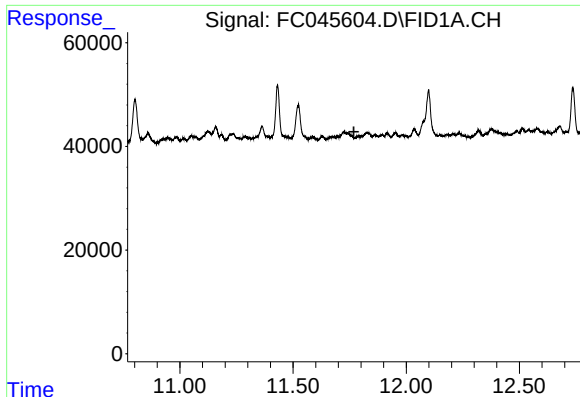

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.769 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

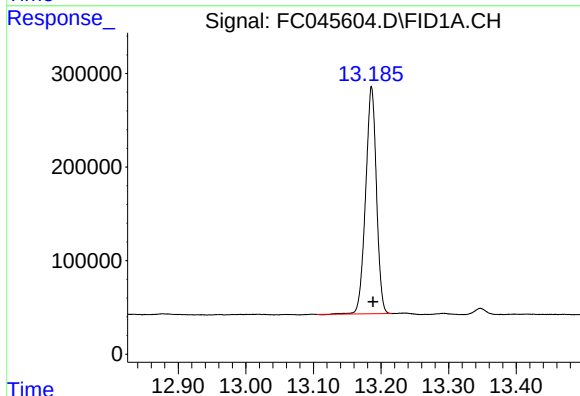


#12 1-chlorooctadecane (SURR)

R.T.: 13.186 min
Delta R.T.: -0.002 min
Response: 2701953
Conc: 31.08 ug/ml

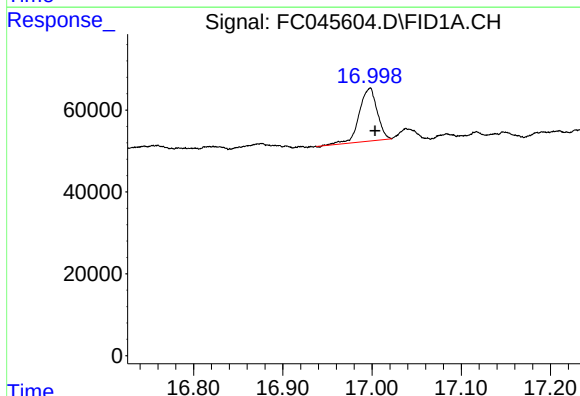


#16 n-Octacosane (C28)

R.T.: 16.998 min
Delta R.T.: -0.006 min
Response: 179592
Conc: 1.76 ug/ml

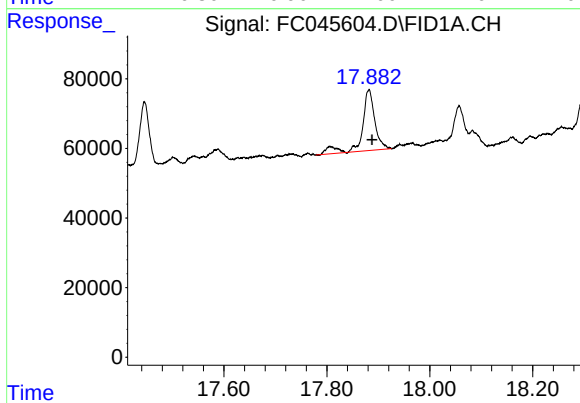

#17 n-Tricontane (C30)


R.T.: 17.882 min
Delta R.T.: -0.006 min
Response: 302665
Conc: 3.08 ug/ml

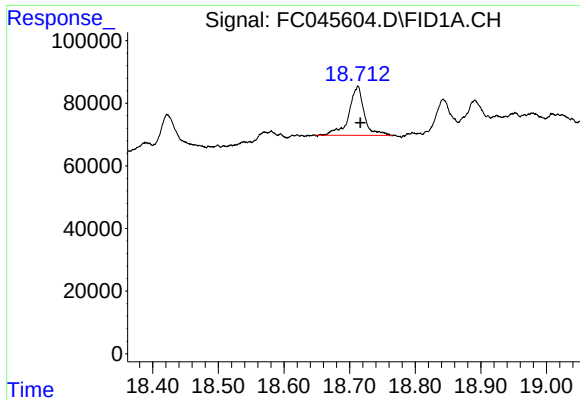

#18 n-Dotriacontane (C32)


R.T.: 18.713 min
Delta R.T.: -0.004 min
Response: 253681
Conc: 3.05 ug/ml

Instrument :
FID_C
ClientSampleId :

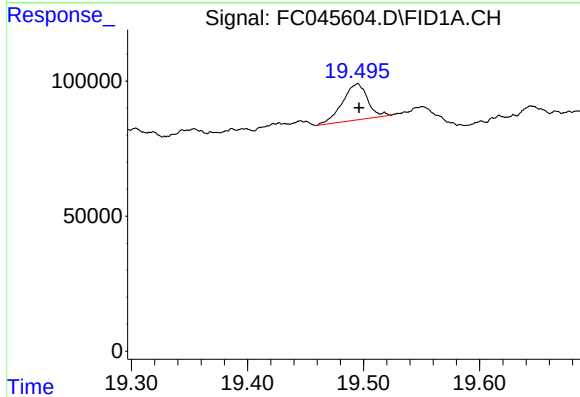


#19 n-Tetratriacontane (C34)

R.T.: 19.495 min
Delta R.T.: -0.001 min
Response: 201351
Conc: 2.85 ug/ml

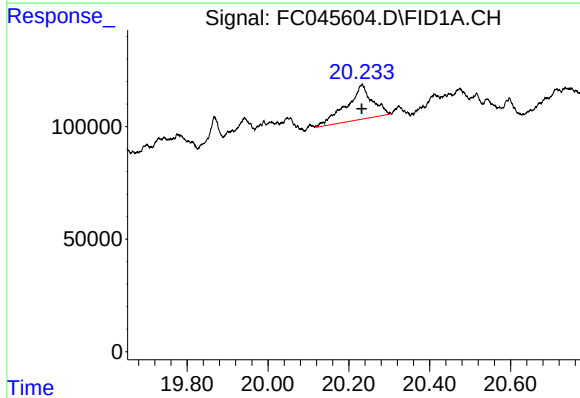

#20 n-Hexatriacontane (C36)

R.T.: 20.233 min
Delta R.T.: 0.000 min
Response: 679341
Conc: 10.59 ug/ml

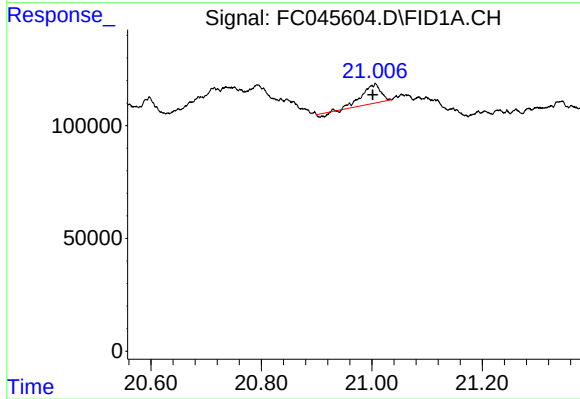

#21 n-Octatriacontane (C38)

R.T.: 21.007 min
Delta R.T.: 0.005 min
Response: 193763
Conc: 3.31 ug/ml