

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC020420AL\
 Data File : FC045676.D
 Signal(s) : FID1A.CH
 Acq On : 05 Feb 2020 2:16
 Operator : DD\AJ
 Sample : L1383-01DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 05 08:12:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 012120.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 22 04:15:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.766	673380	6.126 ug/ml
Spiked Amount 50.000		Recovery =	12.25%
12) S 1-chlorooctadecane (S...	13.187	511861	5.887 ug/ml
Spiked Amount 50.000		Recovery =	11.77%
Target Compounds			
14) T n-Tetracosane (C24)	15.049	237618	2.287 ug/ml
16) T n-Octacosane (C28)	16.949f	238208	2.331 ug/ml
20) T n-Hexatriacontane (C36)	20.186	327518	5.108 ug/ml
21) T n-Octatriacontane (C38)	21.015	239928	4.102 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC020420AL\
Data File : FC045676.D
Signal(s) : FID1A.CH
Acq On : 05 Feb 2020 2:16
Operator : DD\AJ
Sample : L1383-01DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :

Integration File: autoint1.e
Quant Time: Feb 05 08:12:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 012120.M
Quant Title : GC Extractables
QLast Update : Wed Jan 22 04:15:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

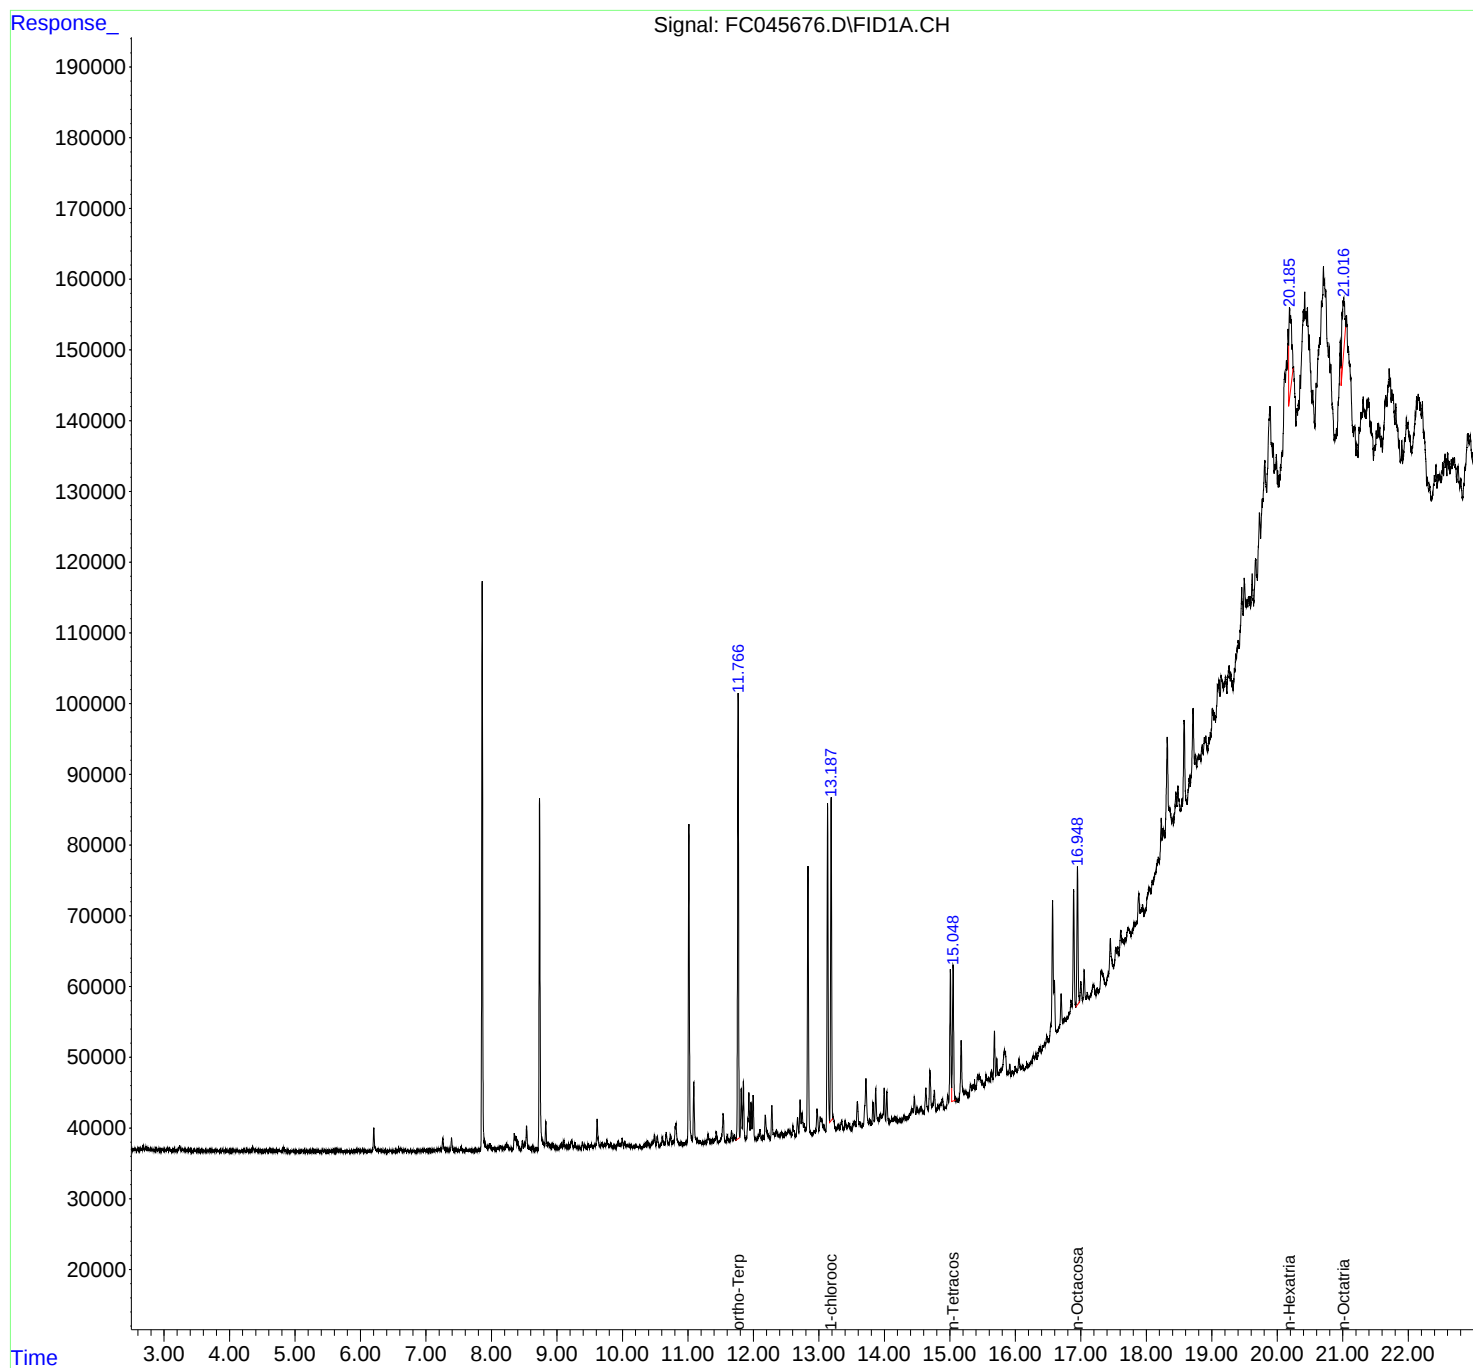


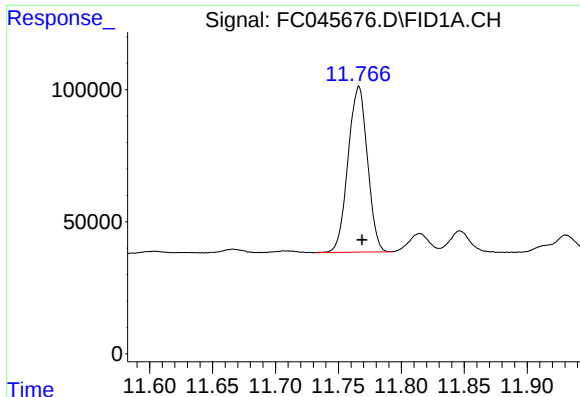

#9 ortho-Terphenyl (SURR)


R.T.: 11.766 min
Delta R.T.: -0.003 min
Response: 673380
Conc: 6.13 ug/ml

Instrument :
FID_C
ClientSampleId :

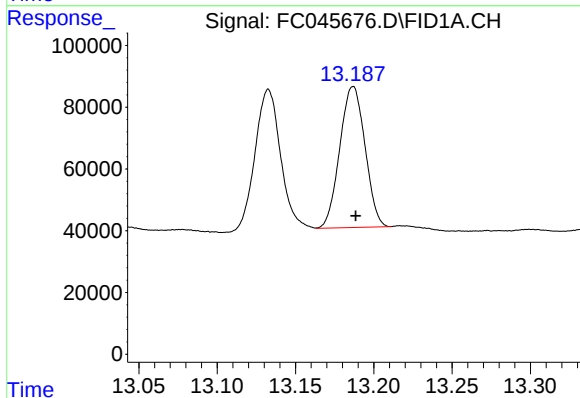


#12 1-chlorooctadecane (SURR)

R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 511861
Conc: 5.89 ug/ml

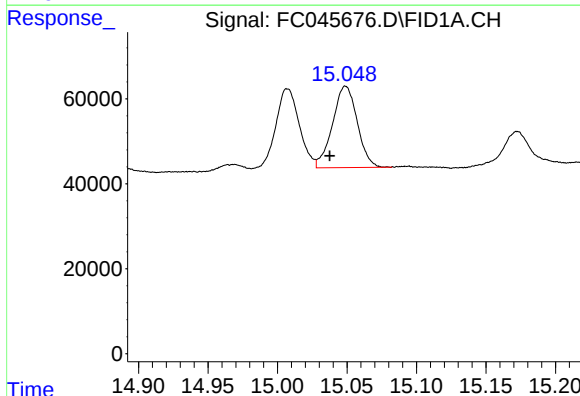


#14 n-Tetracosane (C24)

R.T.: 15.049 min
Delta R.T.: 0.011 min
Response: 237618
Conc: 2.29 ug/ml

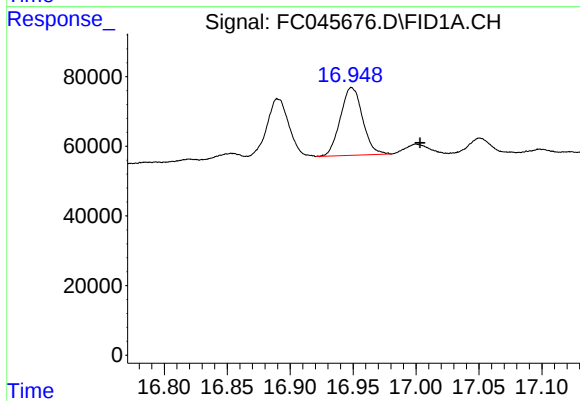

#16 n-Octacosane (C28)


R.T.: 16.949 min
Delta R.T.: -0.054 min
Response: 238208
Conc: 2.33 ug/ml

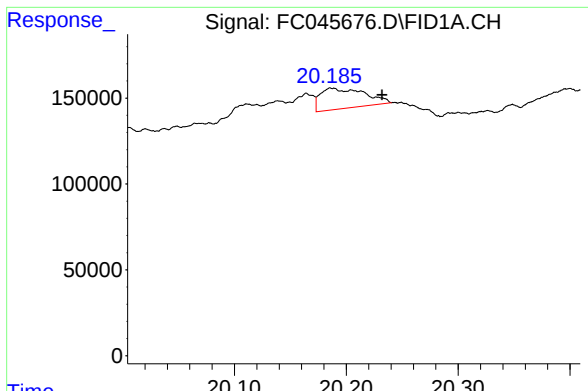

#20 n-Hexatriacontane (C36)

R.T.: 20.186 min
Delta R.T.: -0.046 min
Response: 327518
Conc: 5.11 ug/ml

Instrument :
FID_C
ClientSampleId :

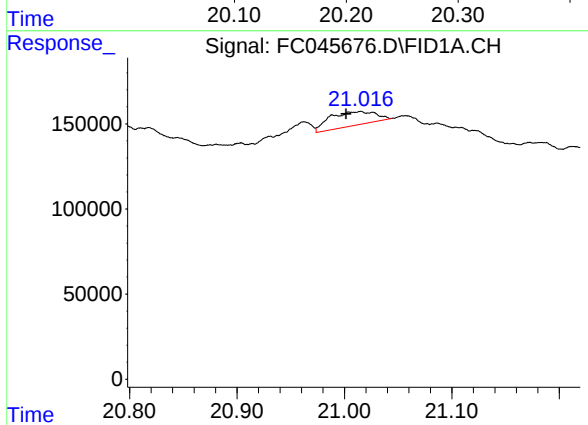

#21 n-Octatriacontane (C38)

R.T.: 21.015 min
Delta R.T.: 0.014 min
Response: 239928
Conc: 4.10 ug/ml