

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021419AL\
 Data File : FC039195.D
 Signal(s) : FID1A.CH
 Acq On : 15 Feb 2019 9:06
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Feb 15 10:09:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	17.351	46450	0.400 ug/ml
18) T	n-Dotriacontane (C32)	18.180	144136	1.325 ug/ml
19) T	n-Tetratriacontane (C34)	18.958	99530	1.075 ug/ml
20) T	n-Hexatriacontane (C36)	19.696	969771	12.209 ug/ml
21) T	n-Octatriacontane (C38)	20.392	1991549	27.117 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021419AL\
Data File : FC039195.D
Signal(s) : FID1A.CH
Acq On : 15 Feb 2019 9:06
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Feb 15 10:09:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

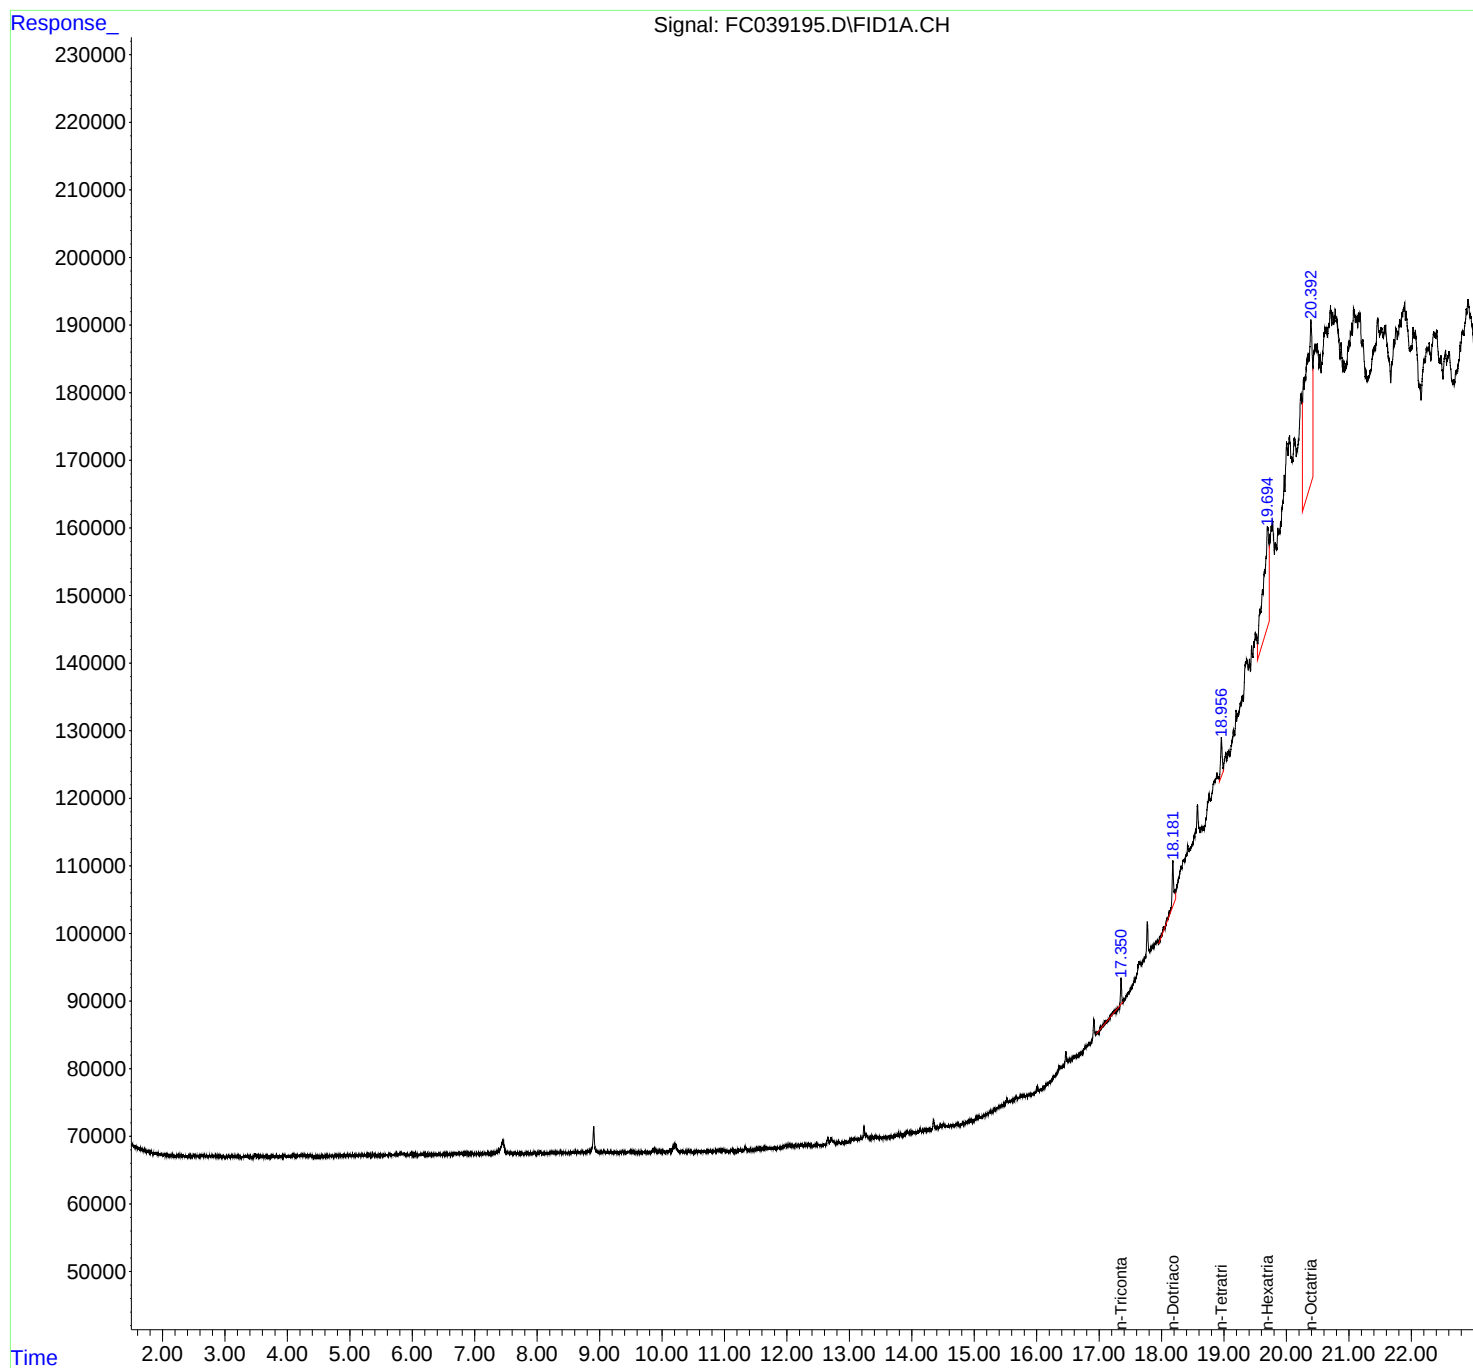


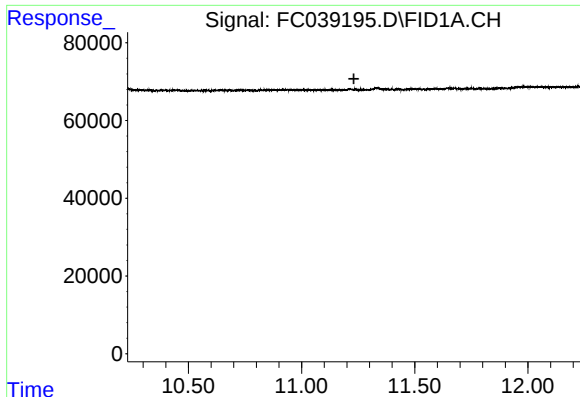

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

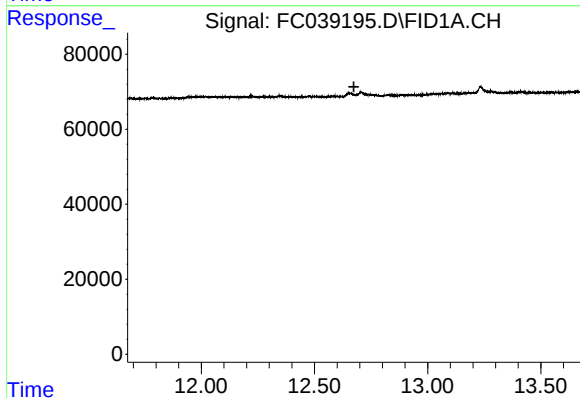


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.674 min
Response: 0
Conc: N.D.

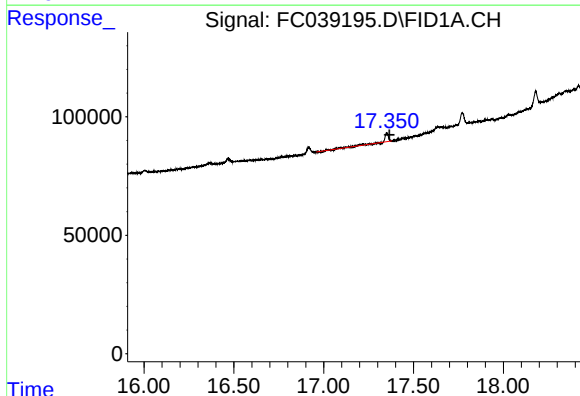


#17 n-Tricontane (C30)

R.T.: 17.351 min
Delta R.T.: -0.015 min
Response: 46450
Conc: 0.40 ug/ml

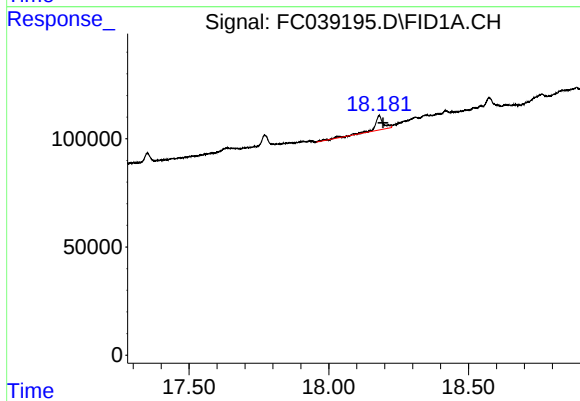

#18 n-Dotriacontane (C32)


R.T.: 18.180 min
Delta R.T.: -0.014 min
Response: 144136
Conc: 1.33 ug/ml

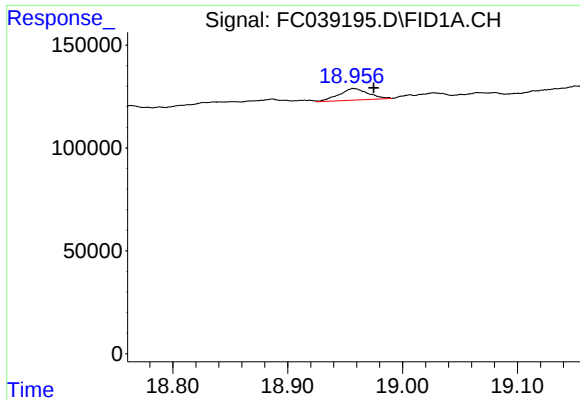

#19 n-Tetratriacontane (C34)


R.T.: 18.958 min
Delta R.T.: -0.017 min
Response: 99530
Conc: 1.07 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK

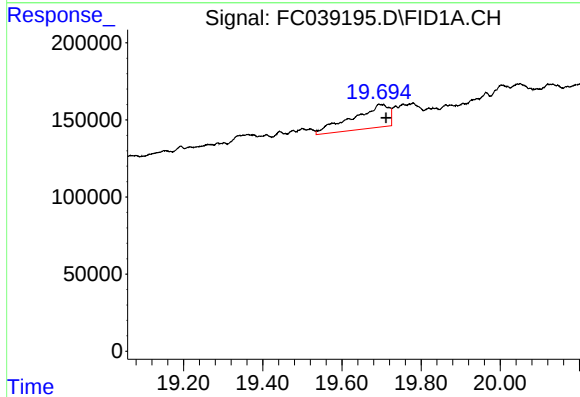

#20 n-Hexatriacontane (C36)

R.T.: 19.696 min
Delta R.T.: -0.016 min
Response: 969771
Conc: 12.21 ug/ml

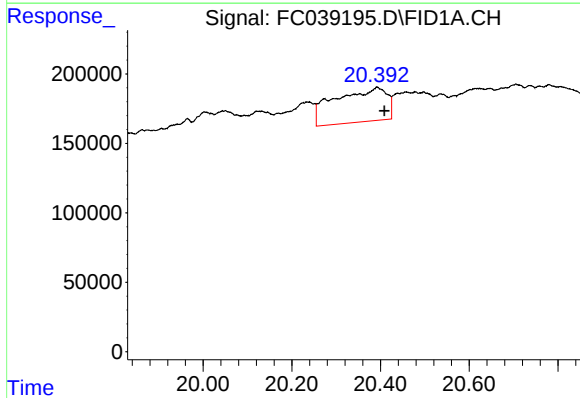

#21 n-Octatriacontane (C38)

R.T.: 20.392 min
Delta R.T.: -0.017 min
Response: 1991549
Conc: 27.12 ug/ml