

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021519AL\
 Data File : FC039214.D
 Signal(s) : FID1A.CH
 Acq On : 15 Feb 2019 20:48
 Operator : AJ\SJ
 Sample : K1346-07DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 CL-01-021419-ADL

Integration File: autoint1.e
 Quant Time: Feb 16 02:52:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.208	486960	3.115 ug/ml
Spiked Amount 50.000		Recovery =	6.23%
12) S 1-chlorooctadecane (S...	12.654	330296	2.801 ug/ml
Spiked Amount 50.000		Recovery =	5.60%
Target Compounds			
17) T n-Tricontane (C30)	17.347	100165	0.863 ug/ml
18) T n-Dotriacontane (C32)	18.174	2313	0.021 ug/ml
20) T n-Hexatriacontane (C36)	19.753	169889	2.139 ug/ml
21) T n-Octatriacontane (C38)	20.389	133704	1.821 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021519AL\
Data File : FC039214.D
Signal(s) : FID1A.CH
Acq On : 15 Feb 2019 20:48
Operator : AJ\SJ
Sample : K1346-07DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :
CL-01-021419-ADL

Integration File: autoint1.e
Quant Time: Feb 16 02:52:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

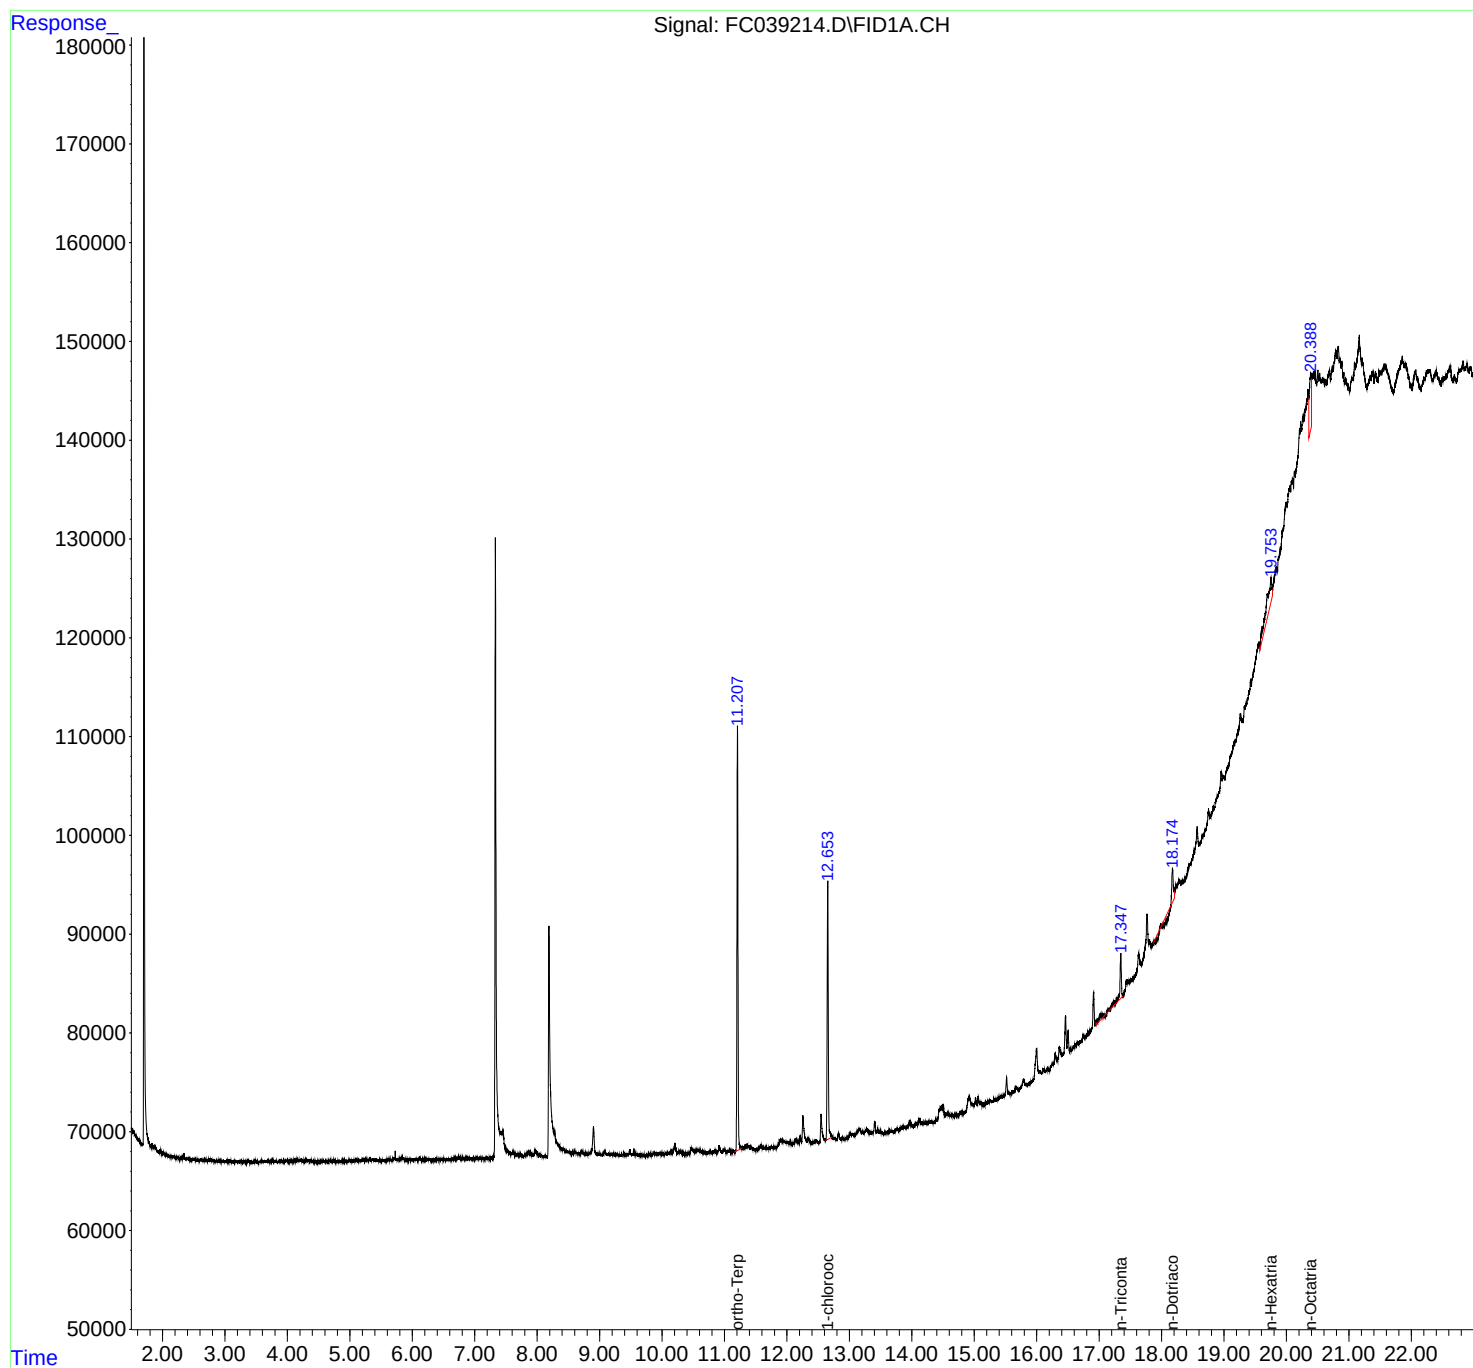


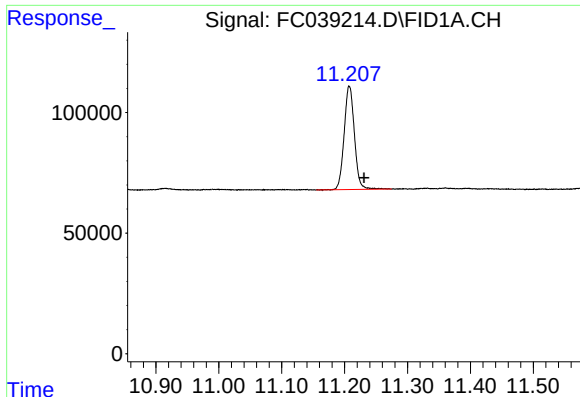

#9 ortho-Terphenyl (SURR)


R.T.: 11.208 min
Delta R.T.: -0.023 min
Response: 486960
Conc: 3.11 ug/ml

Instrument :
FID_C
ClientSampleId :
CL-01-021419-ADL

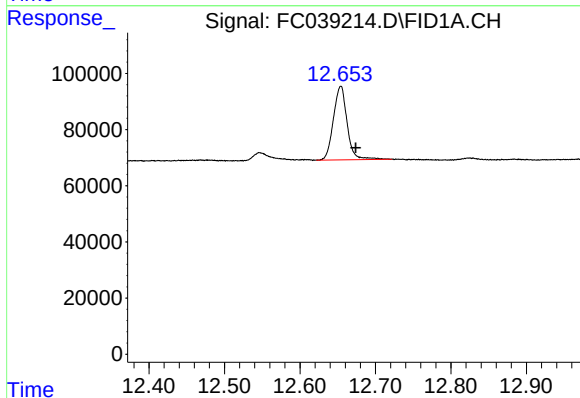


#12 1-chlorooctadecane (SURR)

R.T.: 12.654 min
Delta R.T.: -0.020 min
Response: 330296
Conc: 2.80 ug/ml

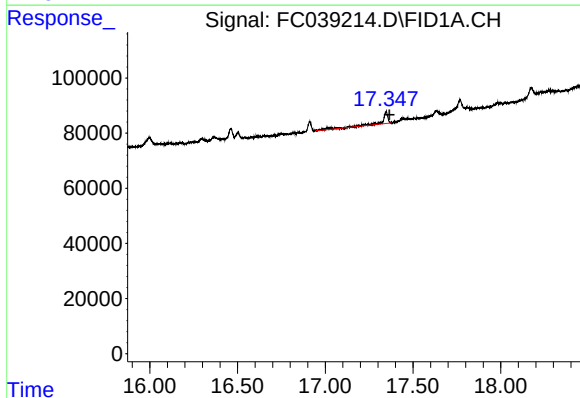


#17 n-Tricontane (C30)

R.T.: 17.347 min
Delta R.T.: -0.019 min
Response: 100165
Conc: 0.86 ug/ml

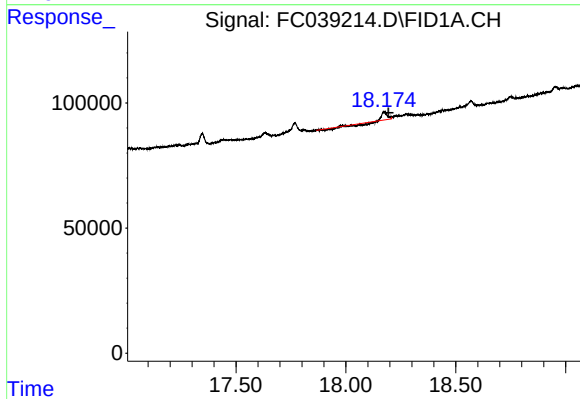

#18 n-Dotriacontane (C32)


R.T.: 18.174 min
Delta R.T.: -0.020 min
Response: 2313
Conc: 0.02 ug/ml

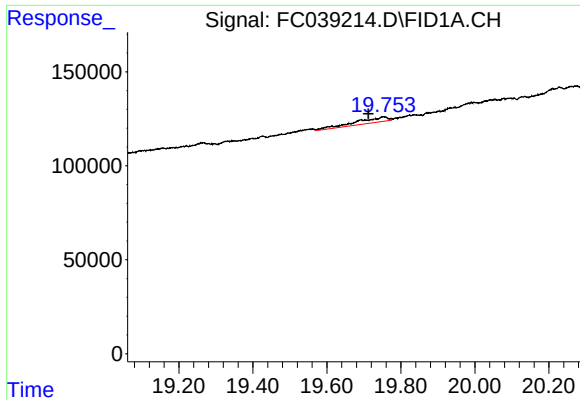

#20 n-Hexatriacontane (C36)

R.T.: 19.753 min
Delta R.T.: 0.041 min
Response: 169889
Conc: 2.14 ug/ml

Instrument :
FID_C
ClientSampleId :
CL-01-021419-ADL

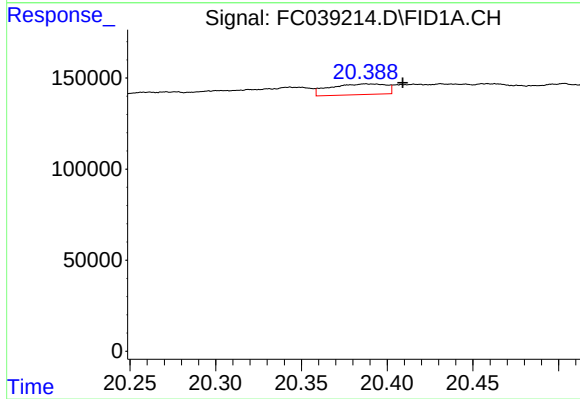

#21 n-Octatriacontane (C38)

R.T.: 20.389 min
Delta R.T.: -0.020 min
Response: 133704
Conc: 1.82 ug/ml