

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021519AL\
 Data File : FC039228.D
 Signal(s) : FID1A.CH
 Acq On : 16 Feb 2019 5:01
 Operator : AJ\SJ
 Sample : K1484-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 M-3-S2

Integration File: autoint1.e
 Quant Time: Feb 17 23:46:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.652	4294193	36.419 ug/ml
Spiked Amount 50.000		Recovery =	72.84%
Target Compounds			
16) T n-Octacosane (C28)	16.460	116777	1.002 ug/ml
17) T n-Tricontane (C30)	17.342	188601	1.625 ug/ml
18) T n-Dotriacontane (C32)	18.173	71285	0.655 ug/ml
19) T n-Tetratriacontane (C34)	18.949	129606	1.399 ug/ml
20) T n-Hexatriacontane (C36)	19.711	114066	1.436 ug/ml
21) T n-Octatriacontane (C38)	20.384	424745	5.783 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021519AL\
Data File : FC039228.D
Signal(s) : FID1A.CH
Acq On : 16 Feb 2019 5:01
Operator : AJ\SJ
Sample : K1484-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
M-3-S2

Integration File: autoint1.e
Quant Time: Feb 17 23:46:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

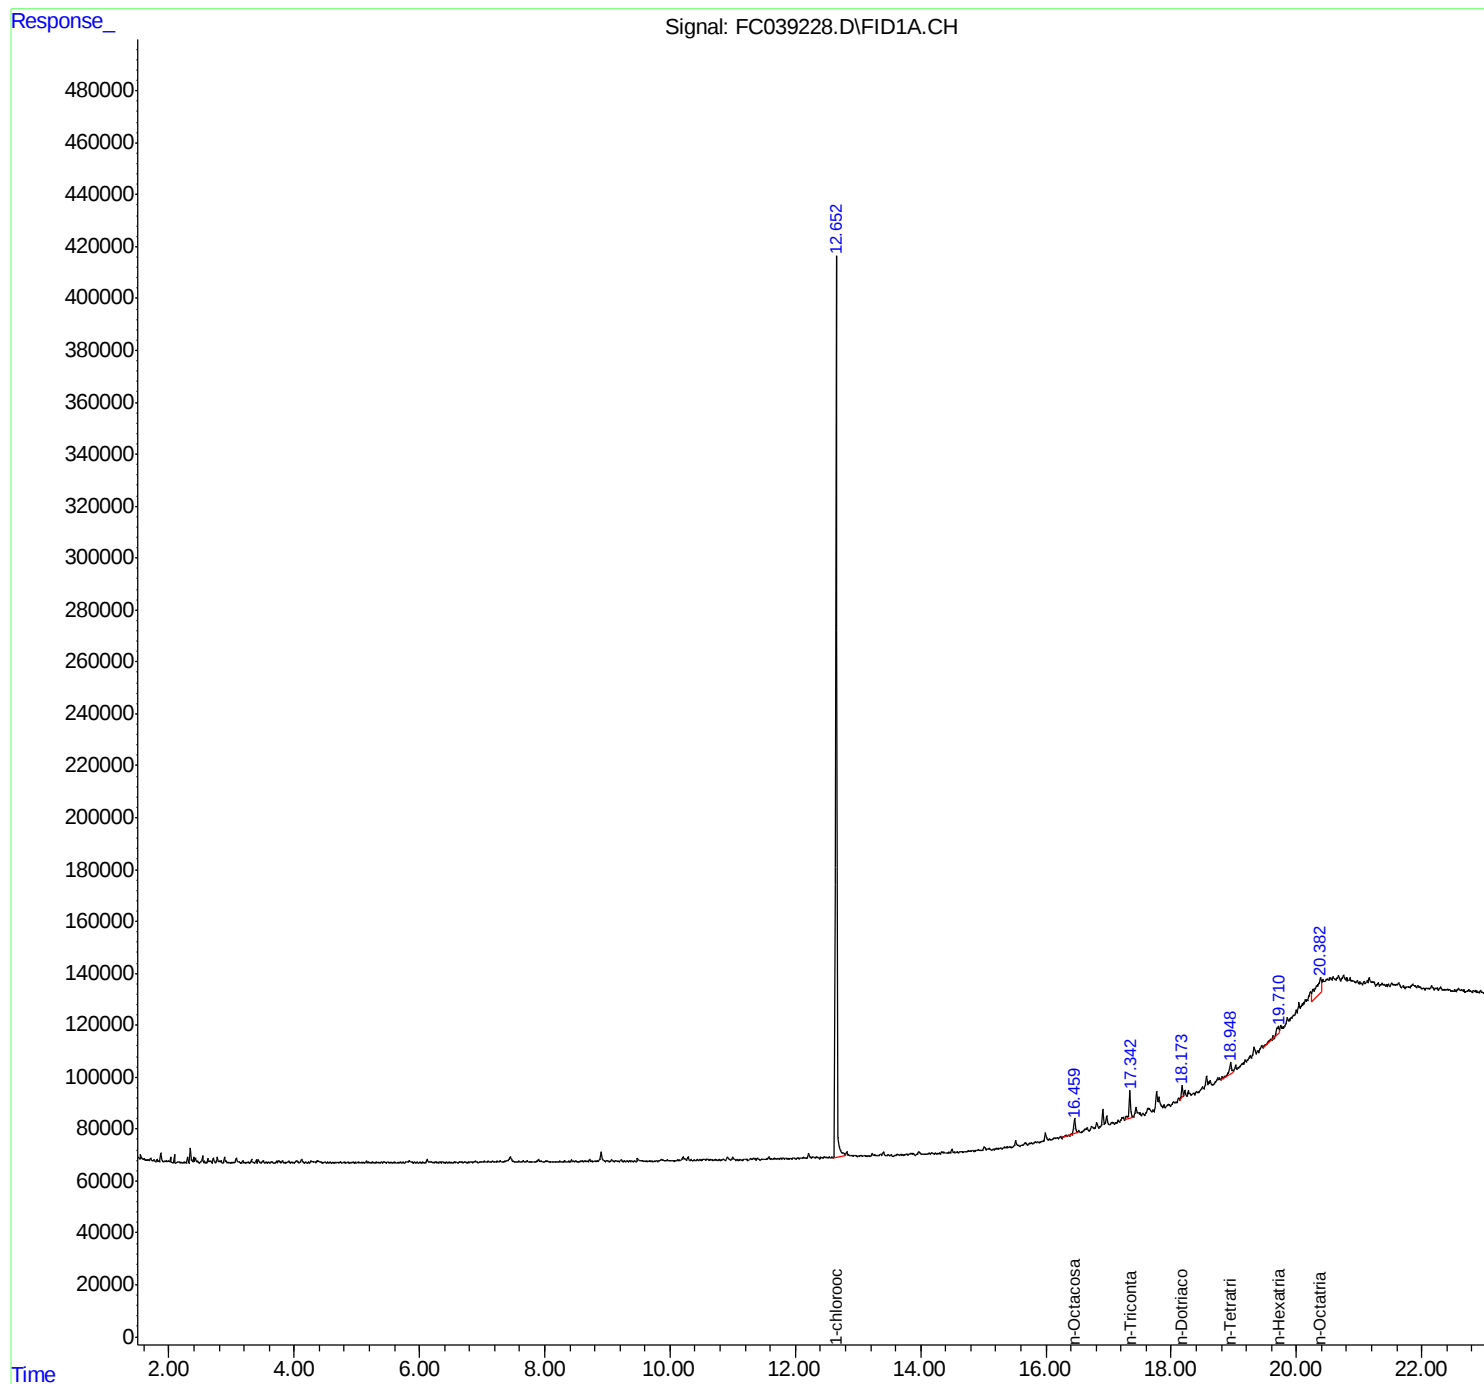


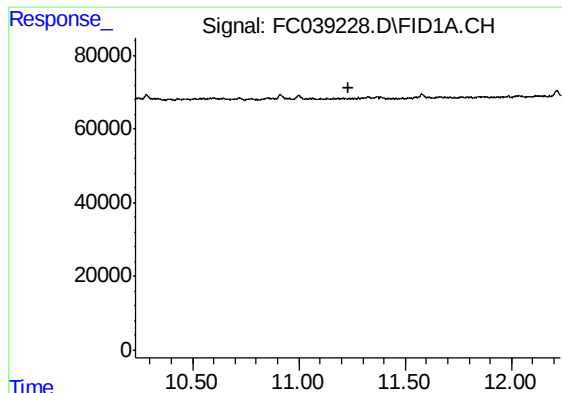

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
M-3-S2

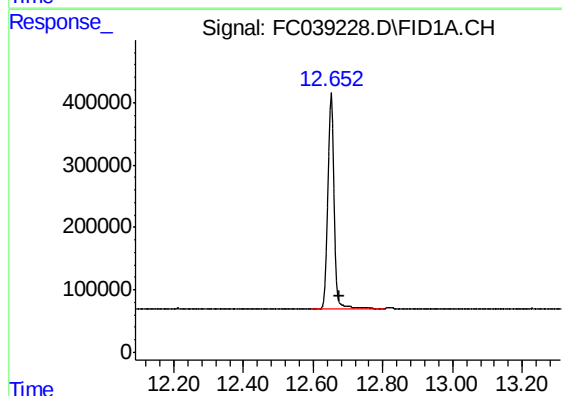


#12 1-chlorooctadecane (SURR)

R.T.: 12.652 min
Delta R.T.: -0.022 min
Response: 4294193
Conc: 36.42 ug/ml

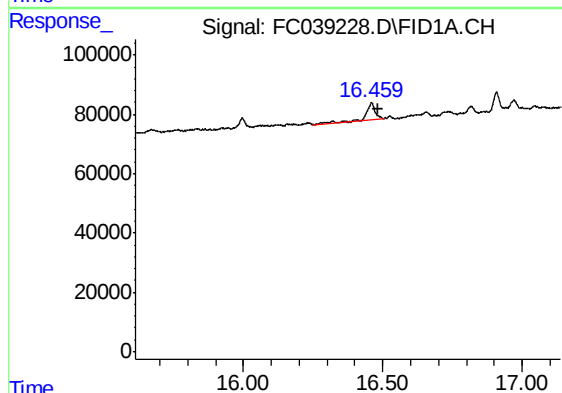


#16 n-Octacosane (C28)

R.T.: 16.460 min
Delta R.T.: -0.023 min
Response: 116777
Conc: 1.00 ug/ml

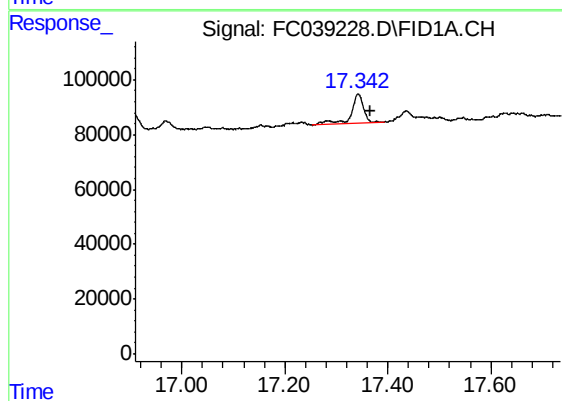

#17 n-Tricontane (C30)


R.T.: 17.342 min
Delta R.T.: -0.024 min
Response: 188601
Conc: 1.63 ug/ml

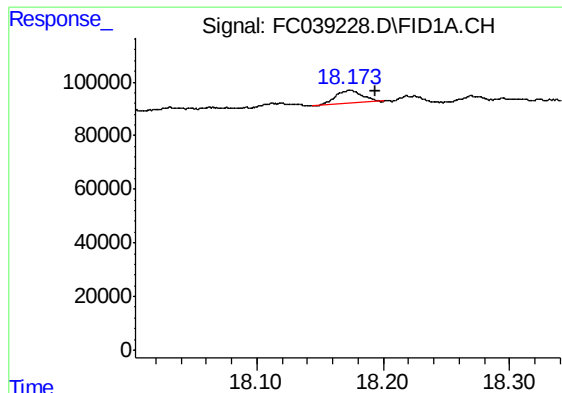

#18 n-Dotriacontane (C32)


R.T.: 18.173 min
Delta R.T.: -0.021 min
Response: 71285
Conc: 0.66 ug/ml

Instrument :
FID_C
ClientSampleId :
M-3-S2

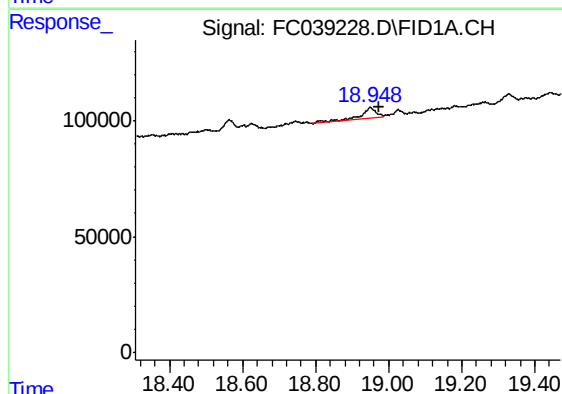


#19 n-Tetratriacontane (C34)

R.T.: 18.949 min
Delta R.T.: -0.026 min
Response: 129606
Conc: 1.40 ug/ml

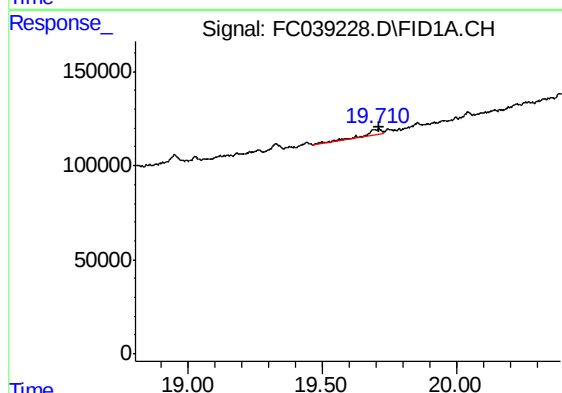

#20 n-Hexatriacontane (C36)

R.T.: 19.711 min
Delta R.T.: -0.001 min
Response: 114066
Conc: 1.44 ug/ml

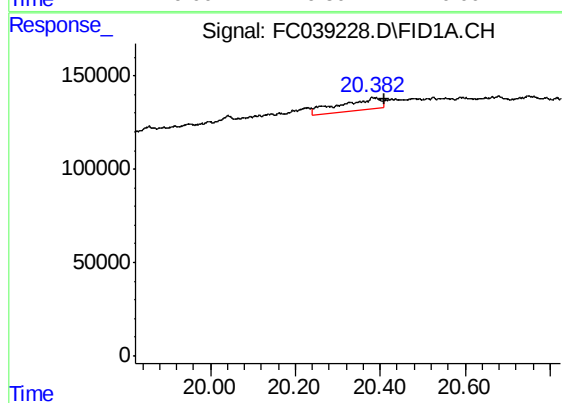

#21 n-Octatriacontane (C38)

R.T.: 20.384 min
Delta R.T.: -0.025 min
Response: 424745
Conc: 5.78 ug/ml