

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021519AL\
 Data File : FC039230.D
 Signal(s) : FID1A.CH
 Acq On : 16 Feb 2019 6:12
 Operator : AJ\SJ
 Sample : K1484-13D
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 M-3-D1D

Integration File: autoint1.e
 Quant Time: Feb 17 23:46:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.651	4103378	34.800 ug/ml
Spiked Amount 50.000		Recovery =	69.60%
Target Compounds			
15) T n-Hexacosane (C26)	15.514	94129	0.810 ug/ml
16) T n-Octacosane (C28)	16.458	170083	1.459 ug/ml
17) T n-Tricontane (C30)	17.341	223854	1.929 ug/ml
18) T n-Dotriacontane (C32)	18.171	178347	1.640 ug/ml
19) T n-Tetratriacontane (C34)	18.950	79220	0.855 ug/ml
21) T n-Octatriacontane (C38)	20.386	45777	0.623 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021519AL\
Data File : FC039230.D
Signal(s) : FID1A.CH
Acq On : 16 Feb 2019 6:12
Operator : AJ\SJ
Sample : K1484-13D
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
M-3-D1D

Integration File: autoint1.e
Quant Time: Feb 17 23:46:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

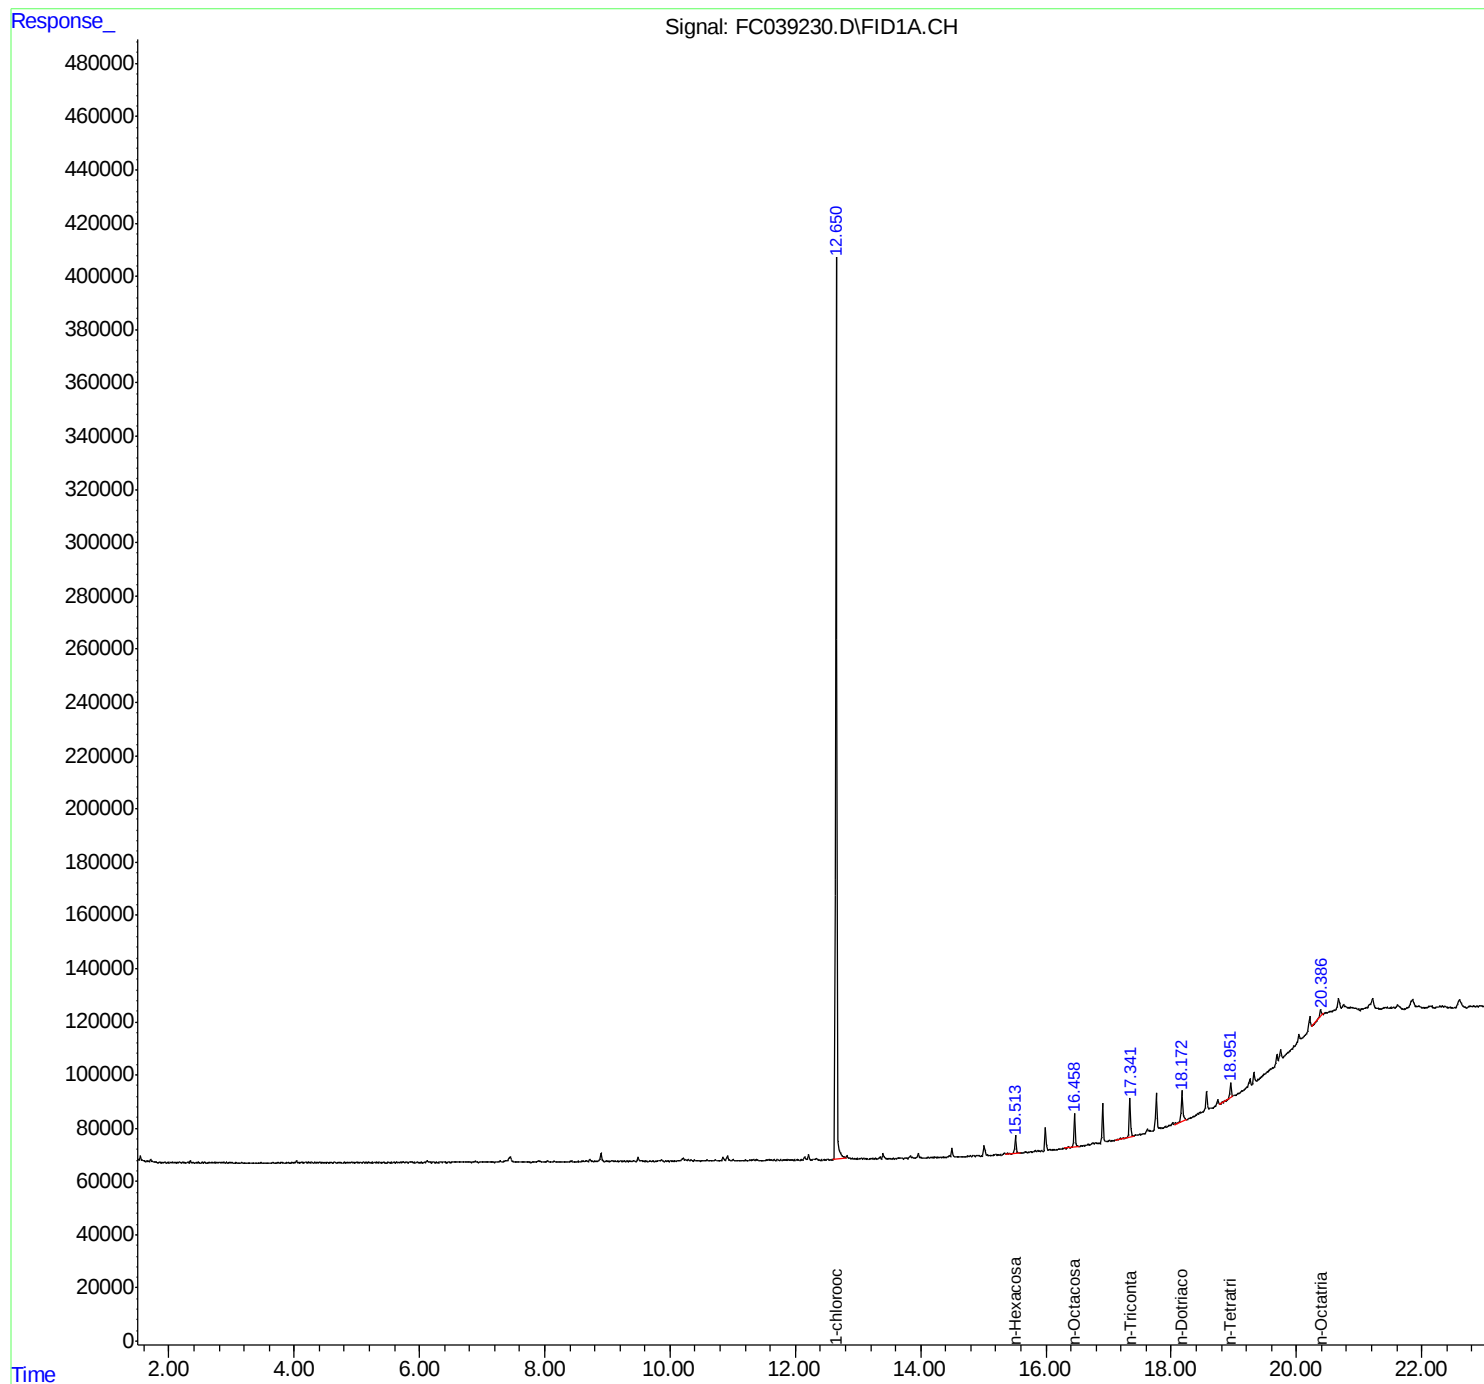


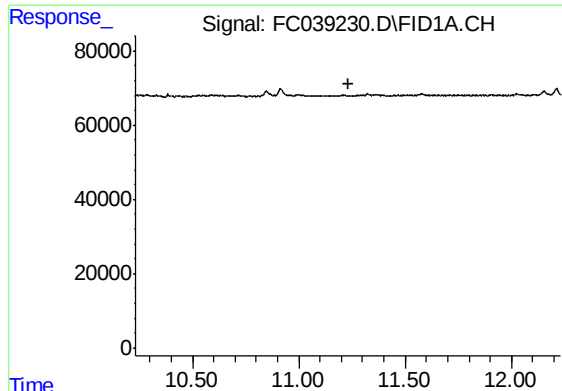

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
M-3-D1D

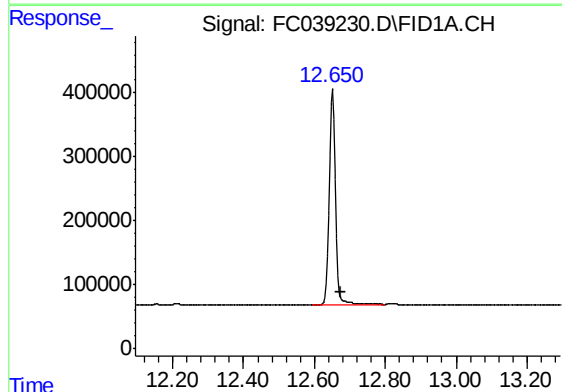


#12 1-chlorooctadecane (SURR)

R.T.: 12.651 min
Delta R.T.: -0.023 min
Response: 4103378
Conc: 34.80 ug/ml

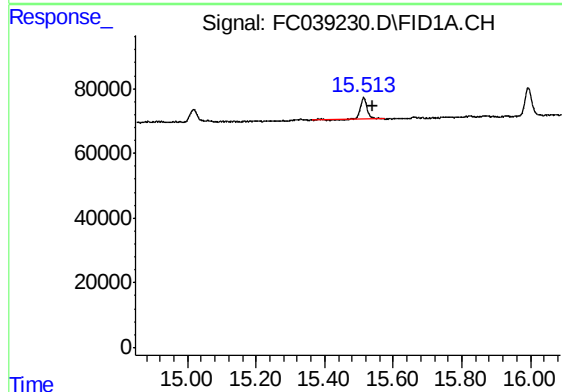


#15 n-Hexacosane (C26)

R.T.: 15.514 min
Delta R.T.: -0.025 min
Response: 94129
Conc: 0.81 ug/ml

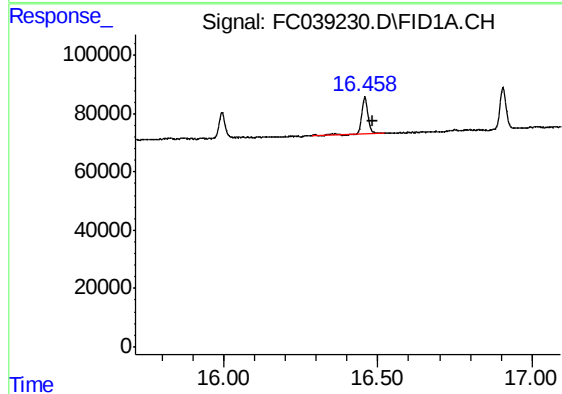

#16 n-Octacosane (C28)


R.T.: 16.458 min
Delta R.T.: -0.025 min
Response: 170083
Conc: 1.46 ug/ml

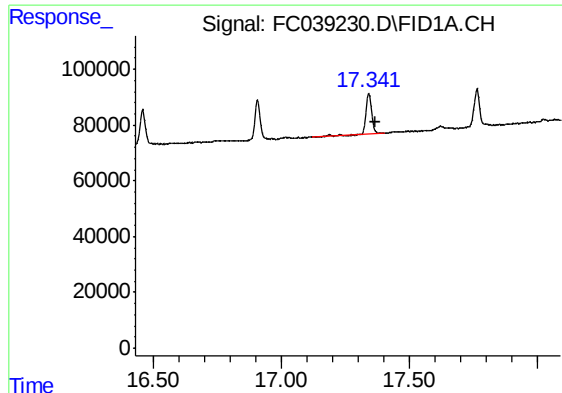

#17 n-Tricontane (C30)


R.T.: 17.341 min
Delta R.T.: -0.025 min
Response: 223854
Conc: 1.93 ug/ml

Instrument :
FID_C
ClientSampleId :
M-3-D1D

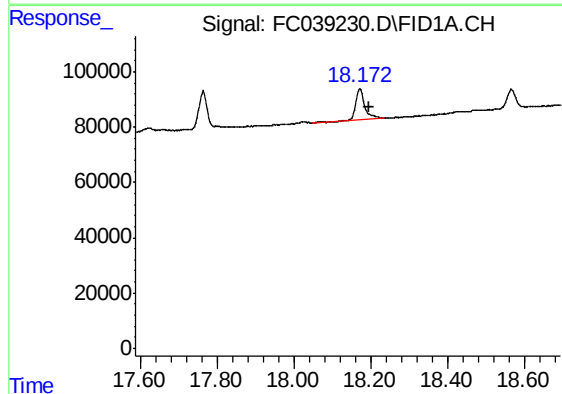


#18 n-Dotriacontane (C32)

R.T.: 18.171 min
Delta R.T.: -0.023 min
Response: 178347
Conc: 1.64 ug/ml

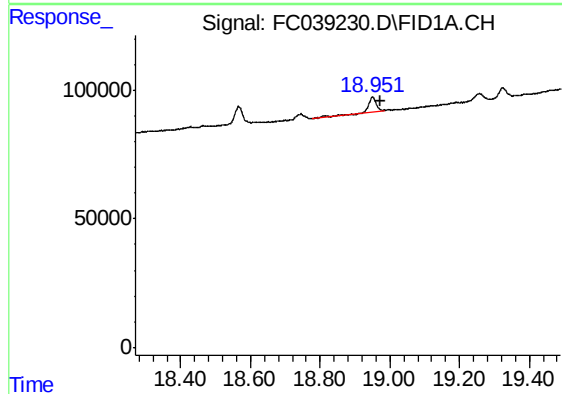

#19 n-Tetratriacontane (C34)

R.T.: 18.950 min
Delta R.T.: -0.025 min
Response: 79220
Conc: 0.86 ug/ml

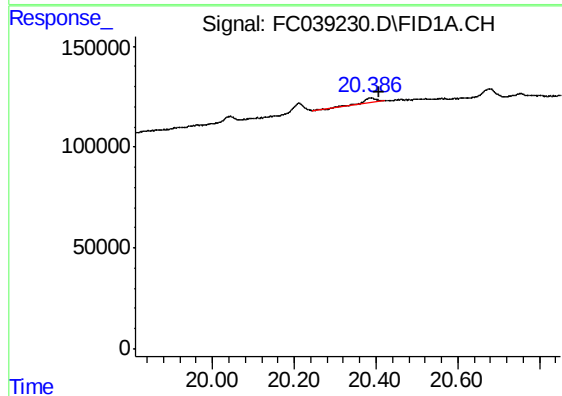

#21 n-Octatriacontane (C38)

R.T.: 20.386 min
Delta R.T.: -0.023 min
Response: 45777
Conc: 0.62 ug/ml