

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
 Data File : FC039288.D
 Signal(s) : FID1A.CH
 Acq On : 19 Feb 2019 17:52
 Operator : AJ\SJ
 Sample : PB117209BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 20 00:58:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.637	6079151	51.557 ug/ml
Spiked Amount 50.000		Recovery =	103.11%
Target Compounds			
17) T n-Tricontane (C30)	17.323	134130	1.156 ug/ml
18) T n-Dotriacontane (C32)	18.150	9718	0.089 ug/ml
19) T n-Tetratriacontane (C34)	18.931	166630	1.799 ug/ml
20) T n-Hexatriacontane (C36)	19.728	207809	2.616 ug/ml
21) T n-Octatriacontane (C38)	20.370	123523	1.682 ug/ml
22) T n-Tetracontane (C40)	21.188	246805	3.308 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
Data File : FC039288.D
Signal(s) : FID1A.CH
Acq On : 19 Feb 2019 17:52
Operator : AJ\SJ
Sample : PB117209BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 20 00:58:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

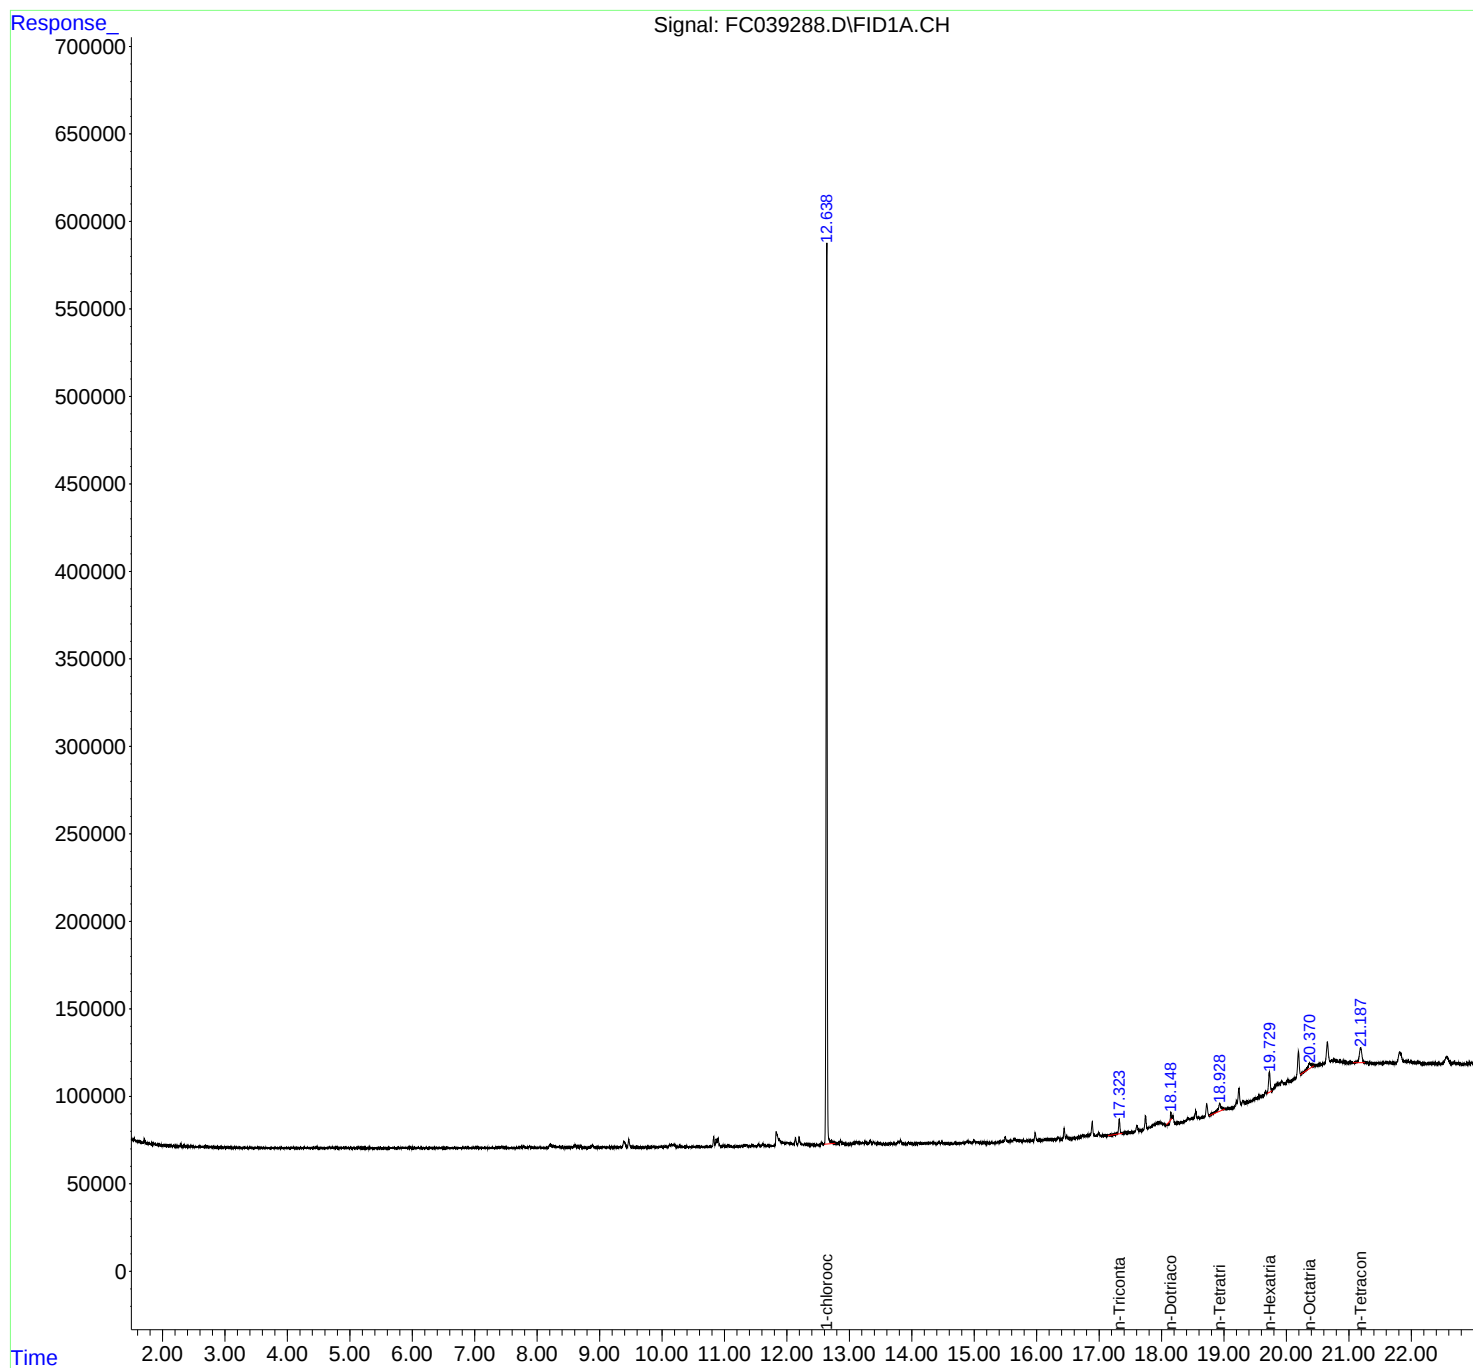


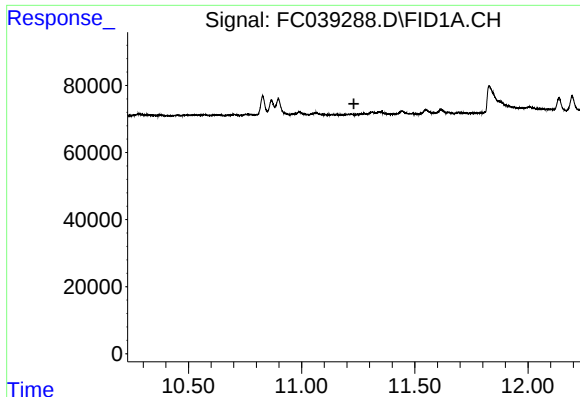

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

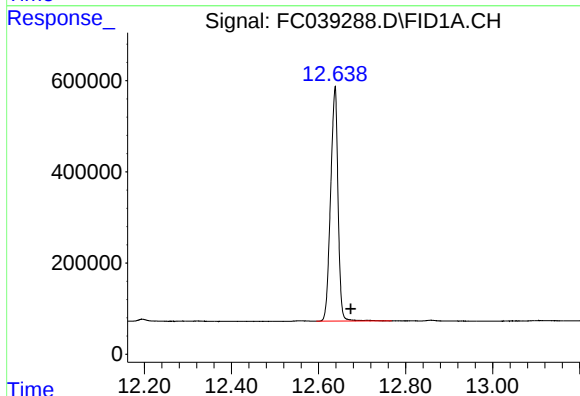


#12 1-chlorooctadecane (SURR)

R.T.: 12.637 min
Delta R.T.: -0.037 min
Response: 6079151
Conc: 51.56 ug/ml

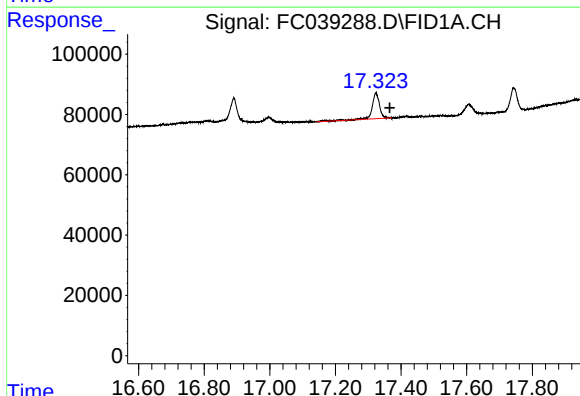


#17 n-Tricontane (C30)

R.T.: 17.323 min
Delta R.T.: -0.043 min
Response: 134130
Conc: 1.16 ug/ml

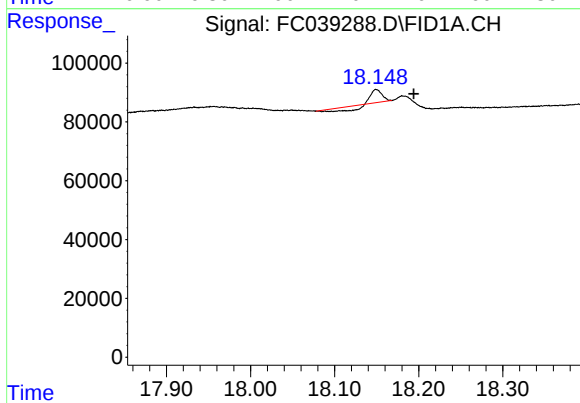

#18 n-Dotriacontane (C32)


R.T.: 18.150 min
Delta R.T.: -0.044 min
Response: 9718
Conc: 0.09 ug/ml

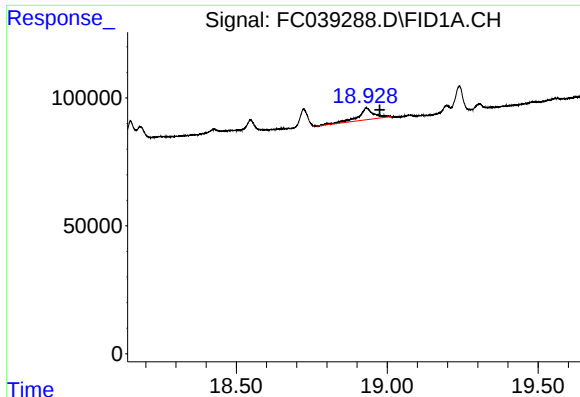

#19 n-Tetratriacontane (C34)


R.T.: 18.931 min
Delta R.T.: -0.044 min
Response: 166630
Conc: 1.80 ug/ml

Instrument :
FID_C
ClientSampleId :

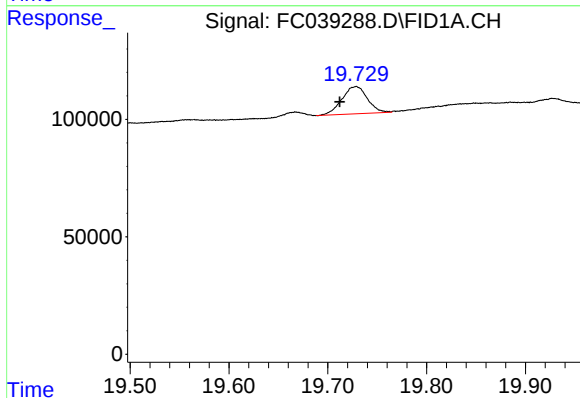


#20 n-Hexatriacontane (C36)

R.T.: 19.728 min
Delta R.T.: 0.016 min
Response: 207809
Conc: 2.62 ug/ml

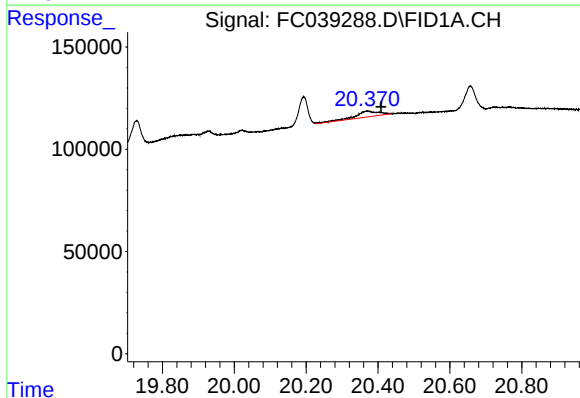

#21 n-Octatriacontane (C38)

R.T.: 20.370 min
Delta R.T.: -0.039 min
Response: 123523
Conc: 1.68 ug/ml

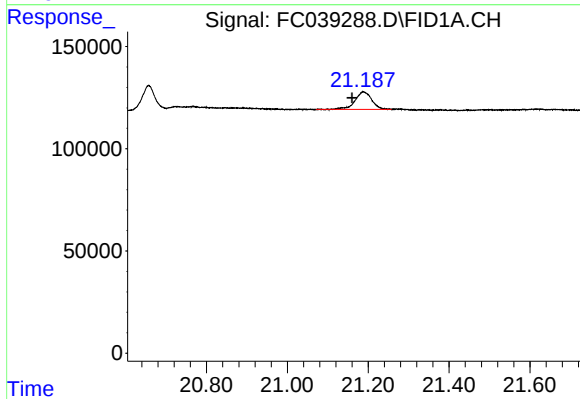

#22 n-Tetracontane (C40)

R.T.: 21.188 min
Delta R.T.: 0.028 min
Response: 246805
Conc: 3.31 ug/ml