

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
 Data File : FC039291.D
 Signal(s) : FID1A.CH
 Acq On : 19 Feb 2019 19:41
 Operator : AJ\SJ
 Sample : K1525-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 20 00:59:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.635	4643733	39.383 ug/ml
Spiked Amount 50.000		Recovery =	78.77%
Target Compounds			
16) T n-Octacosane (C28)	16.438	181729	1.559 ug/ml
17) T n-Tricontane (C30)	17.322	227811	1.963 ug/ml
18) T n-Dotriacontane (C32)	18.150	66466	0.611 ug/ml
19) T n-Tetratriacontane (C34)	18.927	217293	2.346 ug/ml
20) T n-Hexatriacontane (C36)	19.669	96565	1.216 ug/ml
21) T n-Octatriacontane (C38)	20.363	422520	5.753 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
Data File : FC039291.D
Signal(s) : FID1A.CH
Acq On : 19 Feb 2019 19:41
Operator : AJ\SJ
Sample : K1525-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 20 00:59:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

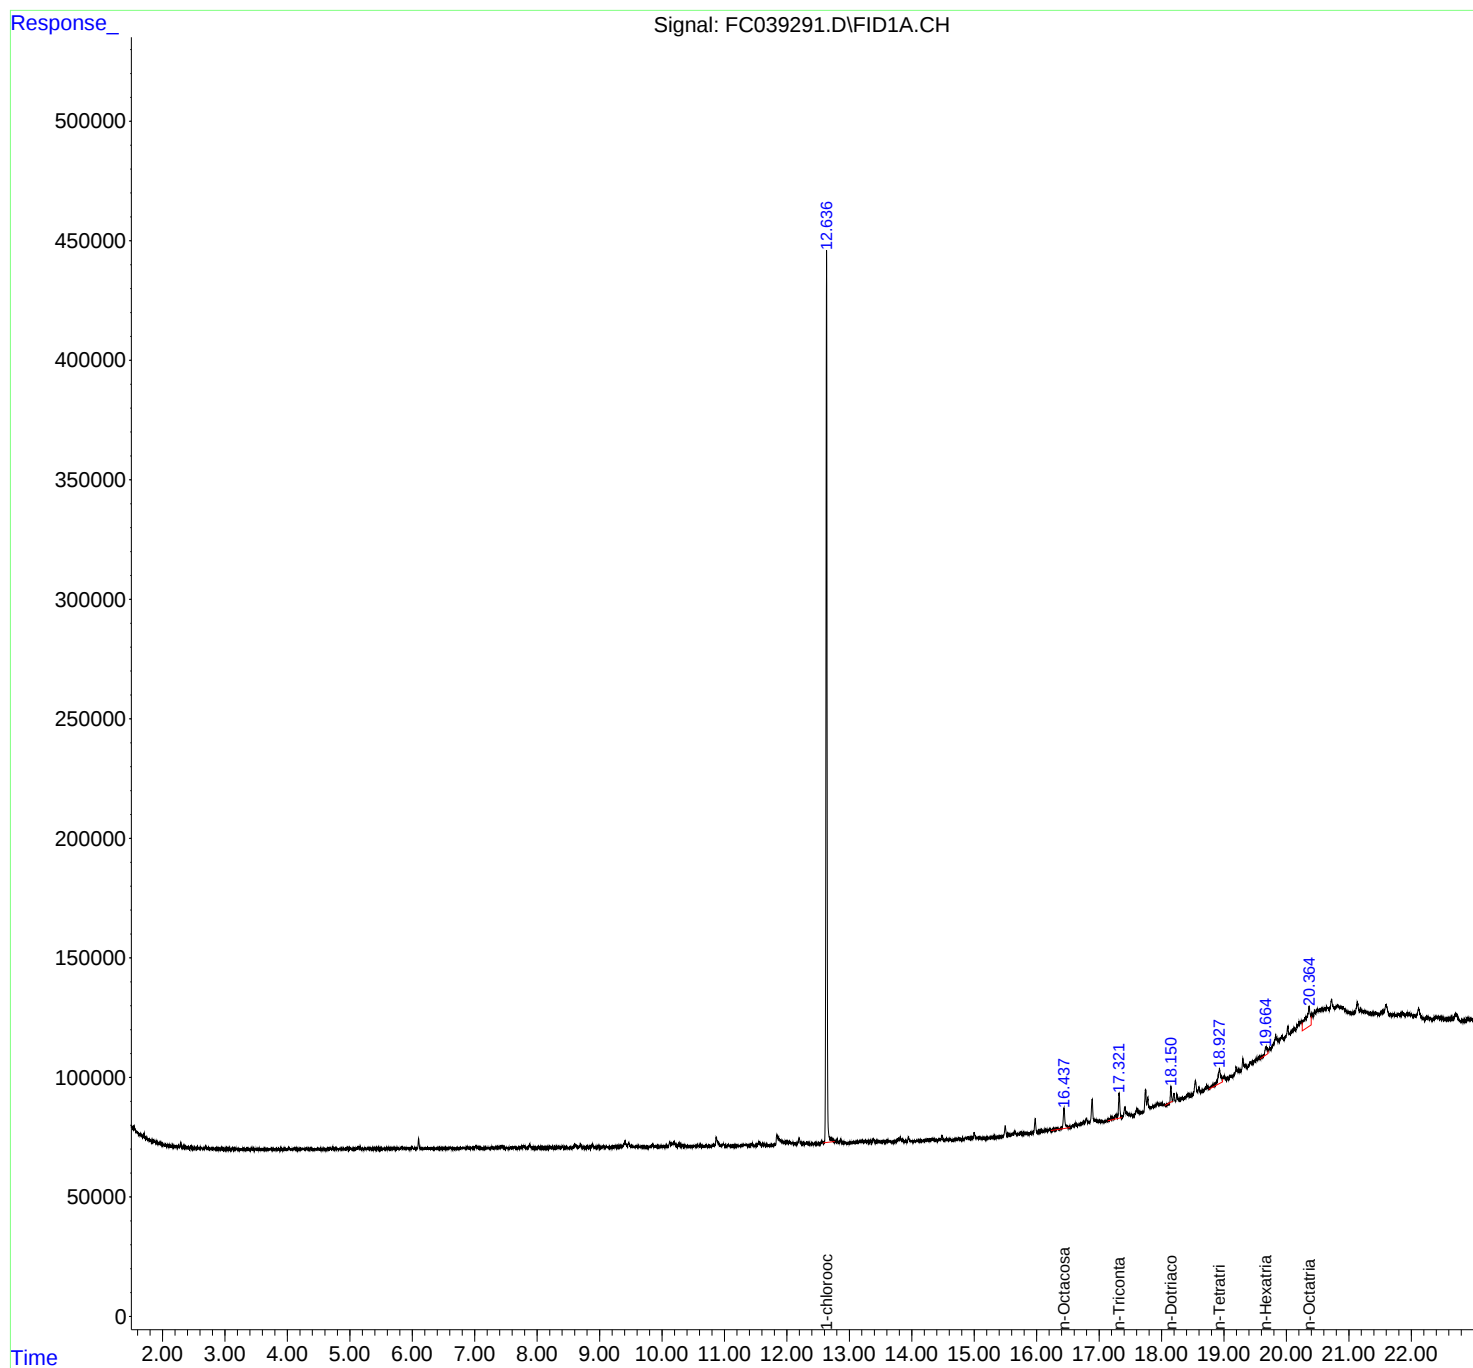


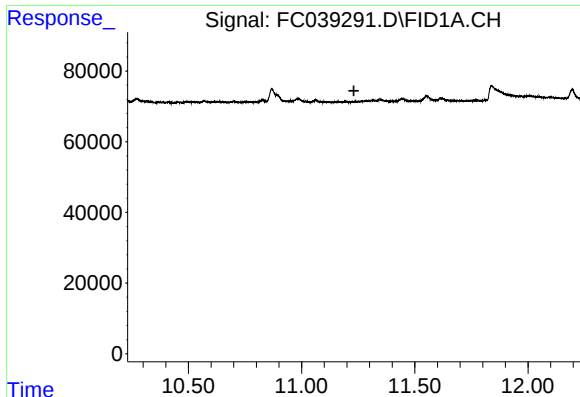

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

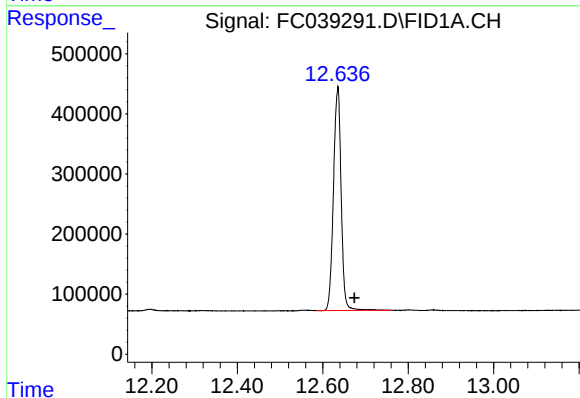


#12 1-chlorooctadecane (SURR)

R.T.: 12.635 min
Delta R.T.: -0.039 min
Response: 4643733
Conc: 39.38 ug/ml

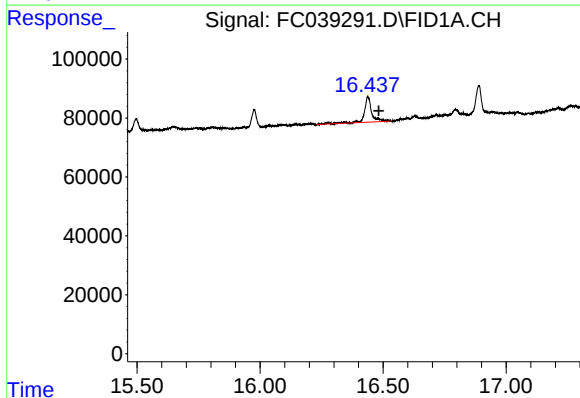


#16 n-Octacosane (C28)

R.T.: 16.438 min
Delta R.T.: -0.045 min
Response: 181729
Conc: 1.56 ug/ml

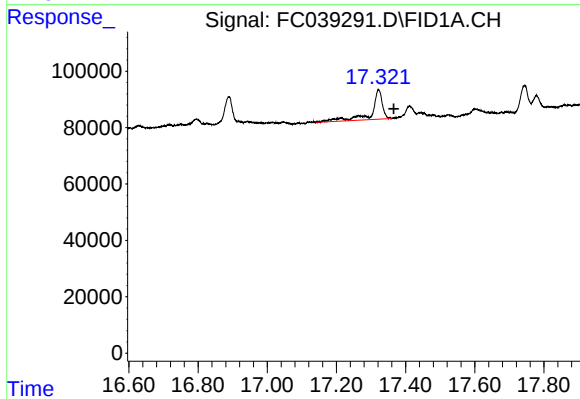

#17 n-Tricontane (C30)


R.T.: 17.322 min
Delta R.T.: -0.044 min
Response: 227811
Conc: 1.96 ug/ml

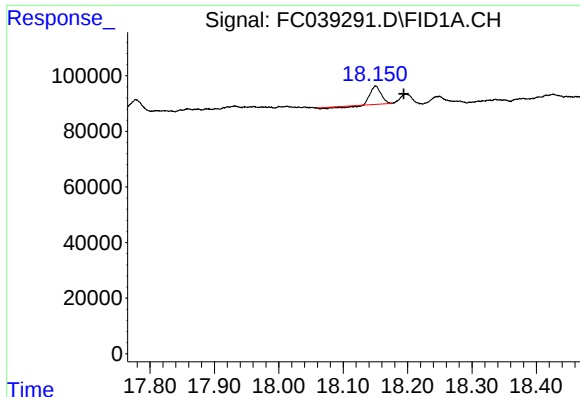

#18 n-Dotriacontane (C32)


R.T.: 18.150 min
Delta R.T.: -0.044 min
Response: 66466
Conc: 0.61 ug/ml

Instrument :
FID_C
ClientSampleId :

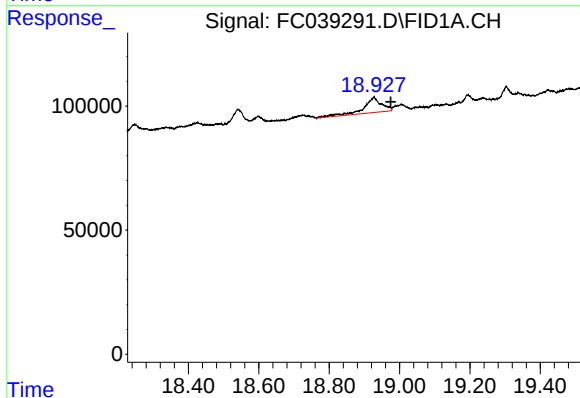


#19 n-Tetratriacontane (C34)

R.T.: 18.927 min
Delta R.T.: -0.048 min
Response: 217293
Conc: 2.35 ug/ml

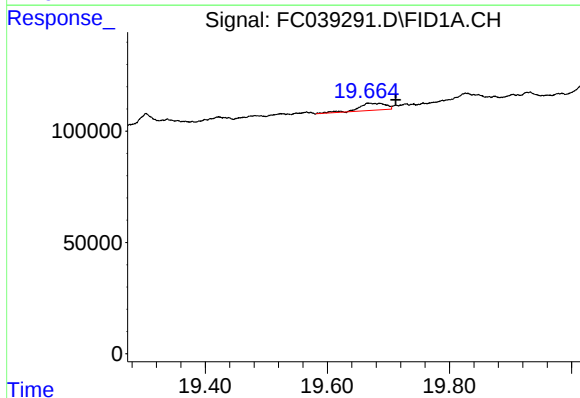

#20 n-Hexatriacontane (C36)

R.T.: 19.669 min
Delta R.T.: -0.043 min
Response: 96565
Conc: 1.22 ug/ml

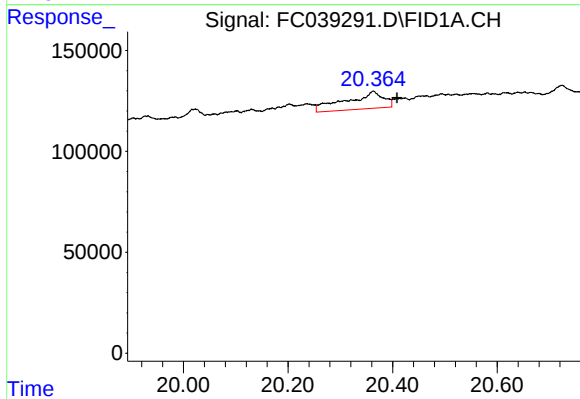

#21 n-Octatriacontane (C38)

R.T.: 20.363 min
Delta R.T.: -0.046 min
Response: 422520
Conc: 5.75 ug/ml