

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
 Data File : FC039293.D
 Signal(s) : FID1A.CH
 Acq On : 19 Feb 2019 20:54
 Operator : AJ\SJ
 Sample : K1525-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 20 00:59:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.634	4278801	36.288 ug/ml
Spiked Amount 50.000		Recovery =	72.58%
Target Compounds			
15) T n-Hexacosane (C26)	15.495	98509	0.847 ug/ml
16) T n-Octacosane (C28)	16.439	192465	1.651 ug/ml
17) T n-Tricontane (C30)	17.321	209181	1.802 ug/ml
18) T n-Dotriacontane (C32)	18.151	145985	1.342 ug/ml
19) T n-Tetratriacontane (C34)	18.929	80505	0.869 ug/ml
20) T n-Hexatriacontane (C36)	19.668	4930	0.062 ug/ml
21) T n-Octatriacontane (C38)	20.363	291115	3.964 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
Data File : FC039293.D
Signal(s) : FID1A.CH
Acq On : 19 Feb 2019 20:54
Operator : AJ\SJ
Sample : K1525-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 20 00:59:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

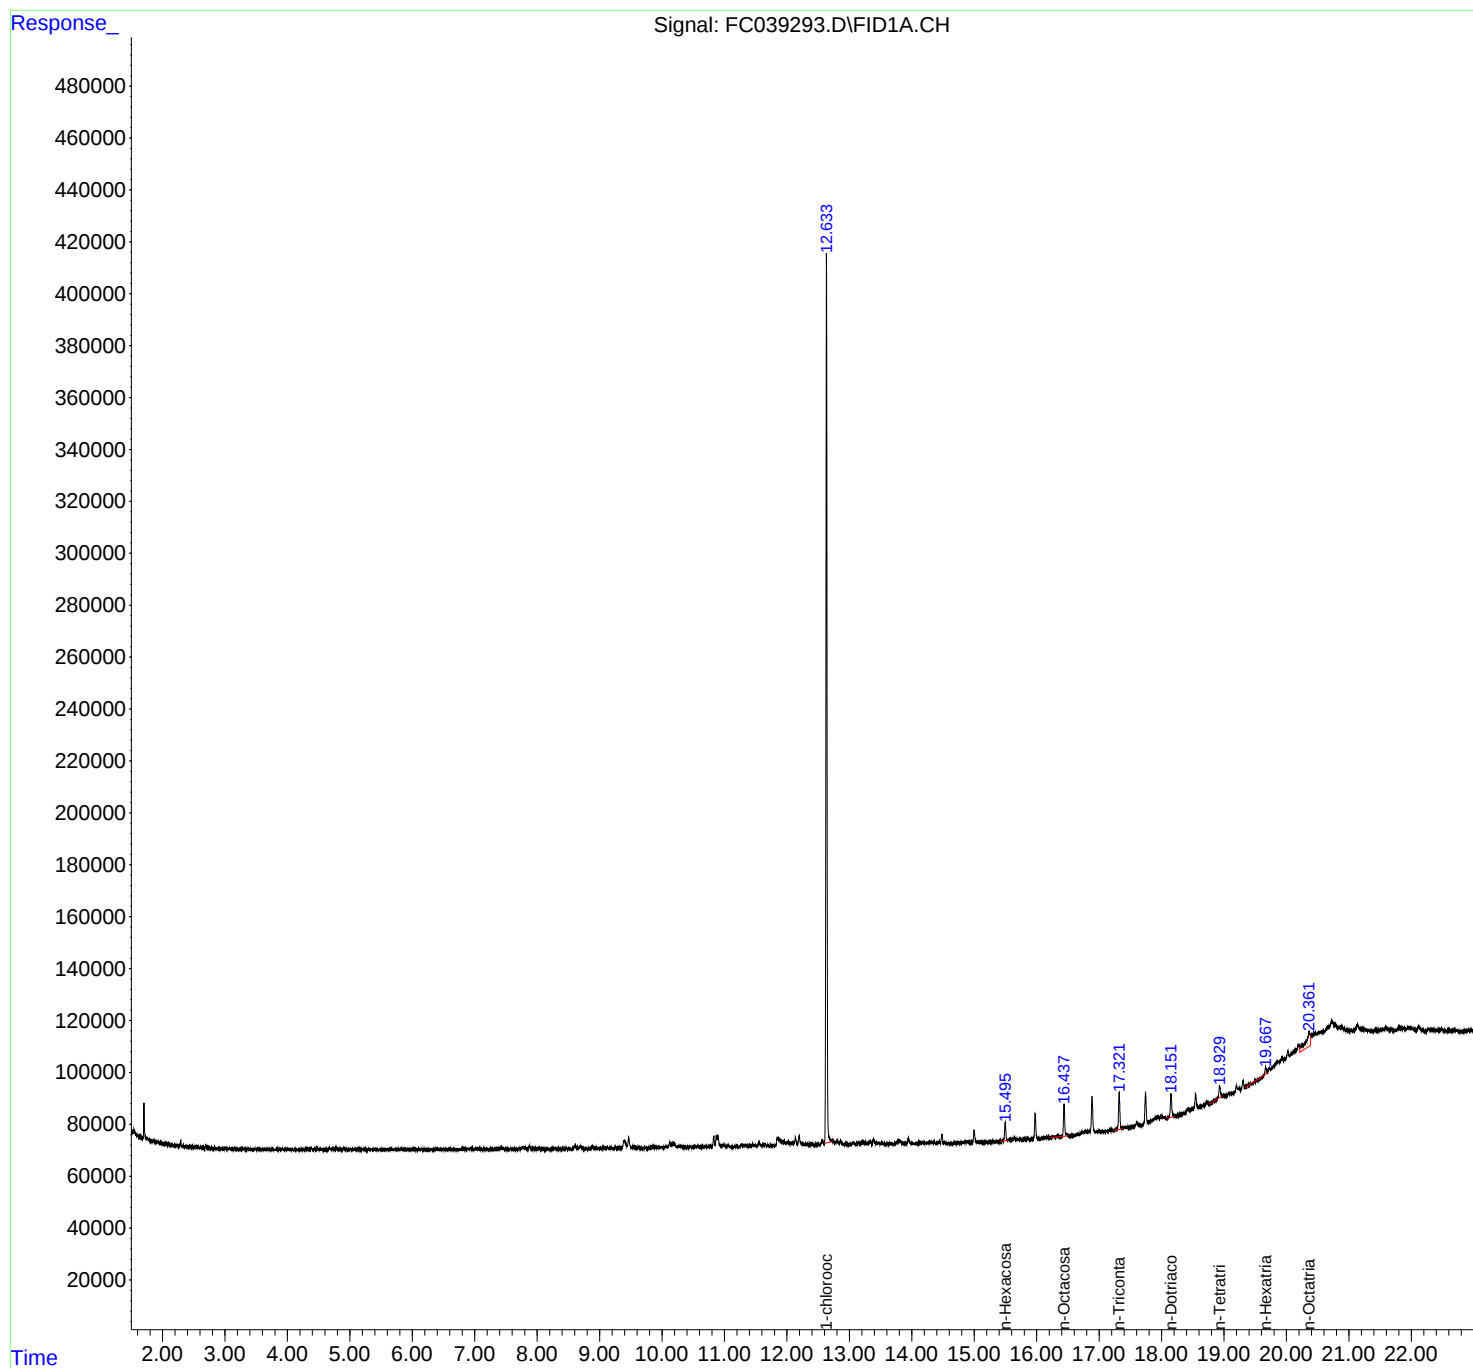


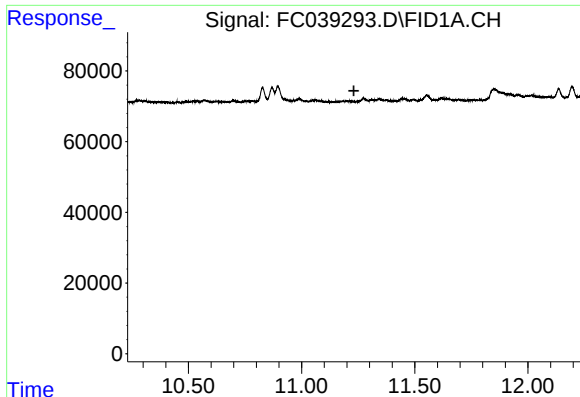

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

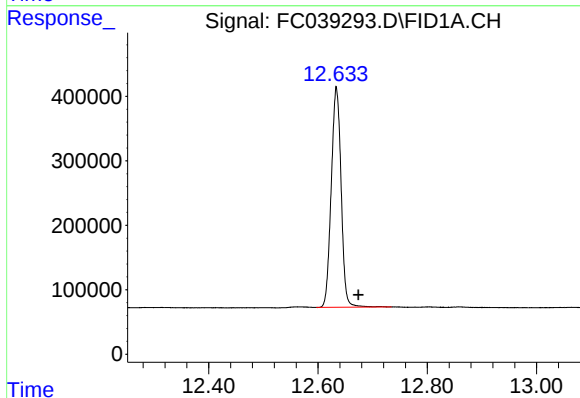


#12 1-chlorooctadecane (SURR)

R.T.: 12.634 min
Delta R.T.: -0.040 min
Response: 4278801
Conc: 36.29 ug/ml

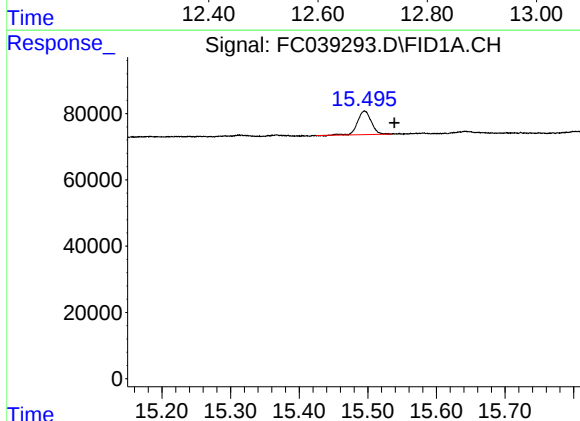


#15 n-Hexacosane (C26)

R.T.: 15.495 min
Delta R.T.: -0.044 min
Response: 98509
Conc: 0.85 ug/ml

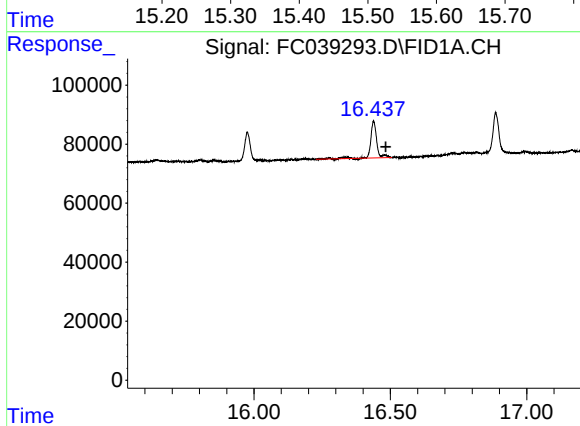

#16 n-Octacosane (C28)


R.T.: 16.439 min
Delta R.T.: -0.044 min
Response: 192465
Conc: 1.65 ug/ml

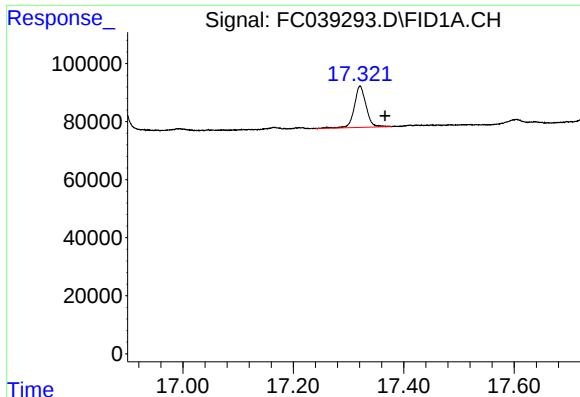

#17 n-Tricontane (C30)


R.T.: 17.321 min
Delta R.T.: -0.045 min
Response: 209181
Conc: 1.80 ug/ml

Instrument :
FID_C
ClientSampleId :

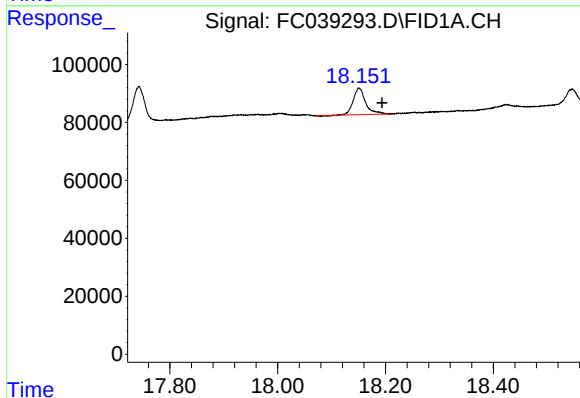


#18 n-Dotriacontane (C32)

R.T.: 18.151 min
Delta R.T.: -0.043 min
Response: 145985
Conc: 1.34 ug/ml

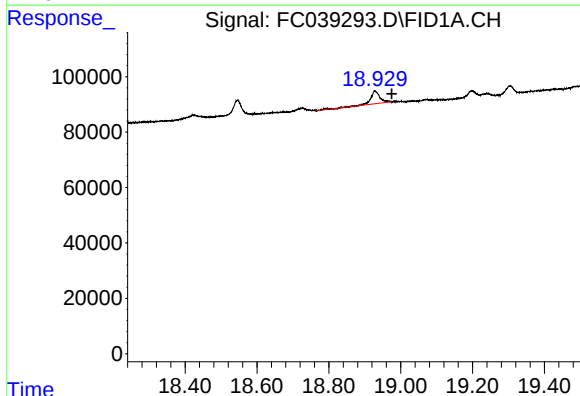


#19 n-Tetratriacontane (C34)

R.T.: 18.929 min
Delta R.T.: -0.046 min
Response: 80505
Conc: 0.87 ug/ml

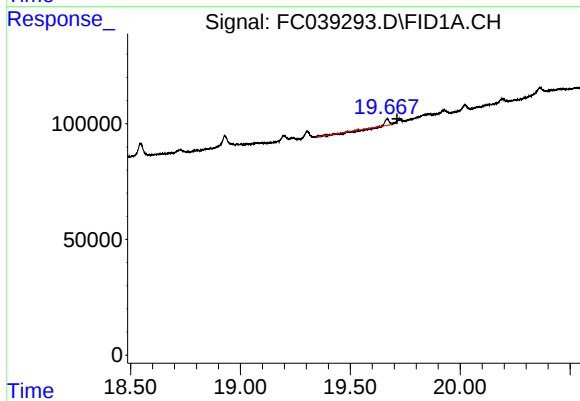

#20 n-Hexatriacontane (C36)

R.T.: 19.668 min
Delta R.T.: -0.044 min
Response: 4930
Conc: 0.06 ug/ml

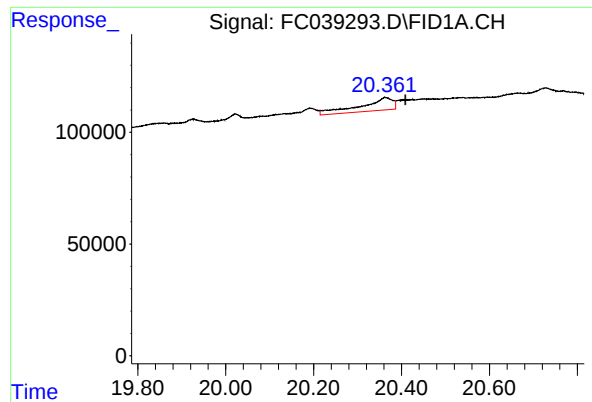

#21 n-Octatriacontane (C38)

R.T.: 20.363 min
Delta R.T.: -0.046 min
Response: 291115
Conc: 3.96 ug/ml

Instrument :
FID_C
ClientSampleId :