

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
 Data File : FC039294.D
 Signal(s) : FID1A.CH
 Acq On : 19 Feb 2019 21:30
 Operator : AJ\SJ
 Sample : K1525-06D
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 20 00:59:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 03:09:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.634	4241224	35.969 ug/ml
Spiked Amount 50.000		Recovery =	71.94%
Target Compounds			
15) T n-Hexacosane (C26)	15.495	89057	0.766 ug/ml
16) T n-Octacosane (C28)	16.439	204152	1.752 ug/ml
17) T n-Tricontane (C30)	17.321	227800	1.963 ug/ml
18) T n-Dotriacontane (C32)	18.149	174104	1.601 ug/ml
19) T n-Tetratriacontane (C34)	18.931	95584	1.032 ug/ml
20) T n-Hexatriacontane (C36)	19.666	39623	0.499 ug/ml
21) T n-Octatriacontane (C38)	20.363	249738	3.400 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC021919AL\
Data File : FC039294.D
Signal(s) : FID1A.CH
Acq On : 19 Feb 2019 21:30
Operator : AJ\SJ
Sample : K1525-06D
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 20 00:59:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 03:09:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

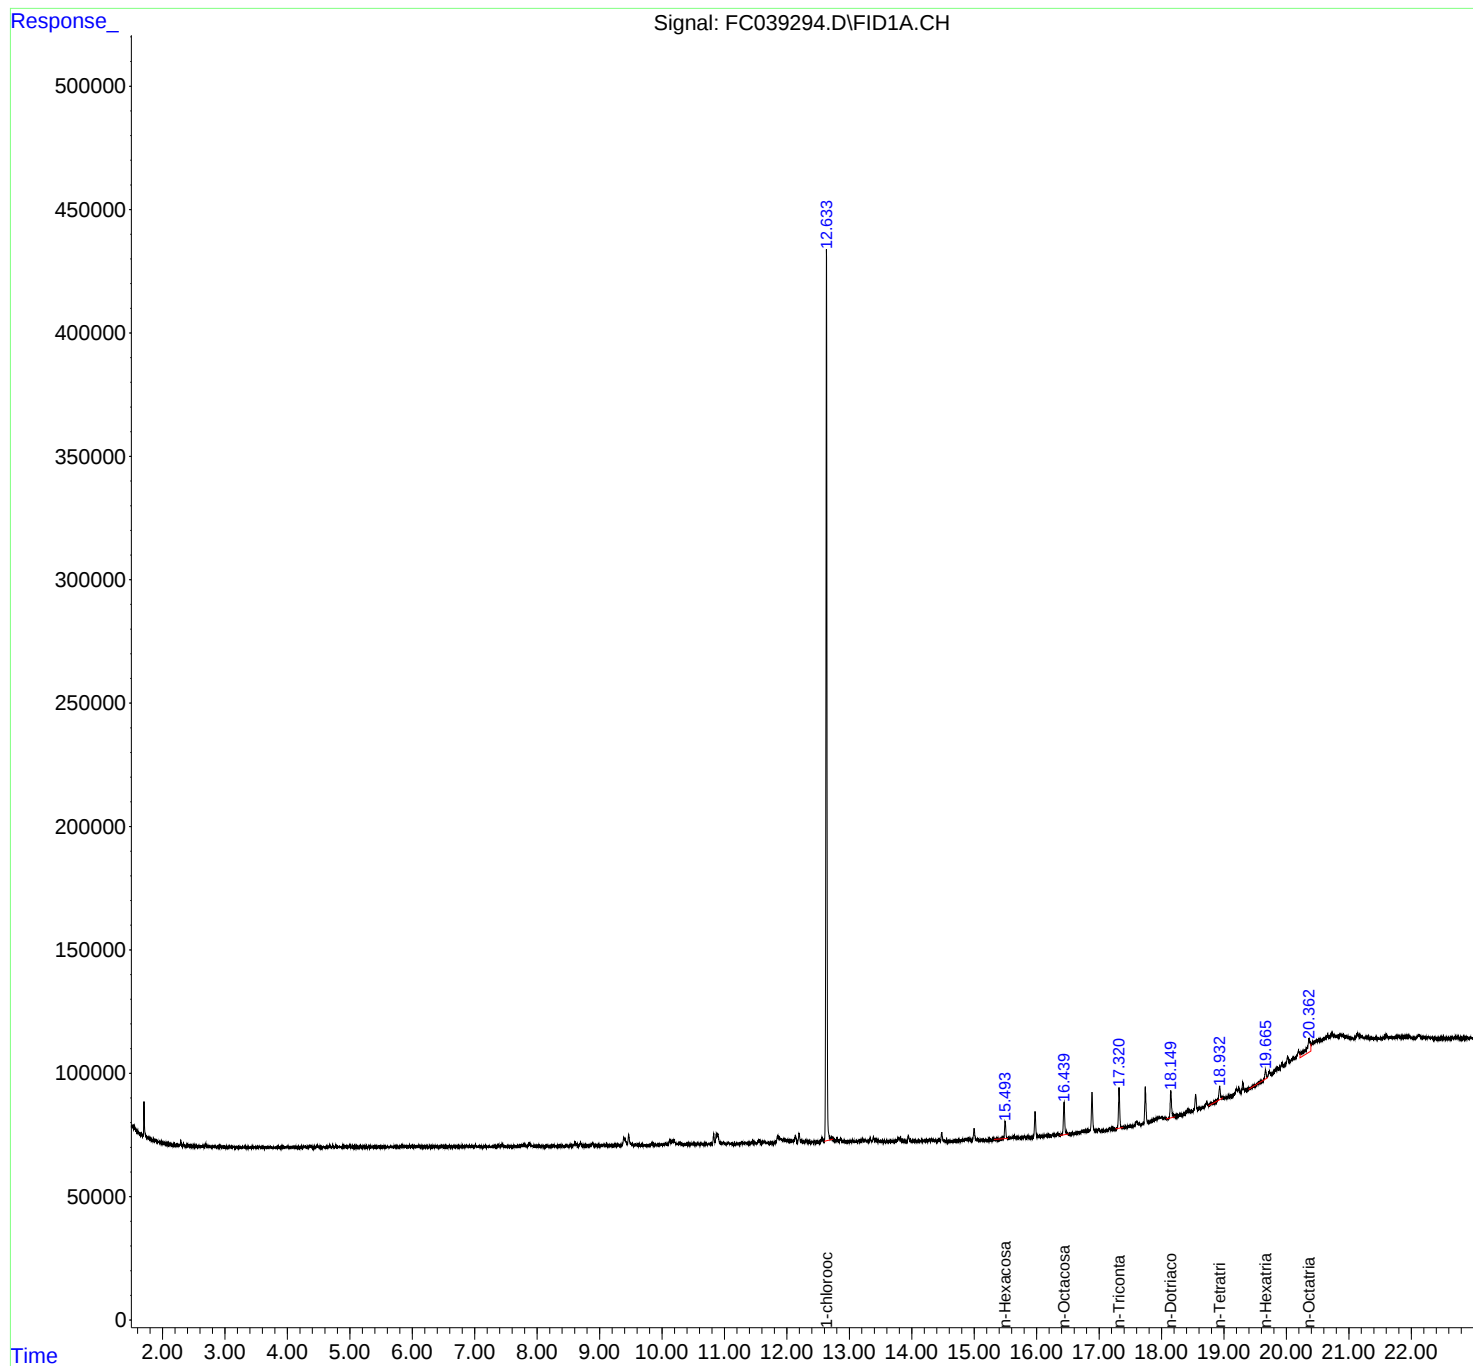


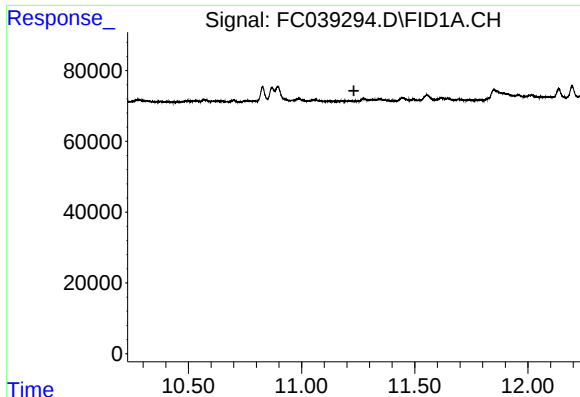

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

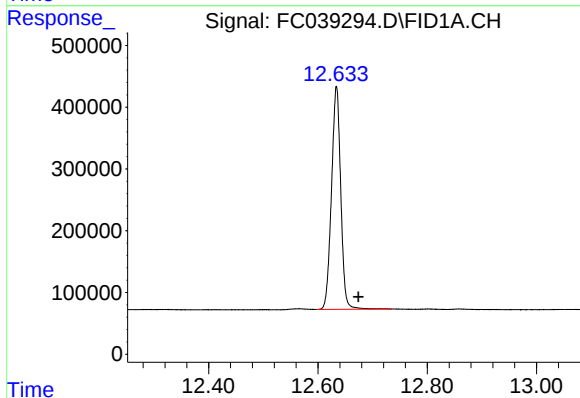


#12 1-chlorooctadecane (SURR)

R.T.: 12.634 min
Delta R.T.: -0.040 min
Response: 4241224
Conc: 35.97 ug/ml

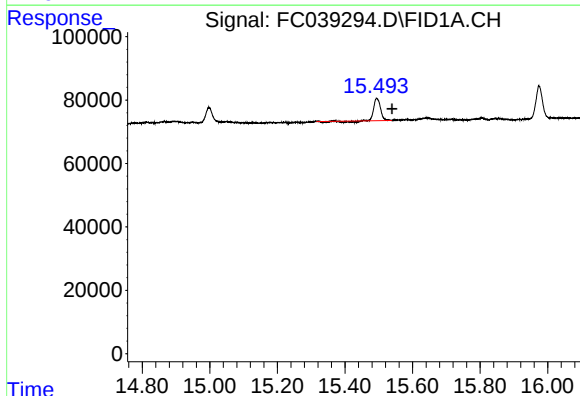


#15 n-Hexacosane (C26)

R.T.: 15.495 min
Delta R.T.: -0.044 min
Response: 89057
Conc: 0.77 ug/ml

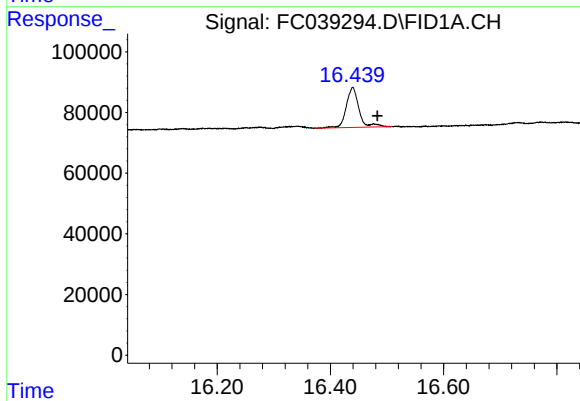

#16 n-Octacosane (C28)


R.T.: 16.439 min
Delta R.T.: -0.044 min
Response: 204152
Conc: 1.75 ug/ml

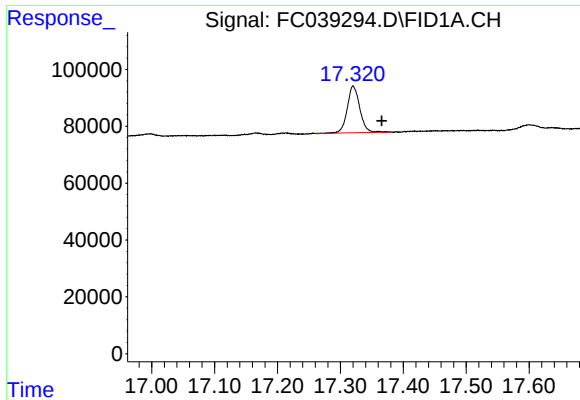

#17 n-Tricontane (C30)


R.T.: 17.321 min
Delta R.T.: -0.045 min
Response: 227800
Conc: 1.96 ug/ml

Instrument :
FID_C
ClientSampleId :

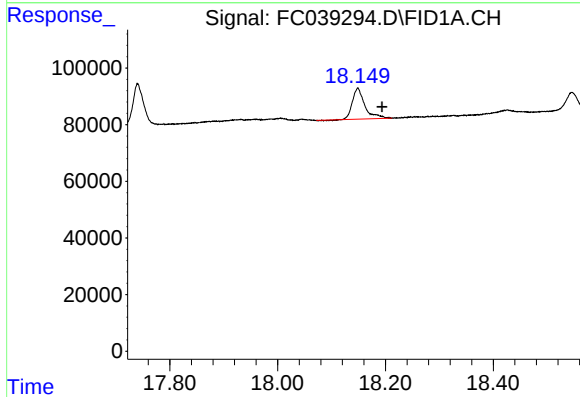


#18 n-Dotriacontane (C32)

R.T.: 18.149 min
Delta R.T.: -0.045 min
Response: 174104
Conc: 1.60 ug/ml

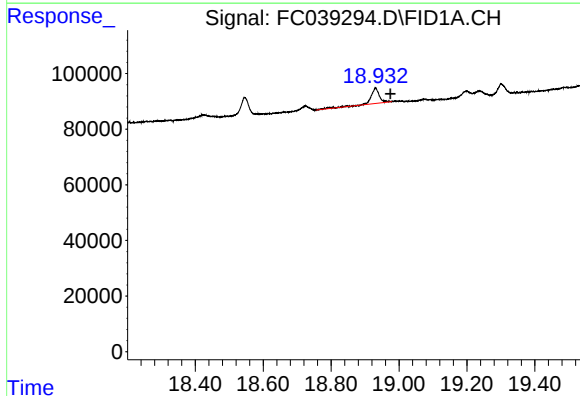


#19 n-Tetratriacontane (C34)

R.T.: 18.931 min
Delta R.T.: -0.044 min
Response: 95584
Conc: 1.03 ug/ml

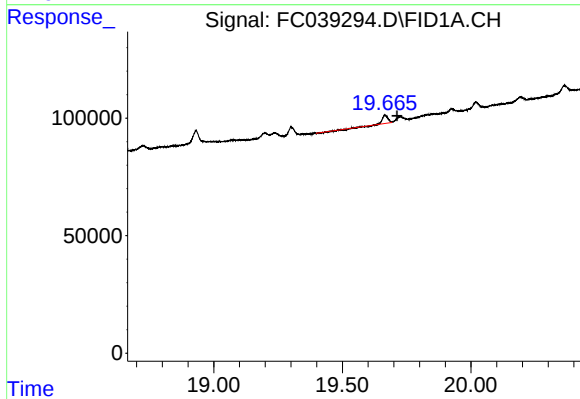

#20 n-Hexatriacontane (C36)

R.T.: 19.666 min
Delta R.T.: -0.046 min
Response: 39623
Conc: 0.50 ug/ml

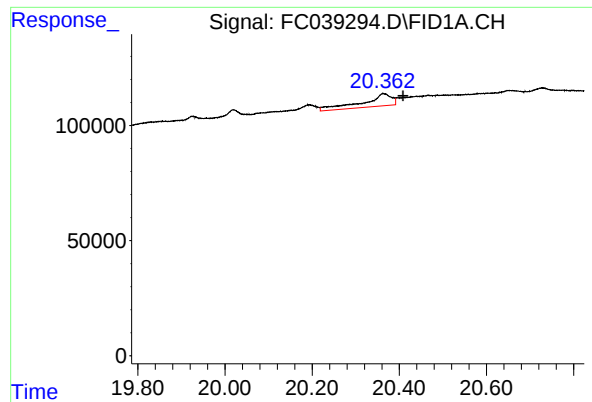

#21 n-Octatriacontane (C38)

R.T.: 20.363 min
Delta R.T.: -0.046 min
Response: 249738
Conc: 3.40 ug/ml

Instrument :
FID_C
ClientSampleId :