

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC022124AL\
Data File : FC065798.D
Signal(s) : FID1A.ch
Acq On : 21 Feb 2024 08:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 10:38:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:26:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.452	1250	0.008 ug/ml
21) T	n-Octatriacontane (C38)	20.686	189540	1.339 ug/ml
22) T	n-Tetracontane (C40)	21.540	37087	0.266 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC022124AL\
Data File : FC065798.D
Signal(s) : FID1A.ch
Acq On : 21 Feb 2024 08:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 10:38:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:26:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

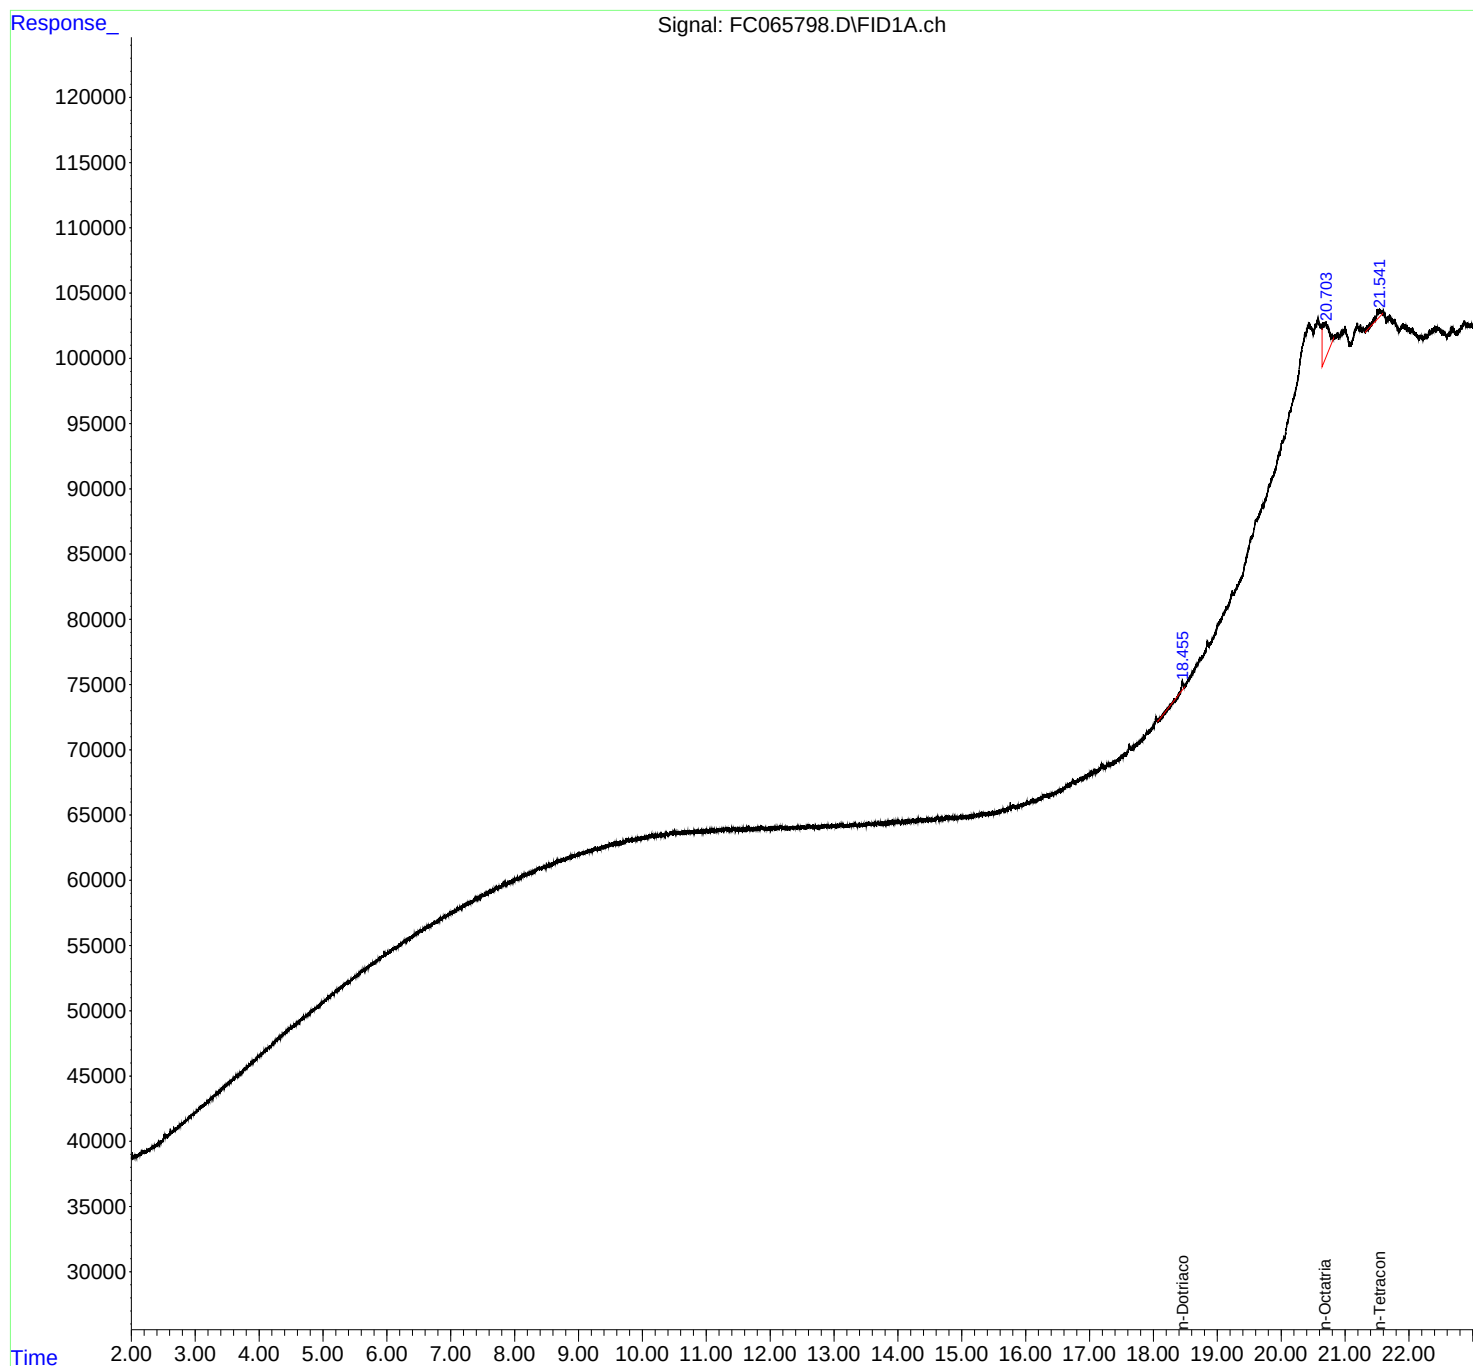


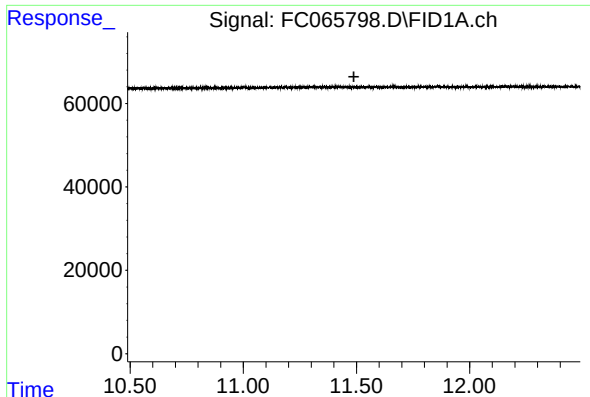

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

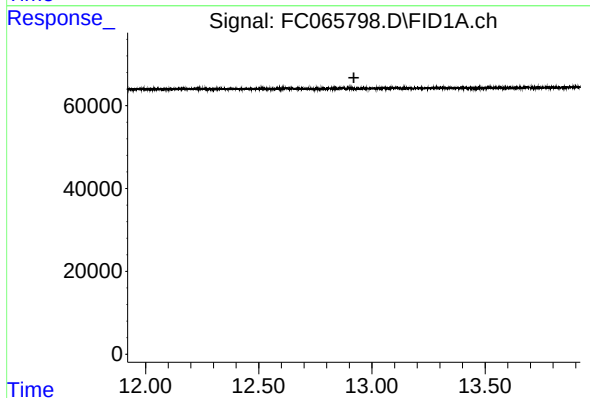


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.920 min
Response: 0
Conc: N.D.

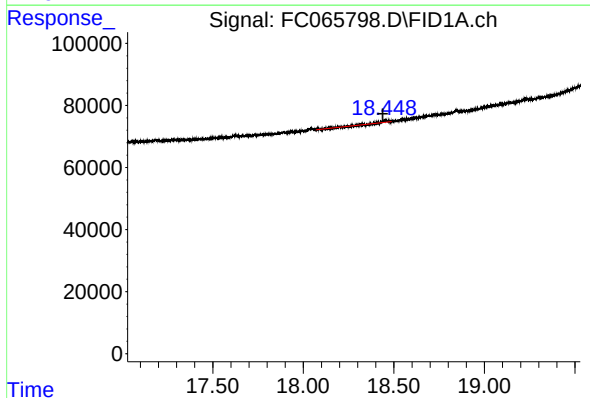


#18 n-Dotriacontane (C32)

R.T.: 18.452 min
Delta R.T.: 0.014 min
Response: 1250
Conc: 0.01 ug/ml

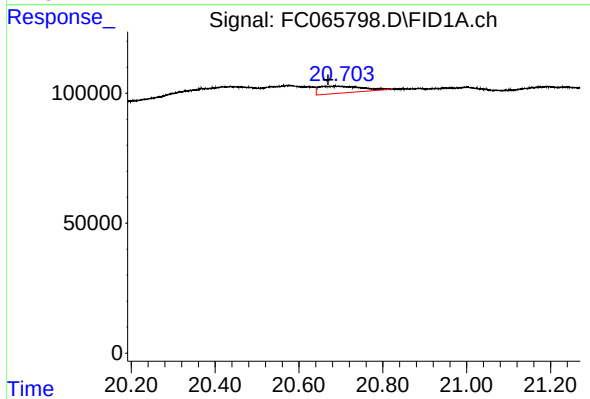

#21 n-Octatriacontane (C38)

R.T.: 20.686 min
Delta R.T.: 0.017 min
Response: 189540
Conc: 1.34 ug/ml

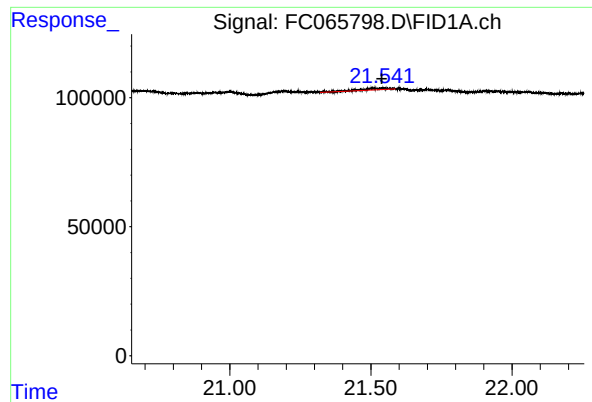

#22 n-Tetracontane (C40)

R.T.: 21.540 min
Delta R.T.: 0.001 min
Response: 37087
Conc: 0.27 ug/ml

Instrument :
FID_C
ClientSampleId :