

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC022624AL\
 Data File : FC065852.D
 Signal(s) : FID1A.ch
 Acq On : 26 Feb 2024 08:58
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 27 02:21:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020824.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 08 13:26:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.464	45600	0.308 ug/ml
19) T	n-Tetratriacontane (C34)	19.233	19599	0.135 ug/ml
20) T	n-Hexatriacontane (C36)	20.005f	229114	1.614 ug/ml
21) T	n-Octatriacontane (C38)	20.651	48845	0.345 ug/ml
22) T	n-Tetracontane (C40)	21.514	306673	2.199 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC022624AL\
Data File : FC065852.D
Signal(s) : FID1A.ch
Acq On : 26 Feb 2024 08:58
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 27 02:21:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:26:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

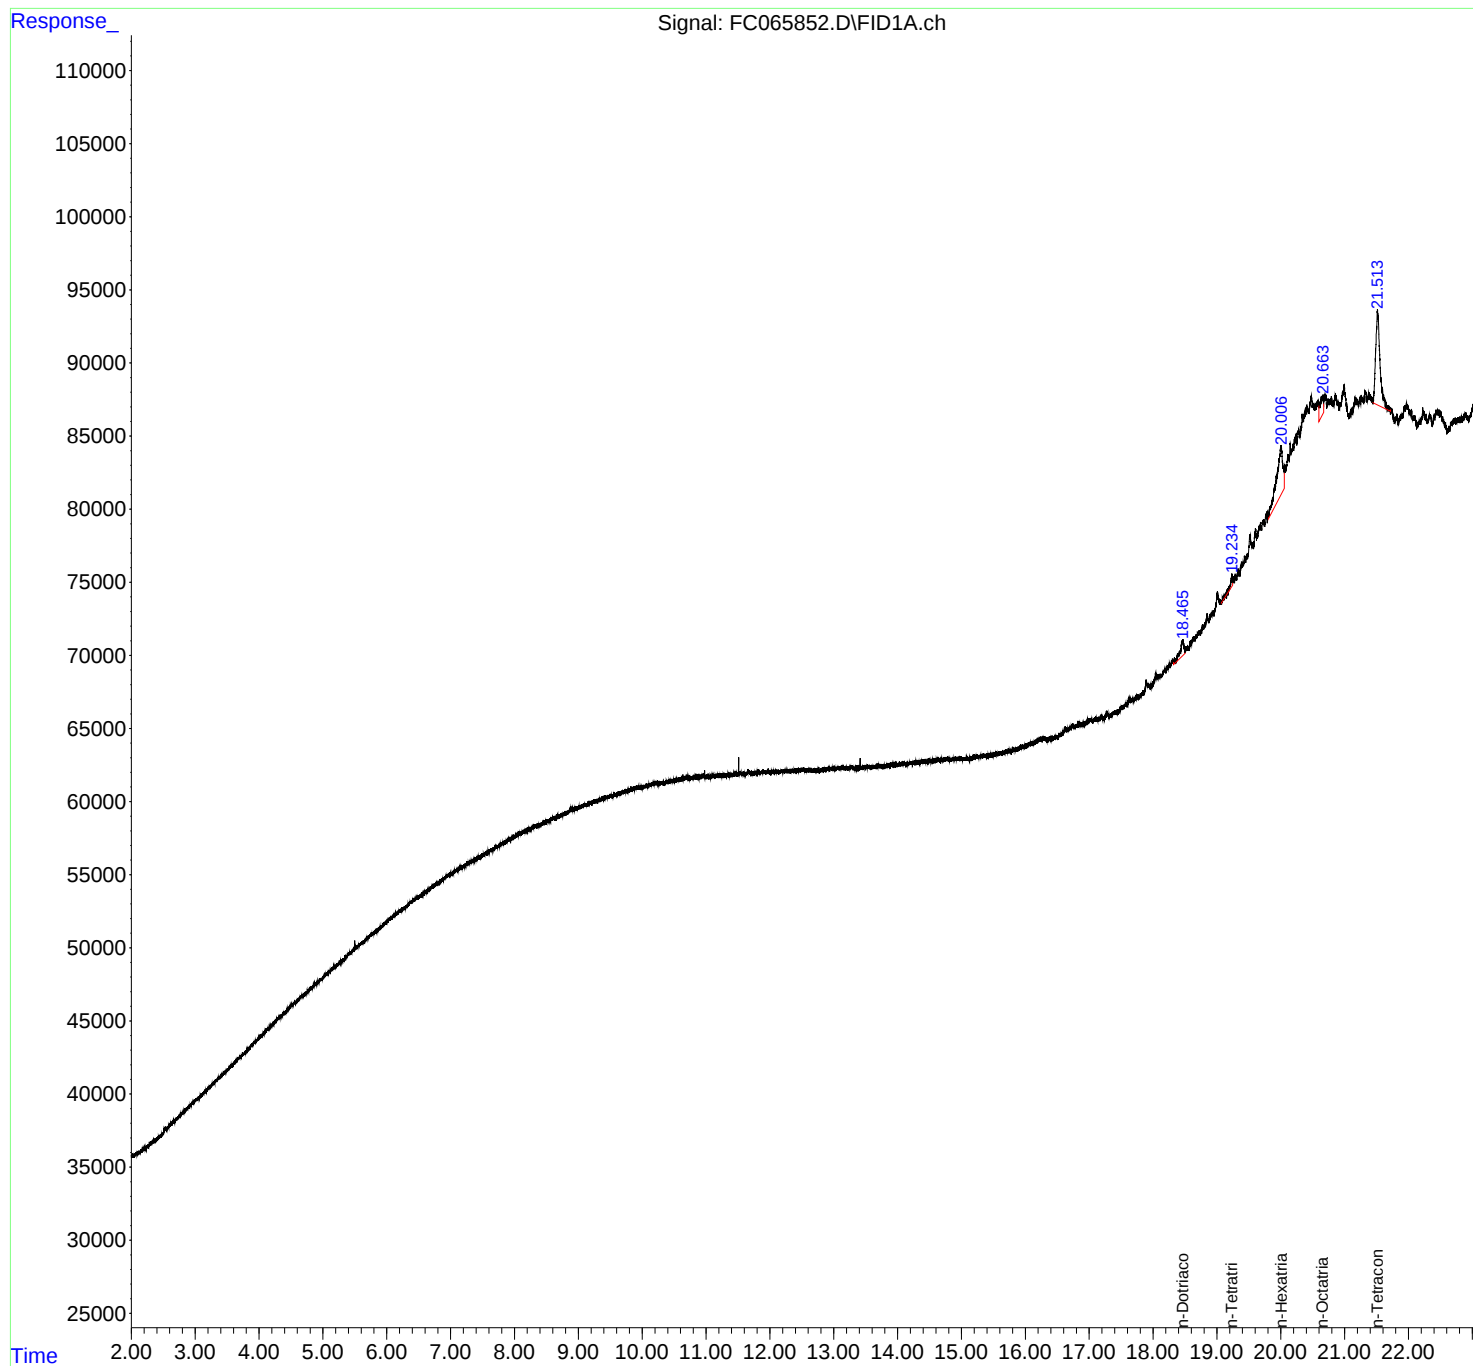


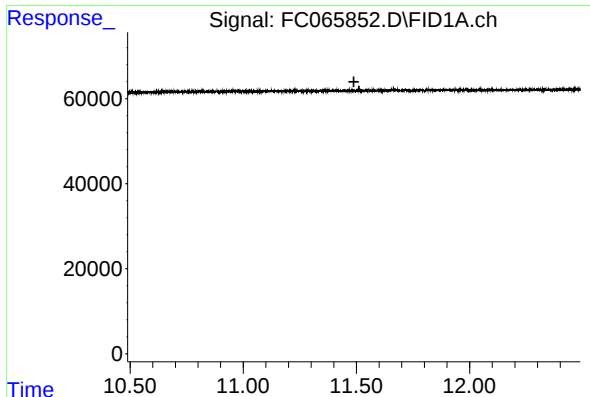

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

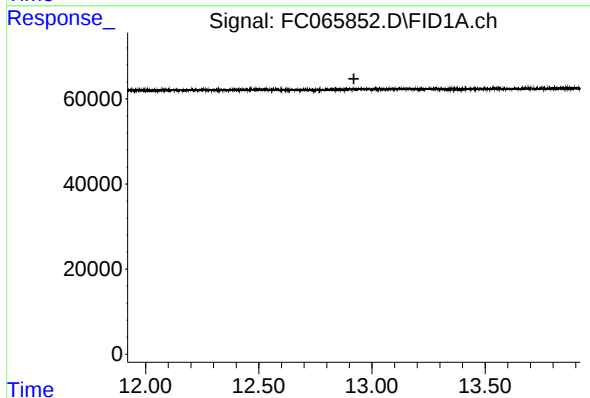


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.920 min
Response: 0
Conc: N.D.

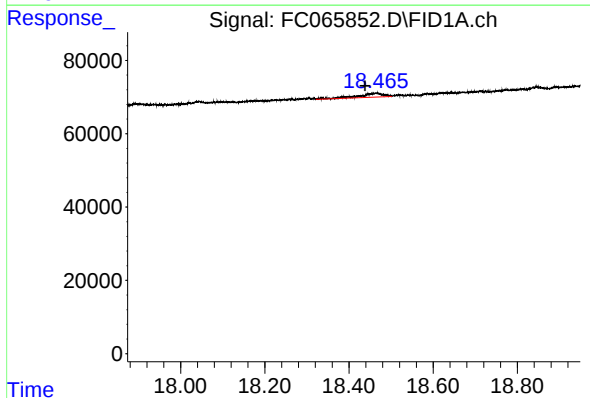


#18 n-Dotriacontane (C32)

R.T.: 18.464 min
Delta R.T.: 0.026 min
Response: 45600
Conc: 0.31 ug/ml

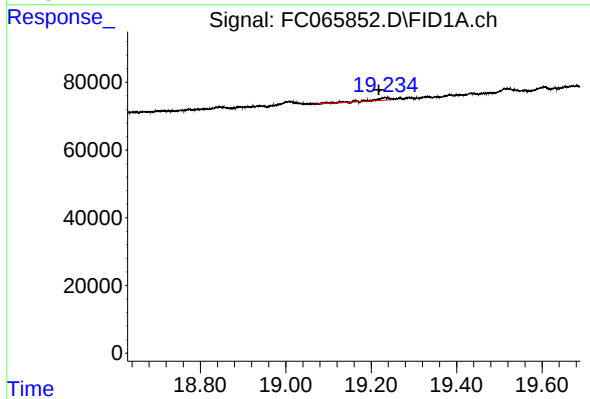

#19 n-Tetratriacontane (C34)


R.T.: 19.233 min
Delta R.T.: 0.015 min
Response: 19599
Conc: 0.14 ug/ml

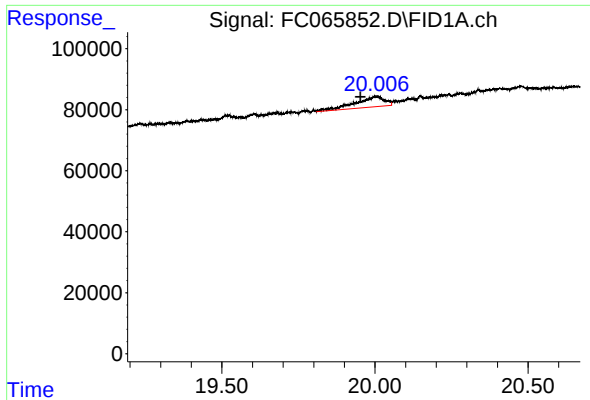

#20 n-Hexatriacontane (C36)


R.T.: 20.005 min
Delta R.T.: 0.052 min
Response: 229114
Conc: 1.61 ug/ml

Instrument :
FID_C
ClientSampleId :

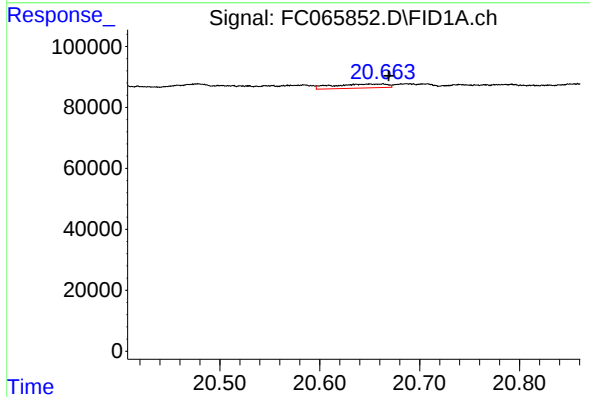

#21 n-Octatriacontane (C38)

R.T.: 20.651 min
Delta R.T.: -0.018 min
Response: 48845
Conc: 0.35 ug/ml

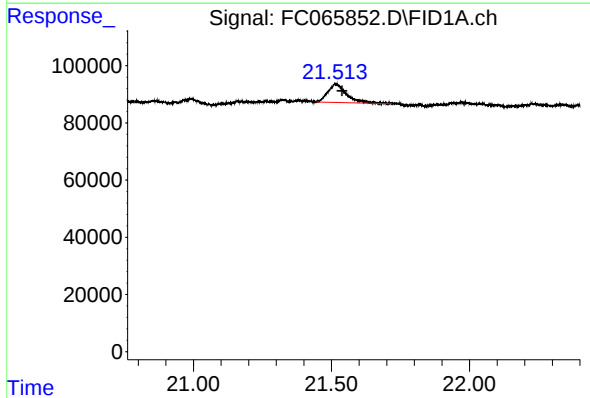

#22 n-Tetracontane (C40)

R.T.: 21.514 min
Delta R.T.: -0.025 min
Response: 306673
Conc: 2.20 ug/ml