

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC022724AL\
Data File : FC065882.D
Signal(s) : FID1A.ch
Acq On : 27 Feb 2024 09:02
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 28 01:06:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:26:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.450	28116	0.190 ug/ml
20) T	n-Hexatriacontane (C36)	19.965	4912	0.035 ug/ml
21) T	n-Octatriacontane (C38)	20.681	71628	0.506 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC022724AL\
Data File : FC065882.D
Signal(s) : FID1A.ch
Acq On : 27 Feb 2024 09:02
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 28 01:06:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:26:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

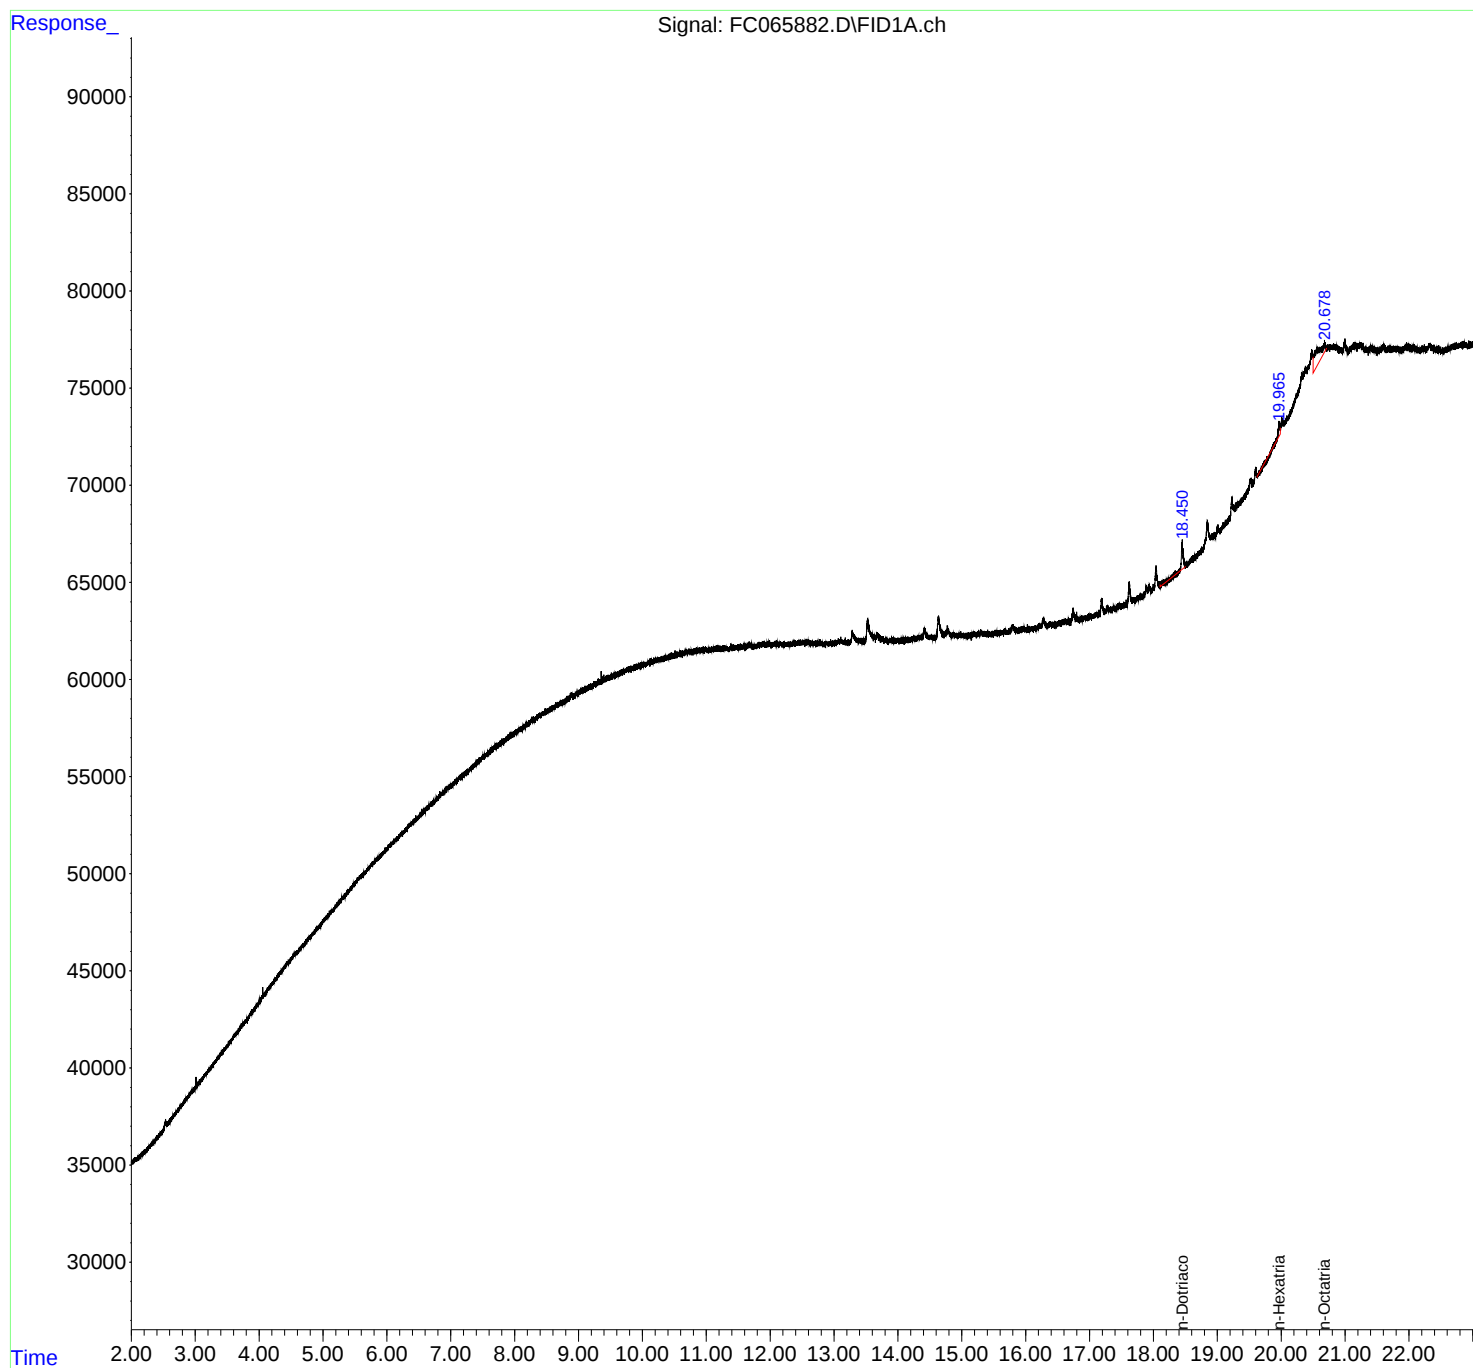


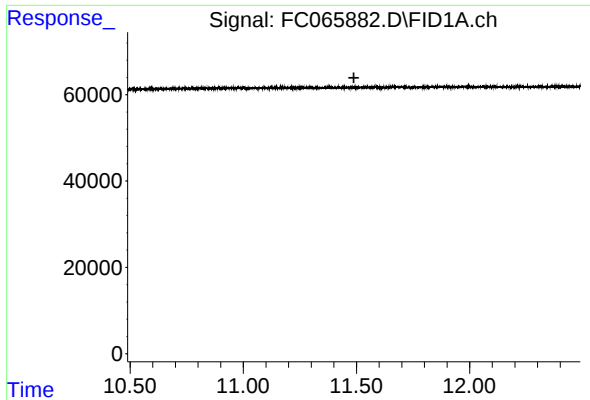

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

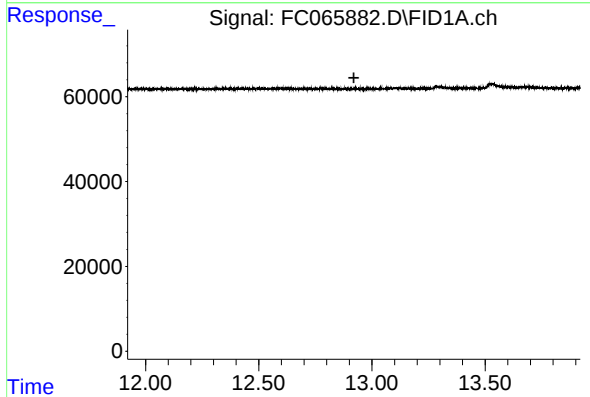


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.920 min
Response: 0
Conc: N.D.

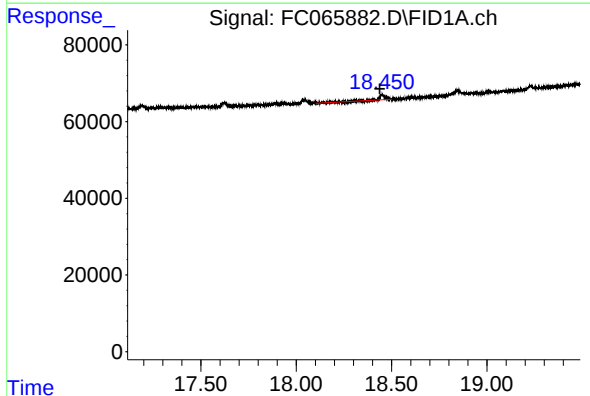


#18 n-Dotriacontane (C32)

R.T.: 18.450 min
Delta R.T.: 0.012 min
Response: 28116
Conc: 0.19 ug/ml

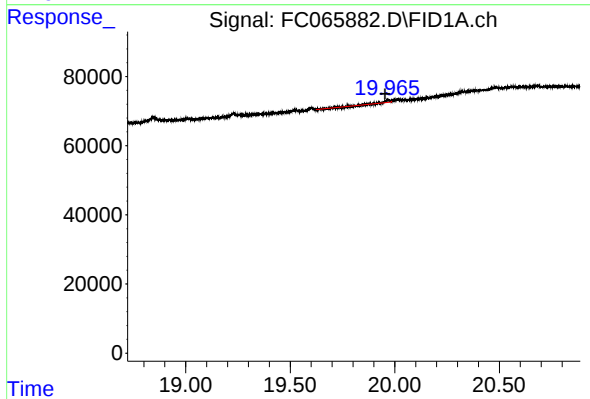

#20 n-Hexatriacontane (C36)

R.T.: 19.965 min
Delta R.T.: 0.012 min
Response: 4912
Conc: 0.03 ug/ml

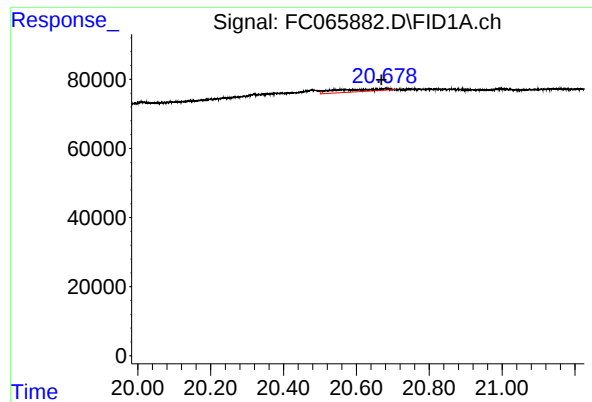

#21 n-Octatriacontane (C38)

R.T.: 20.681 min
Delta R.T.: 0.012 min
Response: 71628
Conc: 0.51 ug/ml

Instrument :

FID_C

ClientSampleId :