

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030119AL\
 Data File : FC039526.D
 Signal(s) : FID1A.CH
 Acq On : 01 Mar 2019 17:37
 Operator : AJ\SJ
 Sample : K1645-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 SR-10-2

Integration File: autoint1.e
 Quant Time: Mar 01 23:25:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 25 18:21:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.609	3811744	30.218 ug/ml
Spiked Amount 50.000		Recovery =	60.44%
Target Compounds			
15) T n-Hexacosane (C26)	15.471	136837	1.097 ug/ml
16) T n-Octacosane (C28)	16.415	245521	1.837 ug/ml
17) T n-Tricontane (C30)	17.298	224115	1.527 ug/ml
18) T n-Dotriacontane (C32)	18.127	125721	0.936 ug/ml
20) T n-Hexatriacontane (C36)	19.645	7259	0.075 ug/ml
21) T n-Octatriacontane (C38)	20.343	4234	0.046 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030119AL\
Data File : FC039526.D
Signal(s) : FID1A.CH
Acq On : 01 Mar 2019 17:37
Operator : AJ\SJ
Sample : K1645-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
SR-10-2

Integration File: autoint1.e
Quant Time: Mar 01 23:25:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
Quant Title : GC Extractables
QLast Update : Mon Feb 25 18:21:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

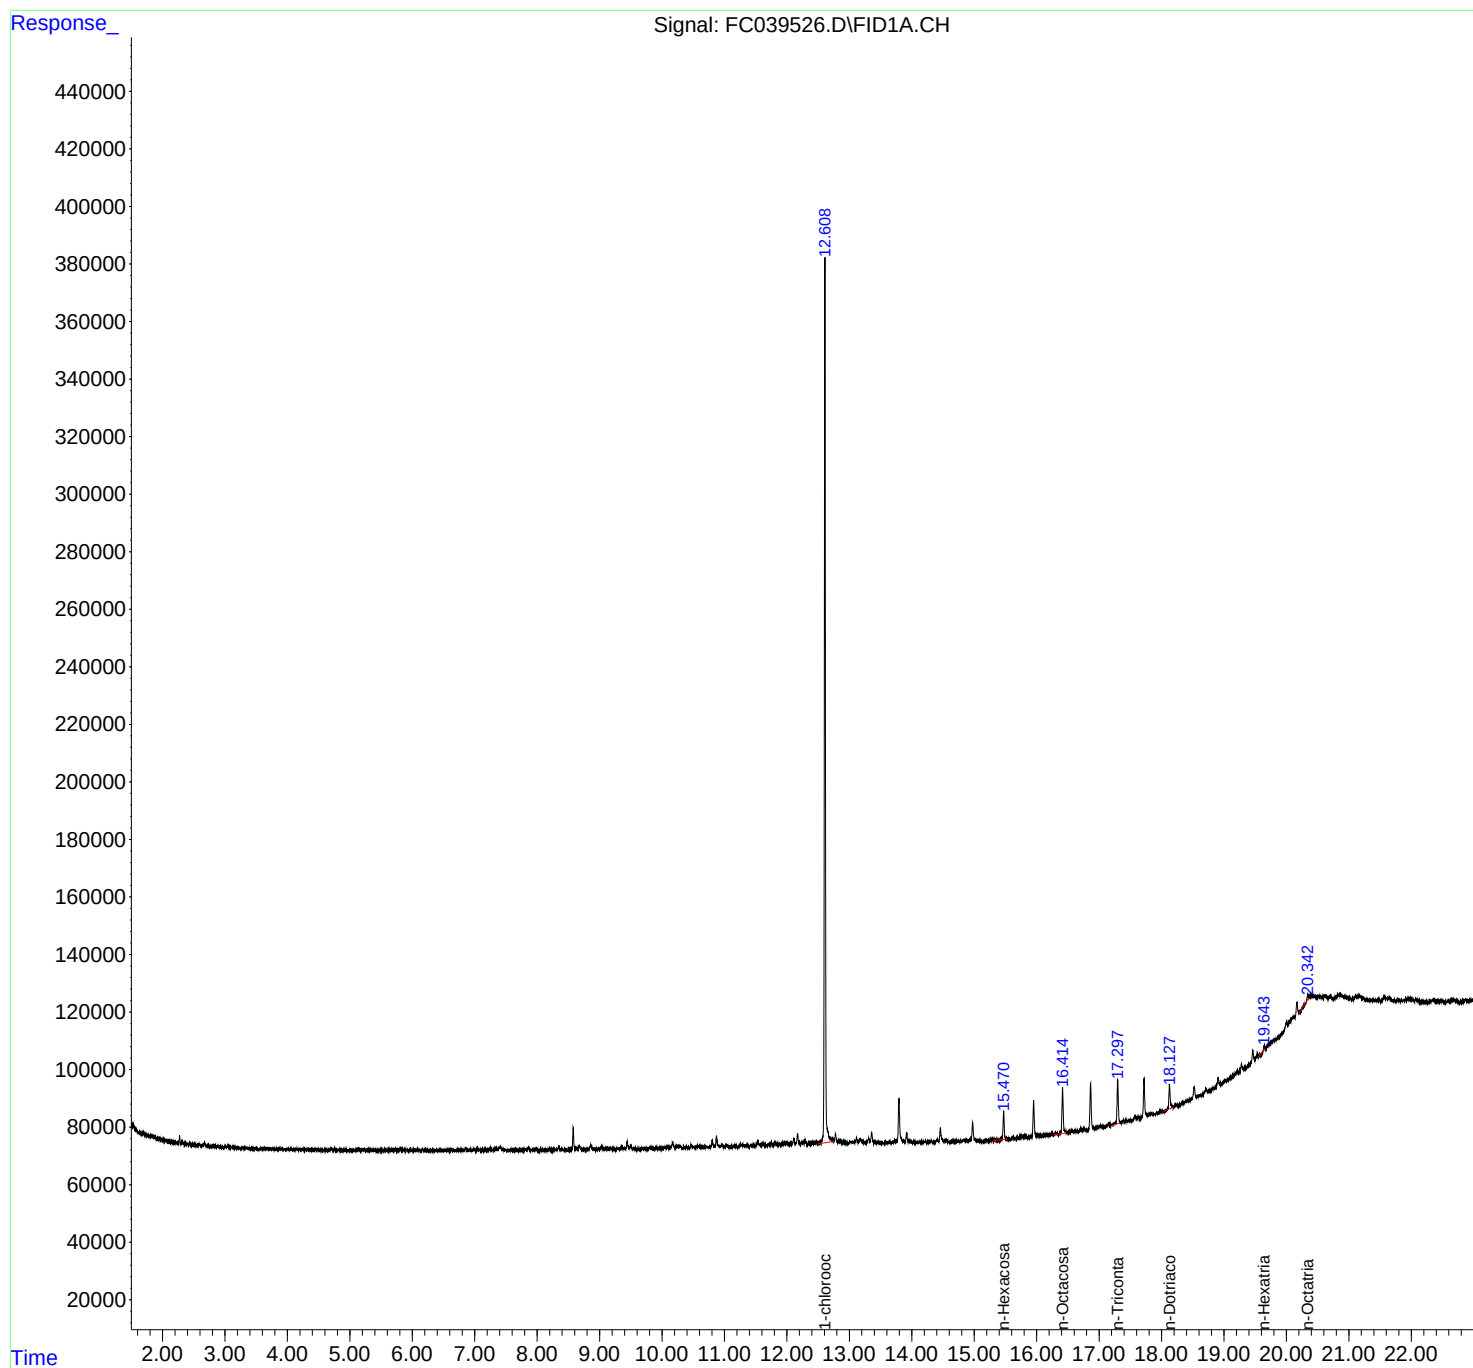


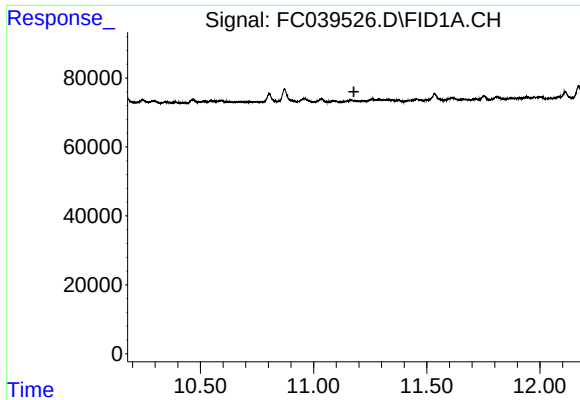

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.178 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
SR-10-2

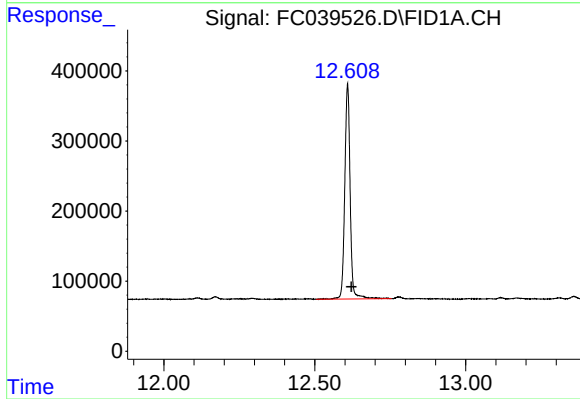


#12 1-chlorooctadecane (SURR)

R.T.: 12.609 min
Delta R.T.: -0.013 min
Response: 3811744
Conc: 30.22 ug/ml

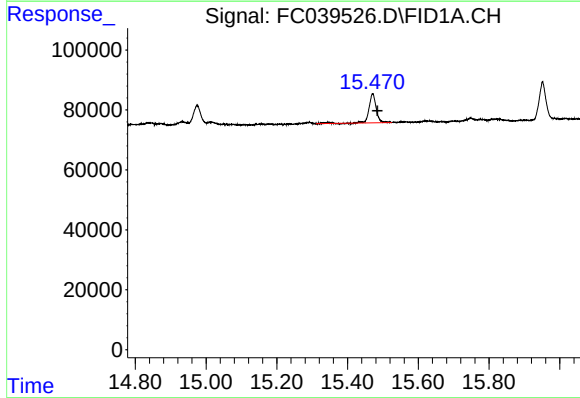


#15 n-Hexacosane (C26)

R.T.: 15.471 min
Delta R.T.: -0.014 min
Response: 136837
Conc: 1.10 ug/ml

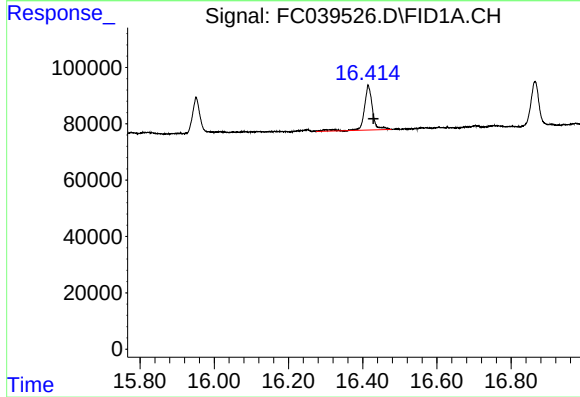

#16 n-Octacosane (C28)


R.T.: 16.415 min
Delta R.T.: -0.014 min
Response: 245521
Conc: 1.84 ug/ml

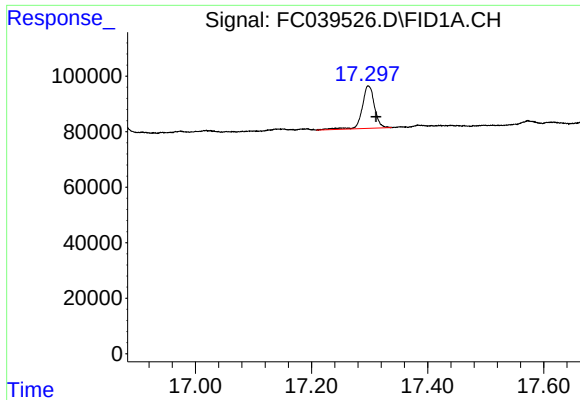

#17 n-Tricontane (C30)


R.T.: 17.298 min
Delta R.T.: -0.013 min
Response: 224115
Conc: 1.53 ug/ml

Instrument :
FID_C
ClientSampleId :
SR-10-2

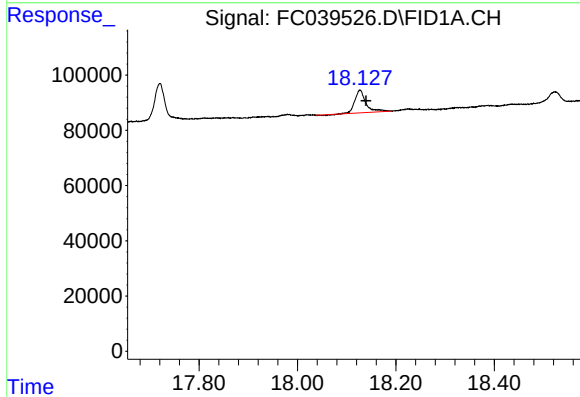


#18 n-Dotriacontane (C32)

R.T.: 18.127 min
Delta R.T.: -0.012 min
Response: 125721
Conc: 0.94 ug/ml

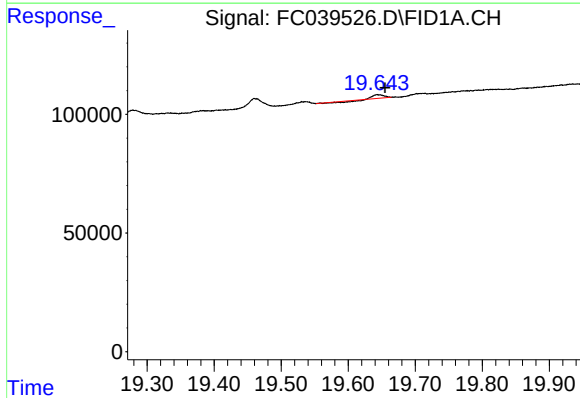

#20 n-Hexatriacontane (C36)

R.T.: 19.645 min
Delta R.T.: -0.010 min
Response: 7259
Conc: 0.08 ug/ml

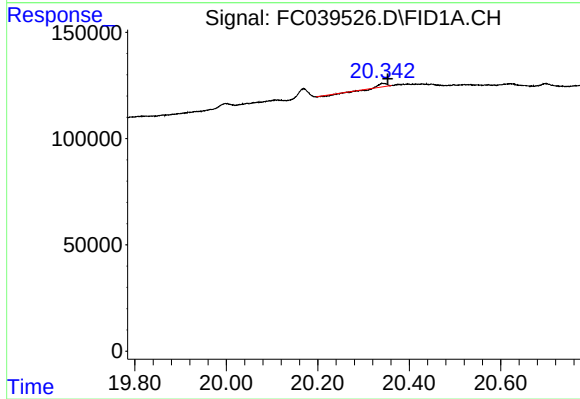

#21 n-Octatriacontane (C38)

R.T.: 20.343 min
Delta R.T.: -0.010 min
Response: 4234
Conc: 0.05 ug/ml