

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030322AL\
 Data File : FC058567.D
 Signal(s) : FID1A.CH
 Acq On : 03 Mar 2022 21:38
 Operator : UA/NP
 Sample : N1751-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 04 01:25:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 022322.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 23 17:15:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.393	3933592	27.007 ug/ml
Spiked Amount 50.000		Recovery =	54.01%
12) S 1-chlorooctadecane (S...	12.827	3017385	26.620 ug/ml
Spiked Amount 50.000		Recovery =	53.24%
Target Compounds			
10) T n-Eicosane (C20)	12.427	726742	5.527 ug/ml
14) T n-Tetracosane (C24)	14.630	224299	1.737 ug/ml
16) T n-Octacosane (C28)	16.626	109900	0.923 ug/ml
17) T n-Tricontane (C30)	17.512	85034	0.755 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030322AL\
Data File : FC058567.D
Signal(s) : FID1A.CH
Acq On : 03 Mar 2022 21:38
Operator : UA/NP
Sample : N1751-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 04 01:25:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 022322.M
Quant Title : GC Extractables
QLast Update : Wed Feb 23 17:15:11 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

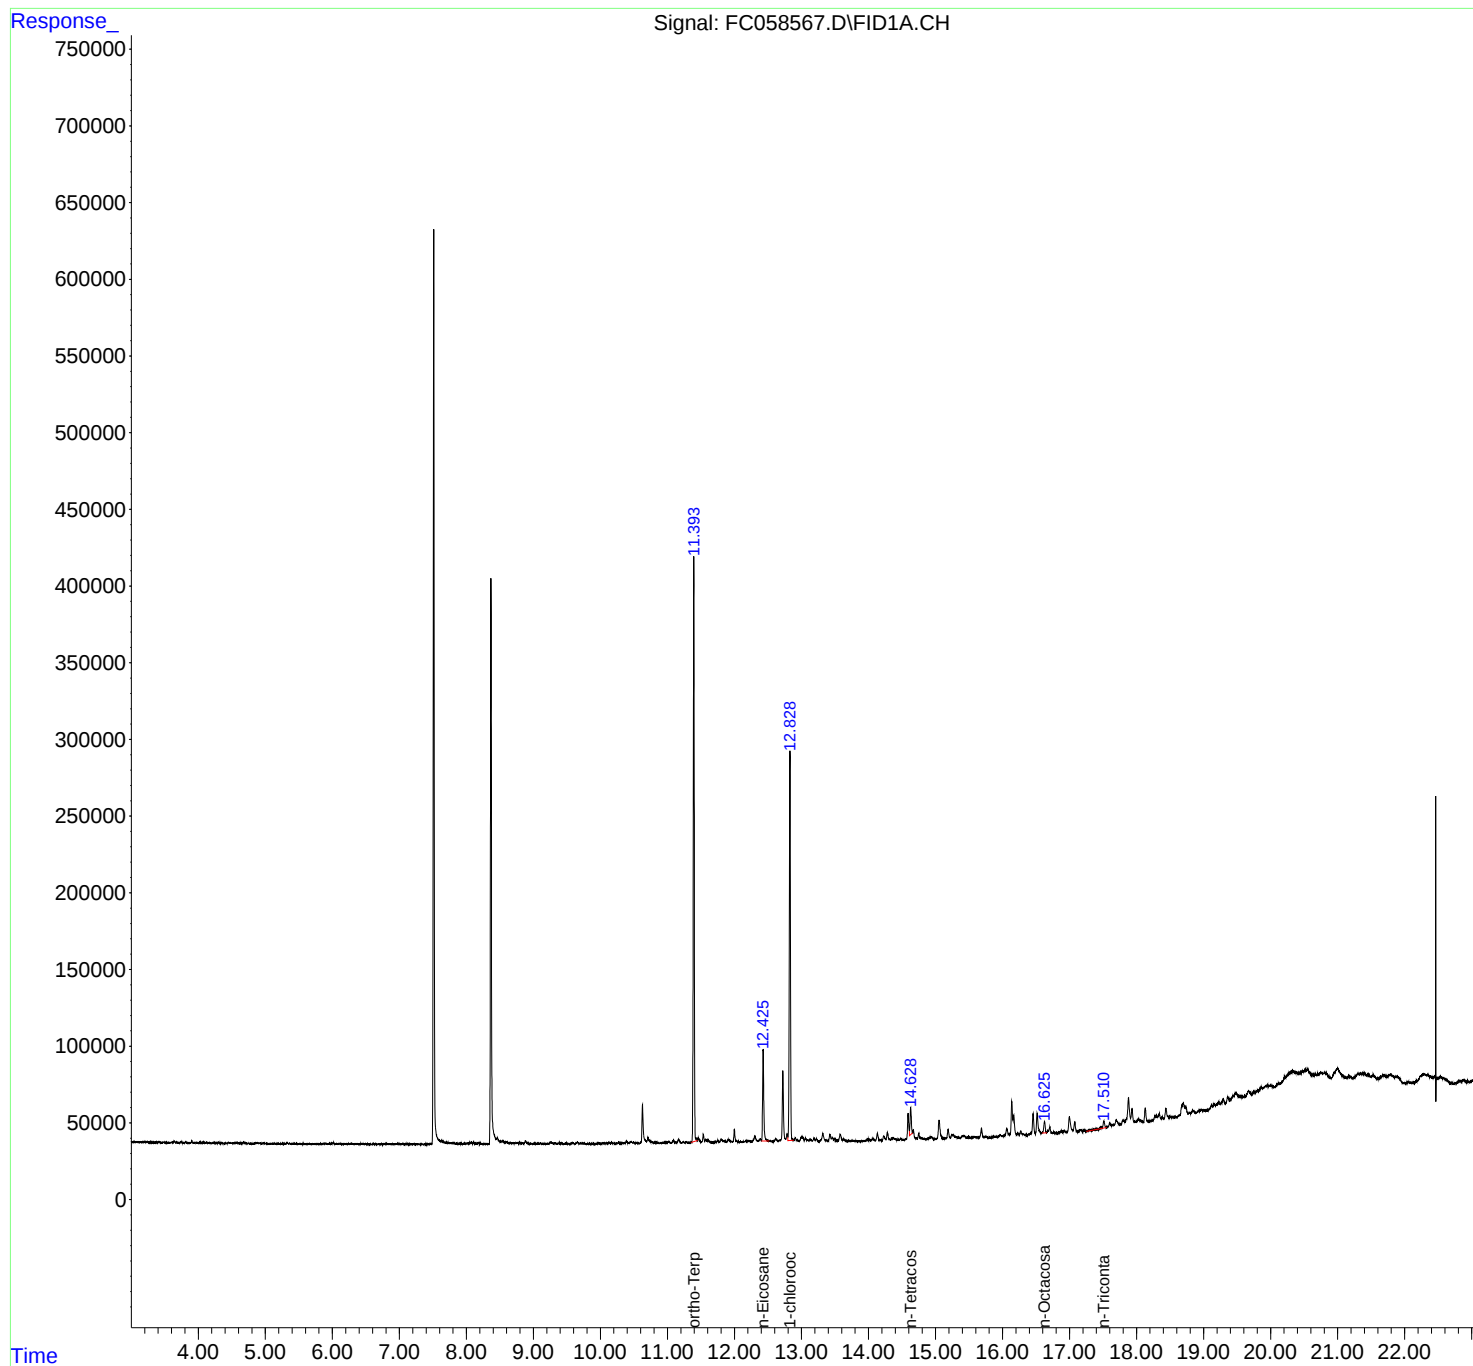


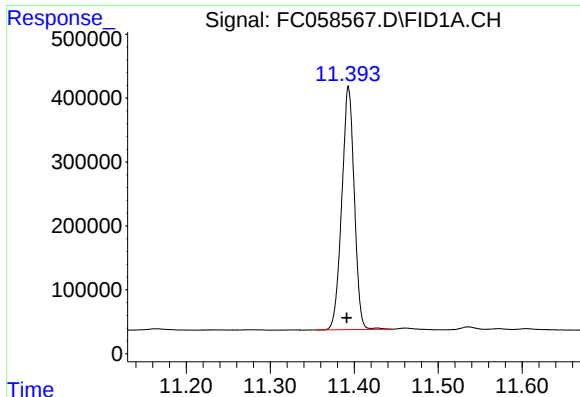

#9 ortho-Terphenyl (SURR)


R.T.: 11.393 min
Delta R.T.: 0.002 min
Response: 3933592
Conc: 27.01 ug/ml

Instrument :
FID_C
ClientSampleId :

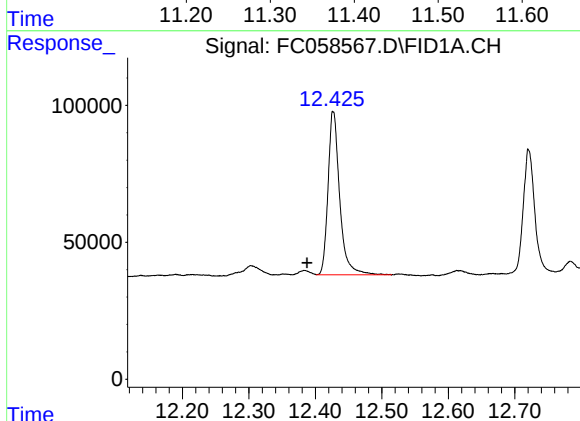


#10 n-Eicosane (C20)

R.T.: 12.427 min
Delta R.T.: 0.040 min
Response: 726742
Conc: 5.53 ug/ml

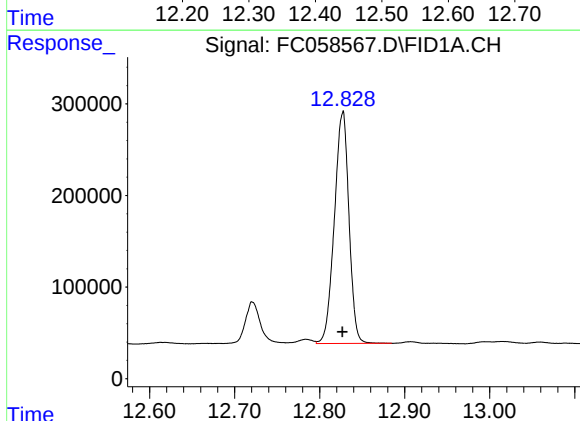


#12 1-chlorooctadecane (SURR)

R.T.: 12.827 min
Delta R.T.: 0.000 min
Response: 3017385
Conc: 26.62 ug/ml

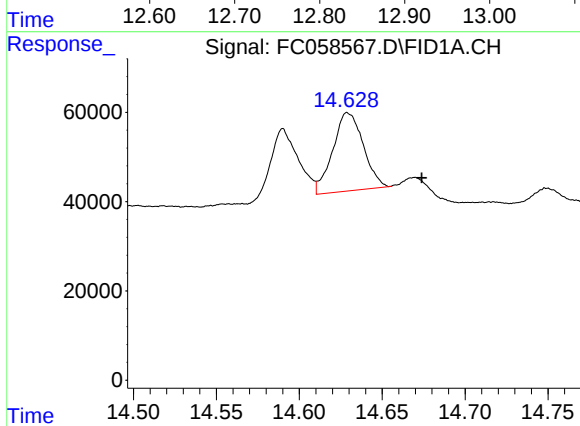

#14 n-Tetracosane (C24)

R.T.: 14.630 min
Delta R.T.: -0.044 min
Response: 224299
Conc: 1.74 ug/ml

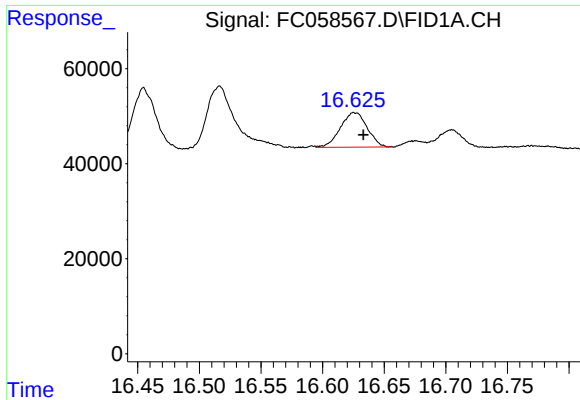

#16 n-Octacosane (C28)


R.T.: 16.626 min

Delta R.T.: -0.007 min

Response: 109900

Conc: 0.92 ug/ml

Instrument :
FID_C
ClientSampleId :

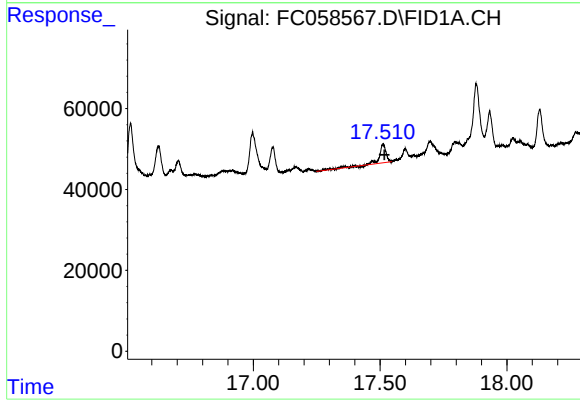

#17 n-Tricontane (C30)

R.T.: 17.512 min

Delta R.T.: -0.005 min

Response: 85034

Conc: 0.76 ug/ml