

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030519AL\
 Data File : FC039614.D
 Signal(s) : FID1A.CH
 Acq On : 05 Mar 2019 17:41
 Operator : AJ\SJ
 Sample : K1715-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-4-B-D2

Integration File: autoint1.e
 Quant Time: Mar 06 02:16:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 25 18:21:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.604	4215986	33.423 ug/ml
Spiked Amount 50.000		Recovery =	66.85%
Target Compounds			
16) T n-Octacosane (C28)	16.396	392100	2.934 ug/ml
17) T n-Tricontane (C30)	17.294	234308	1.597 ug/ml
18) T n-Dotriacontane (C32)	18.123	161483	1.202 ug/ml
19) T n-Tetratriacontane (C34)	18.904	386759	3.400 ug/ml
20) T n-Hexatriacontane (C36)	19.645	420761	4.363 ug/ml
21) T n-Octatriacontane (C38)	20.341	334048	3.638 ug/ml
22) T n-Tetracontane (C40)	21.102	252948	2.787 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030519AL\
Data File : FC039614.D
Signal(s) : FID1A.CH
Acq On : 05 Mar 2019 17:41
Operator : AJ\SJ
Sample : K1715-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
Client Sampled :
TP-4-B-D2

Integration File: autoint1.e
Quant Time: Mar 06 02:16:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 022219.M
Quant Title : GC Extractables
QLast Update : Mon Feb 25 18:21:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

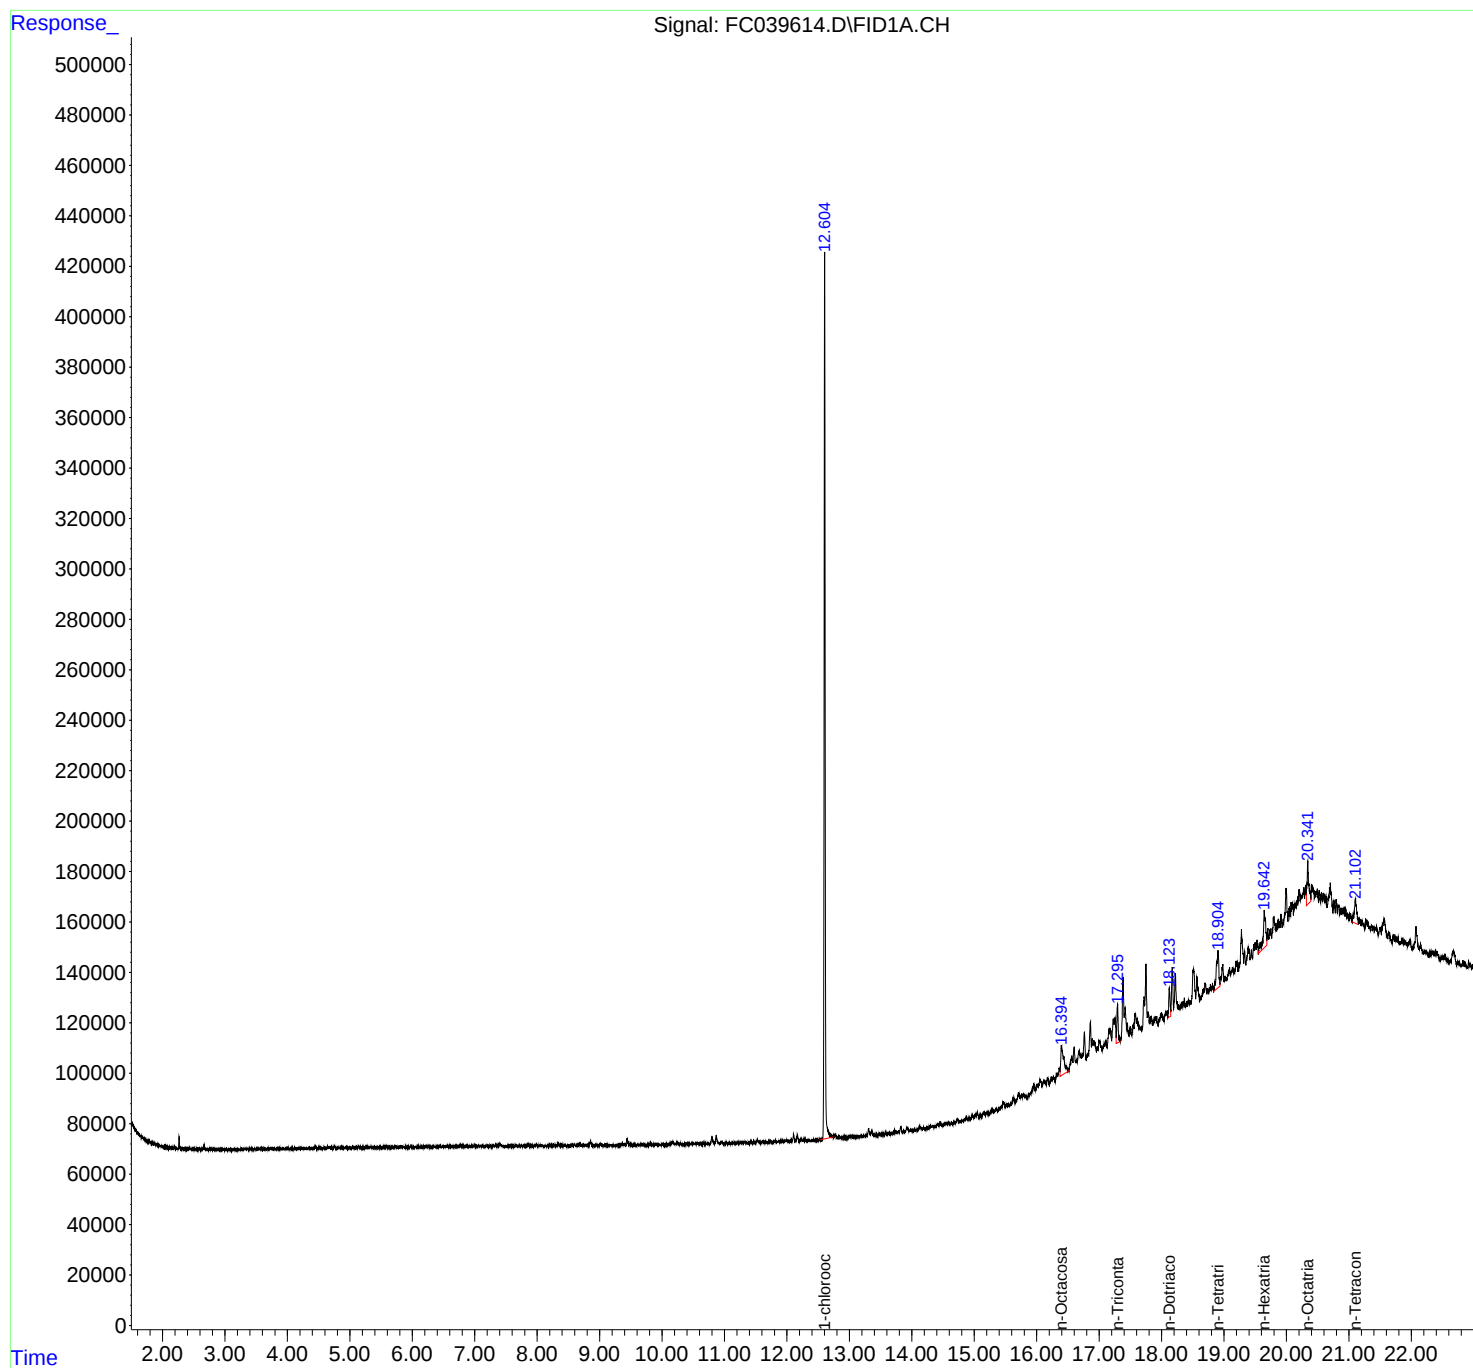


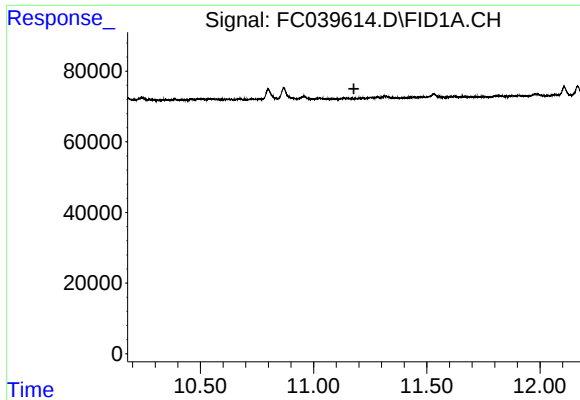

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.178 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
TP-4-B-D2

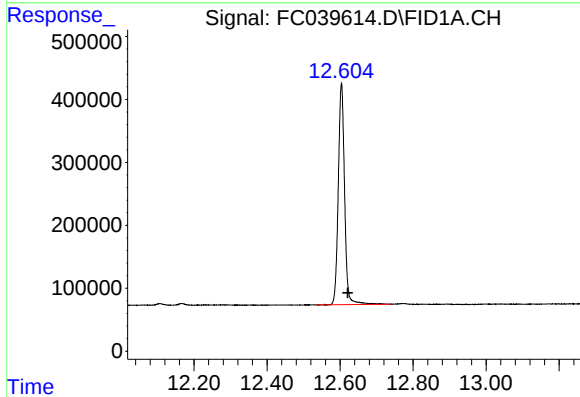


#12 1-chlorooctadecane (SURR)

R.T.: 12.604 min
Delta R.T.: -0.018 min
Response: 4215986
Conc: 33.42 ug/ml

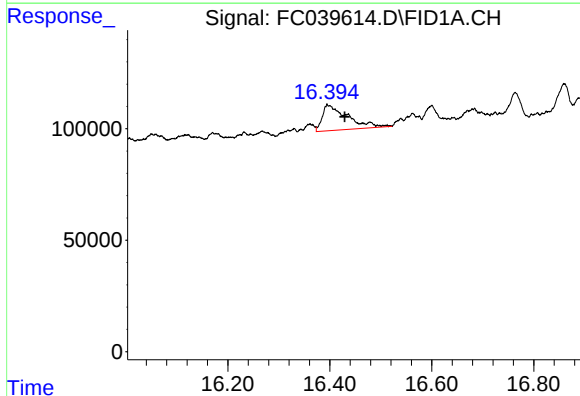


#16 n-Octacosane (C28)

R.T.: 16.396 min
Delta R.T.: -0.032 min
Response: 392100
Conc: 2.93 ug/ml

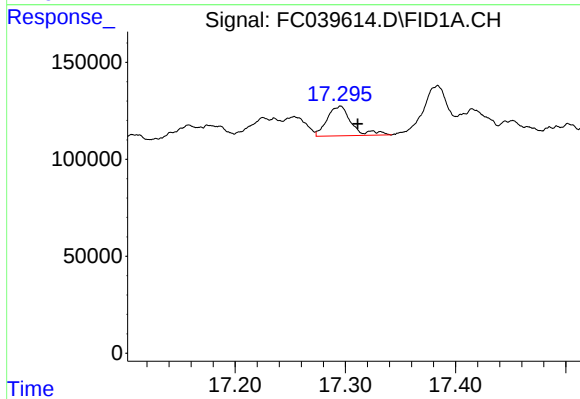

#17 n-Tricontane (C30)


R.T.: 17.294 min
Delta R.T.: -0.017 min
Response: 234308
Conc: 1.60 ug/ml

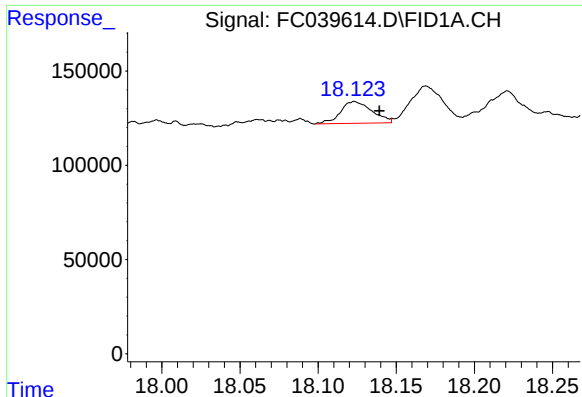

#18 n-Dotriacontane (C32)


R.T.: 18.123 min
Delta R.T.: -0.016 min
Response: 161483
Conc: 1.20 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-4-B-D2

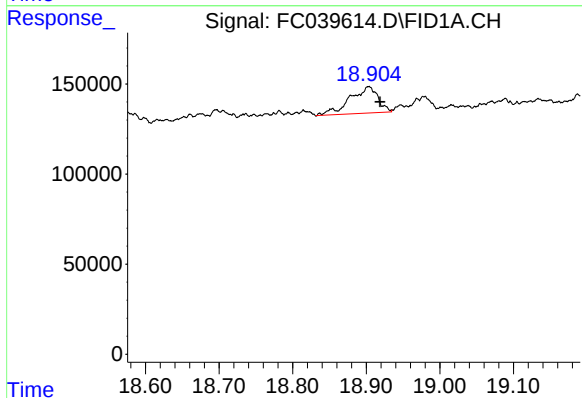


#19 n-Tetratriacontane (C34)

R.T.: 18.904 min
Delta R.T.: -0.015 min
Response: 386759
Conc: 3.40 ug/ml

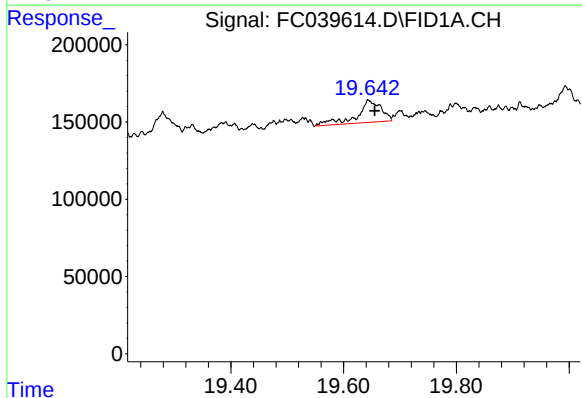


#20 n-Hexatriacontane (C36)

R.T.: 19.645 min
Delta R.T.: -0.010 min
Response: 420761
Conc: 4.36 ug/ml

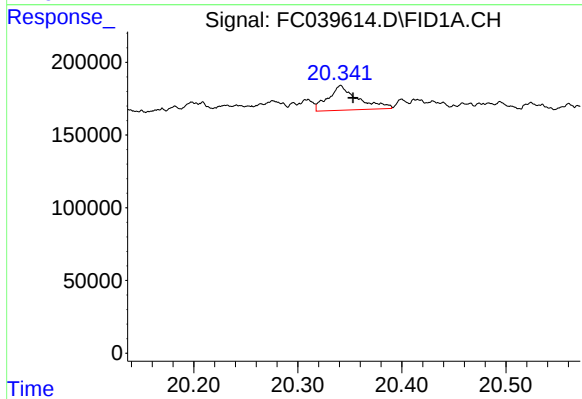

#21 n-Octatriacontane (C38)

R.T.: 20.341 min
Delta R.T.: -0.012 min
Response: 334048
Conc: 3.64 ug/ml

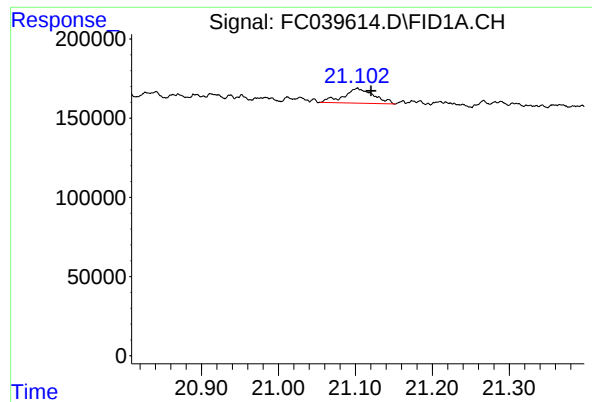

#22 n-Tetracontane (C40)

R.T.: 21.102 min
Delta R.T.: -0.018 min
Response: 252948
Conc: 2.79 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-4-B-D2