

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030821AL\
 Data File : FC052315.D
 Signal(s) : FID1A.CH
 Acq On : 09 Mar 2021 1:26
 Operator : DD\AJ
 Sample : M1582-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 03:00:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 04 03:56:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.611	3988181	30.242 ug/ml
Spiked Amount 50.000		Recovery =	60.48%
12) S 1-chlorooctadecane (S...	13.049	3496760	33.623 ug/ml
Spiked Amount 50.000		Recovery =	67.25%
Target Compounds			
10) T n-Eicosane (C20)	12.661f	420692	3.414 ug/ml
14) T n-Tetracosane (C24)	14.881	235282	2.018 ug/ml
16) T n-Octacosane (C28)	16.936	243272	2.373 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030821AL\
Data File : FC052315.D
Signal(s) : FID1A.CH
Acq On : 09 Mar 2021 1:26
Operator : DD\AJ
Sample : M1582-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 03:00:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
Quant Title : GC Extractables
QLast Update : Thu Mar 04 03:56:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

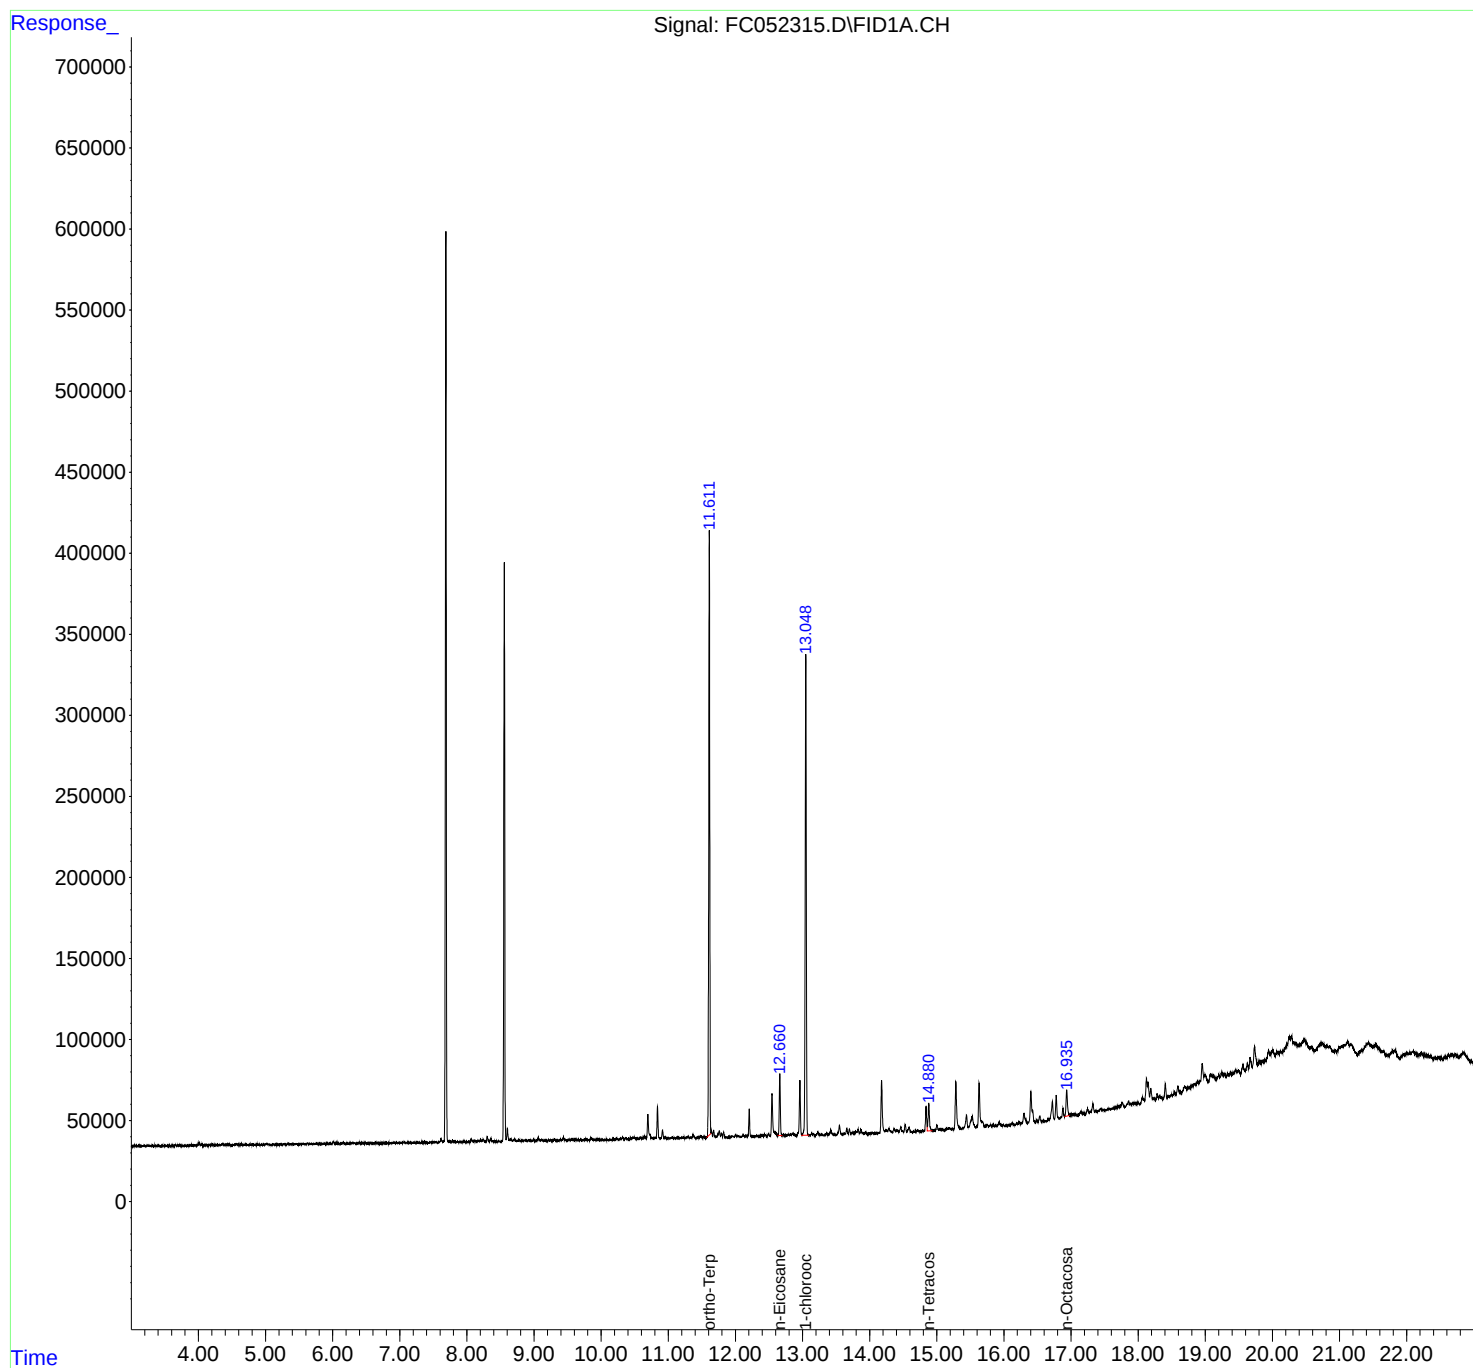


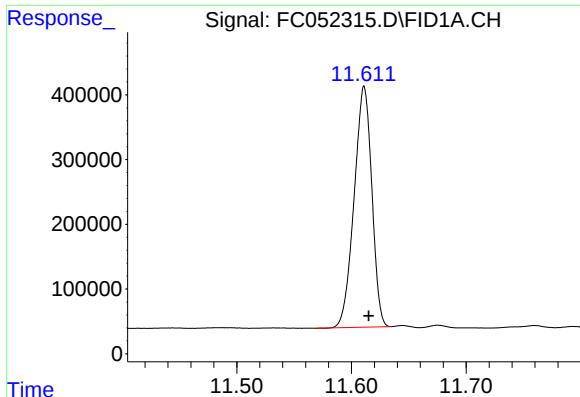

#9 ortho-Terphenyl (SURR)


R.T.: 11.611 min
Delta R.T.: -0.004 min
Response: 3988181
Conc: 30.24 ug/ml

Instrument :
FID_C
ClientSampleId :

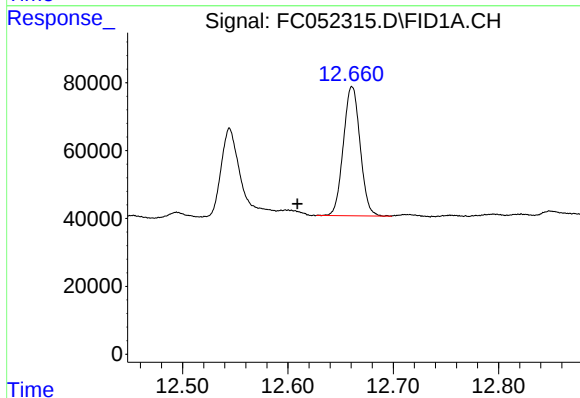


#10 n-Eicosane (C20)

R.T.: 12.661 min
Delta R.T.: 0.052 min
Response: 420692
Conc: 3.41 ug/ml

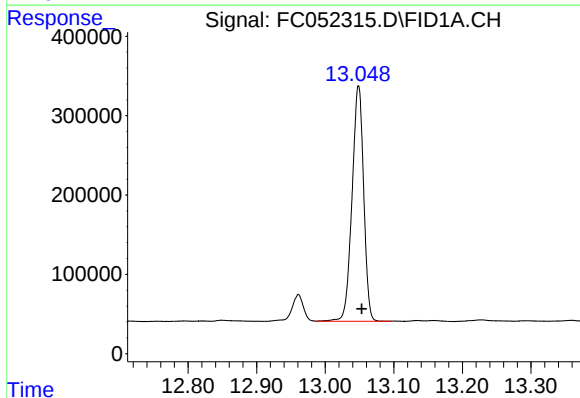


#12 1-chlorooctadecane (SURR)

R.T.: 13.049 min
Delta R.T.: -0.005 min
Response: 3496760
Conc: 33.62 ug/ml

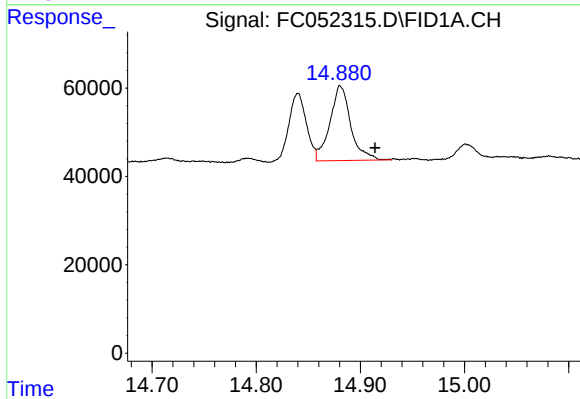

#14 n-Tetracosane (C24)

R.T.: 14.881 min
Delta R.T.: -0.033 min
Response: 235282
Conc: 2.02 ug/ml

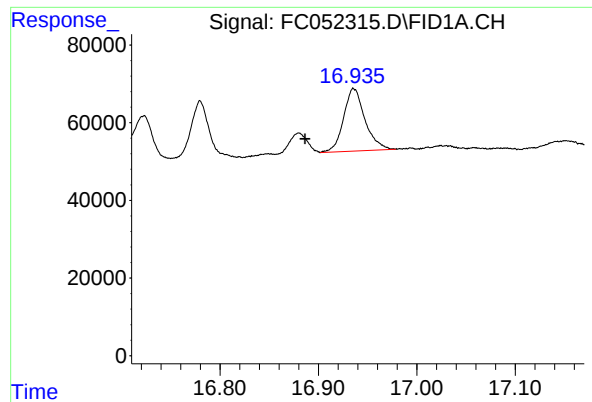

#16 n-Octacosane (C28)

R.T.: 16.936 min
Delta R.T.: 0.049 min
Response: 243272
Conc: 2.37 ug/ml

Instrument :
FID_C
ClientSampleId :