

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030922AL\
 Data File : FC058655.D
 Signal(s) : FID1A.CH
 Acq On : 10 Mar 2022 1:11
 Operator : UA/NP
 Sample : N1830-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 10 01:46:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 022322.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 23 17:15:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.396	4763452	32.704 ug/ml
Spiked Amount 50.000		Recovery =	65.41%
12) S 1-chlorooctadecane (S...	12.828	3664674	32.330 ug/ml
Spiked Amount 50.000		Recovery =	64.66%
Target Compounds			
10) T n-Eicosane (C20)	12.432	930414	7.076 ug/ml
14) T n-Tetracosane (C24)	14.637	428454	3.318 ug/ml
16) T n-Octacosane (C28)	16.633	86768	0.729 ug/ml
19) T n-Tetratriacontane (C34)	19.124	111187	1.148 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC030922AL\
Data File : FC058655.D
Signal(s) : FID1A.CH
Acq On : 10 Mar 2022 1:11
Operator : UA/NP
Sample : N1830-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 01:46:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 022322.M
Quant Title : GC Extractables
QLast Update : Wed Feb 23 17:15:11 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

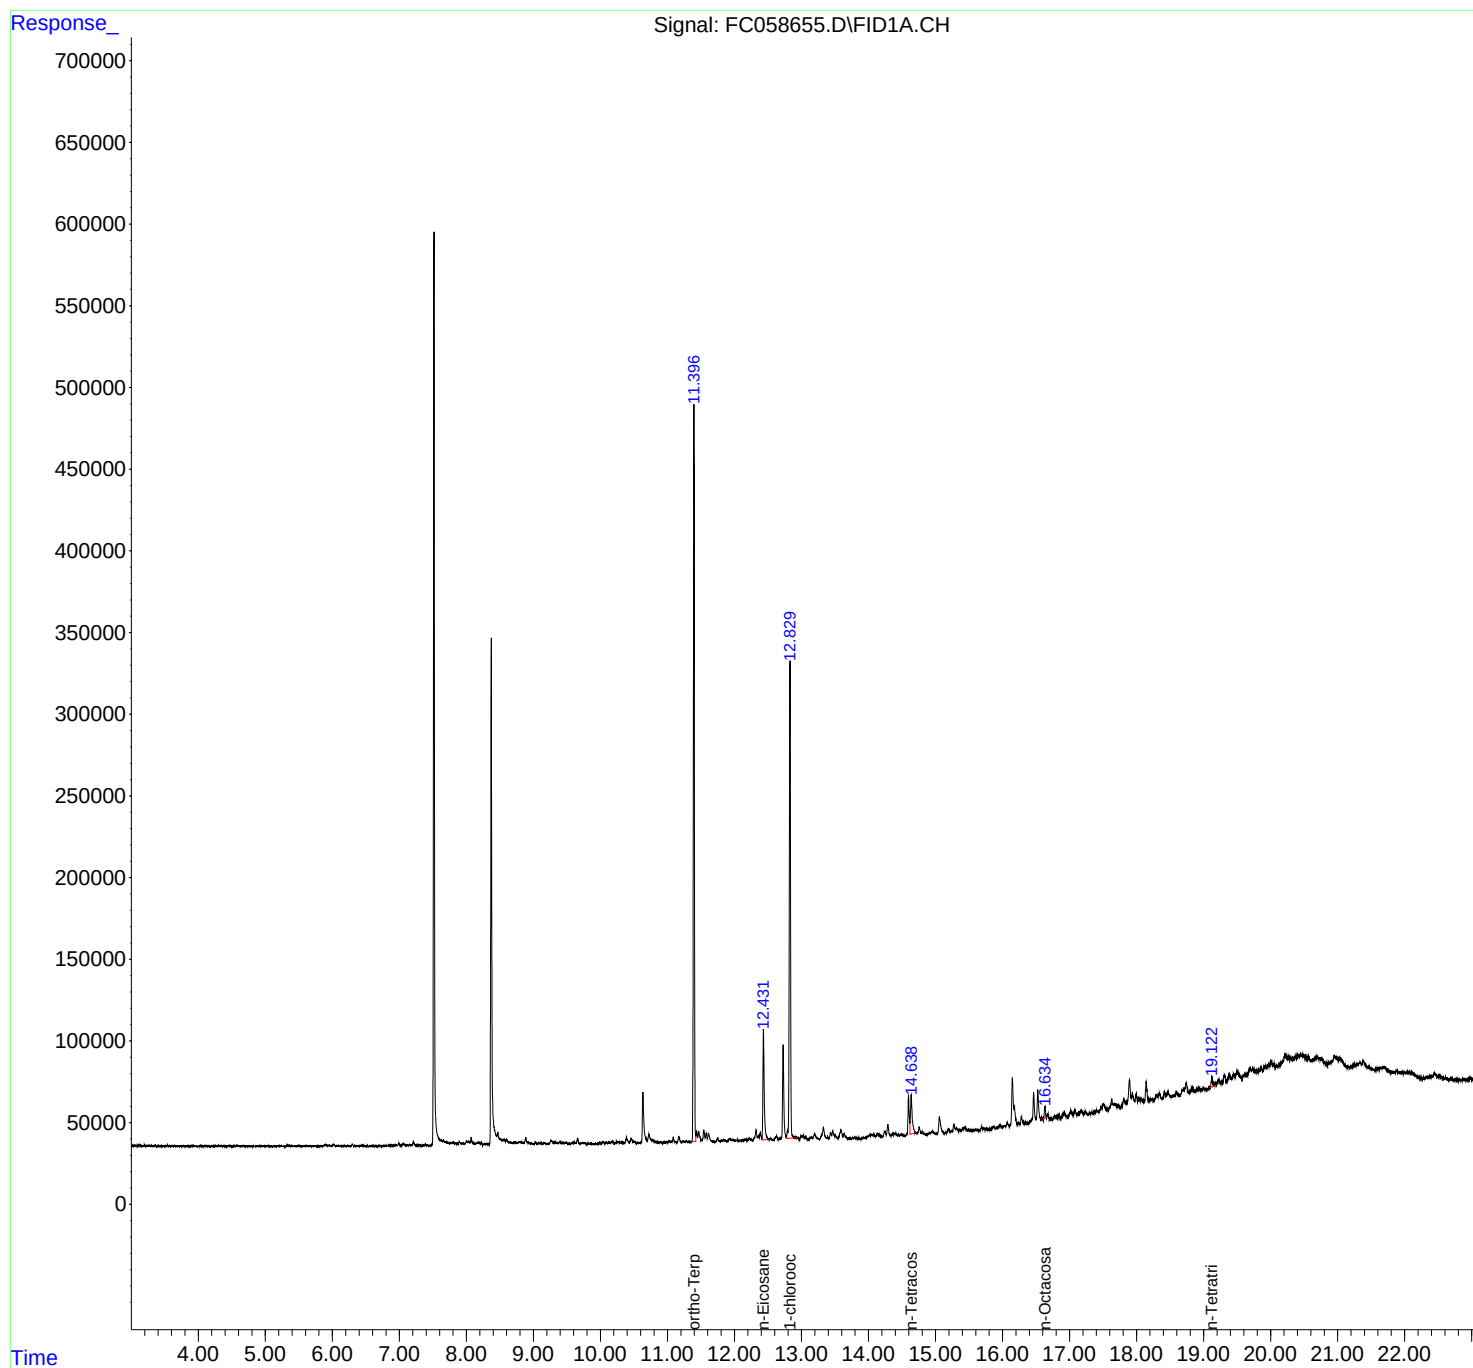


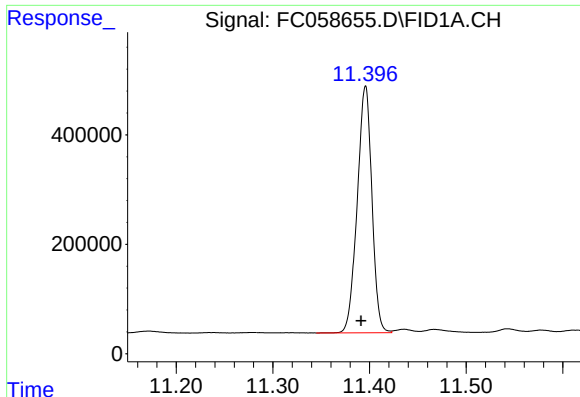

#9 ortho-Terphenyl (SURR)


R.T.: 11.396 min
Delta R.T.: 0.005 min
Response: 4763452
Conc: 32.70 ug/ml

Instrument :
FID_C
ClientSampleId :

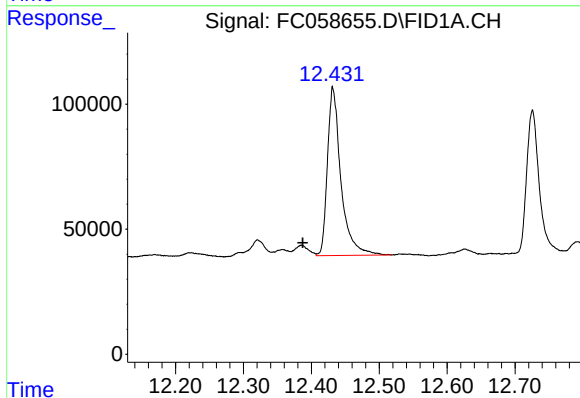


#10 n-Eicosane (C20)

R.T.: 12.432 min
Delta R.T.: 0.045 min
Response: 930414
Conc: 7.08 ug/ml

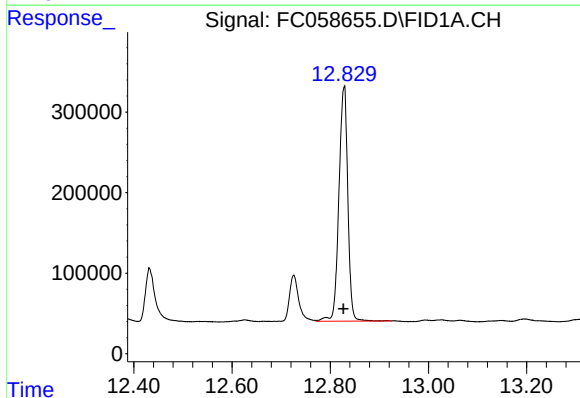


#12 1-chlorooctadecane (SURR)

R.T.: 12.828 min
Delta R.T.: 0.000 min
Response: 3664674
Conc: 32.33 ug/ml

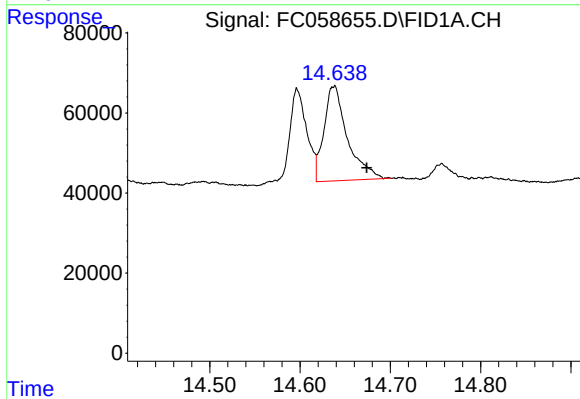

#14 n-Tetracosane (C24)


R.T.: 14.637 min
Delta R.T.: -0.036 min
Response: 428454
Conc: 3.32 ug/ml

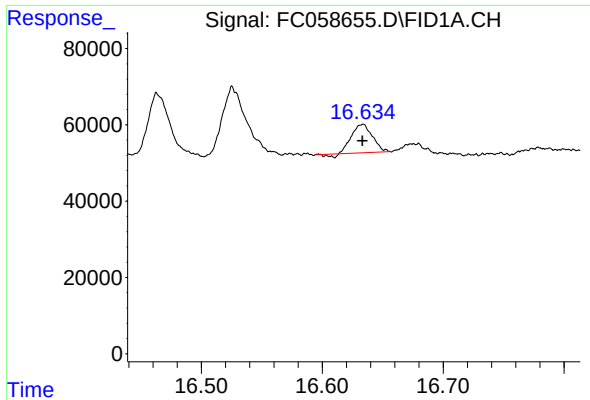

#16 n-Octacosane (C28)

R.T.: 16.633 min
Delta R.T.: 0.000 min
Response: 86768
Conc: 0.73 ug/ml

Instrument :
FID_C
ClientSampleId :

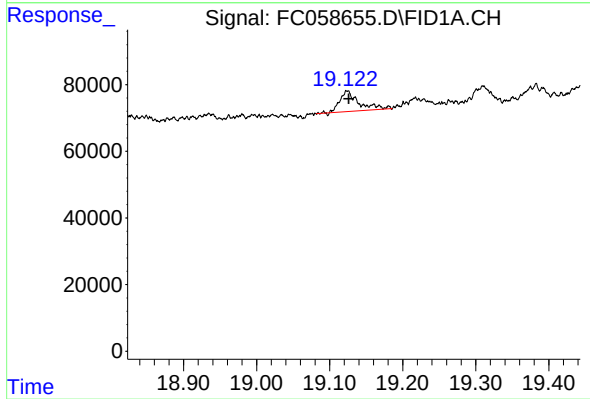

#19 n-Tetratriacontane (C34)

R.T.: 19.124 min
Delta R.T.: -0.002 min
Response: 111187
Conc: 1.15 ug/ml