

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031219AL\
 Data File : FC039780.D
 Signal(s) : FID1A.CH
 Acq On : 13 Mar 2019 3:15
 Operator : AJ\SJ
 Sample : K1807-09RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-5RE

Integration File: autoint1.e
 Quant Time: Mar 13 04:03:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 25 18:21:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.145	2757837	16.396 ug/ml
Spiked Amount 50.000		Recovery =	32.79%
12) S 1-chlorooctadecane (S...	12.591	2130111	16.887 ug/ml
Spiked Amount 50.000		Recovery =	33.77%
Target Compounds			
17) T n-Tricontane (C30)	17.279	109168	0.744 ug/ml
18) T n-Dotriacontane (C32)	18.107	104843	0.780 ug/ml
20) T n-Hexatriacontane (C36)	19.621	26269	0.272 ug/ml
21) T n-Octatriacontane (C38)	20.321	310034	3.377 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031219AL\
Data File : FC039780.D
Signal(s) : FID1A.CH
Acq On : 13 Mar 2019 3:15
Operator : AJ\SJ
Sample : K1807-09RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
TP-5RE

Integration File: autoint1.e
Quant Time: Mar 13 04:03:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
Quant Title : GC Extractables
QLast Update : Mon Feb 25 18:21:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

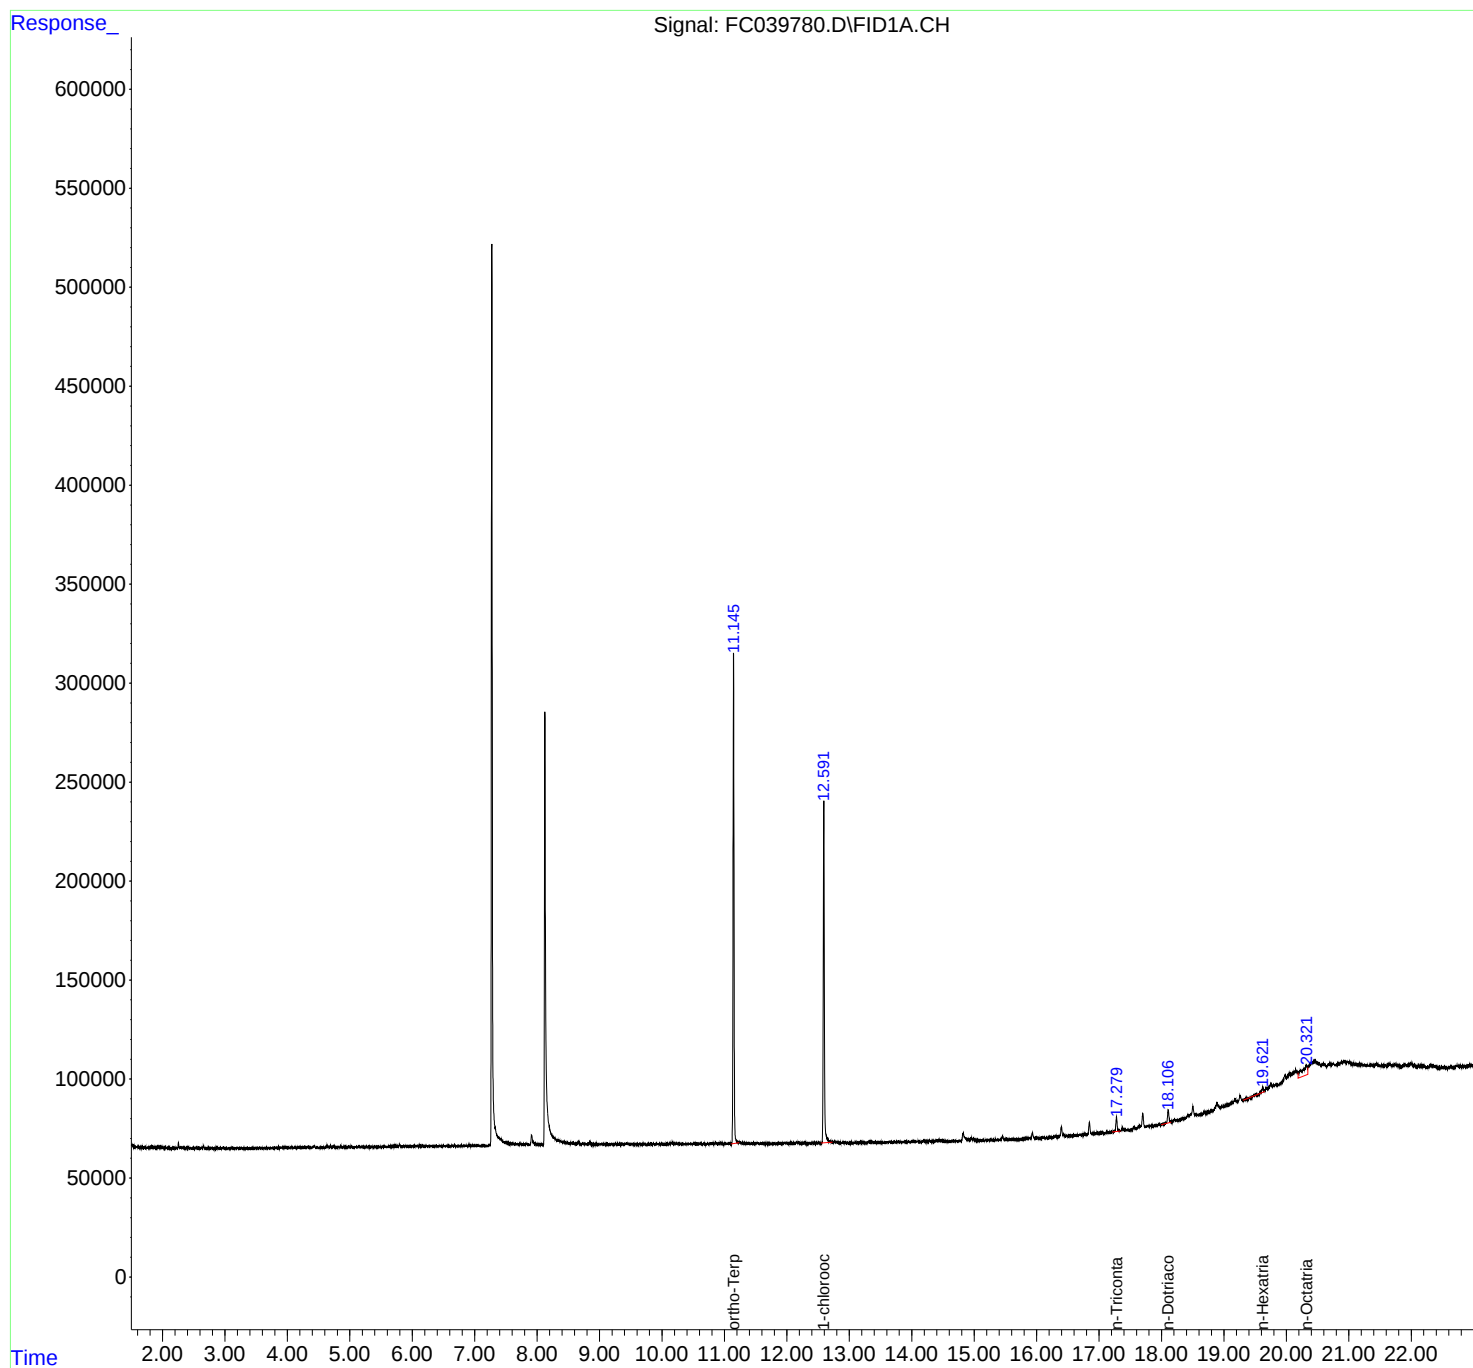


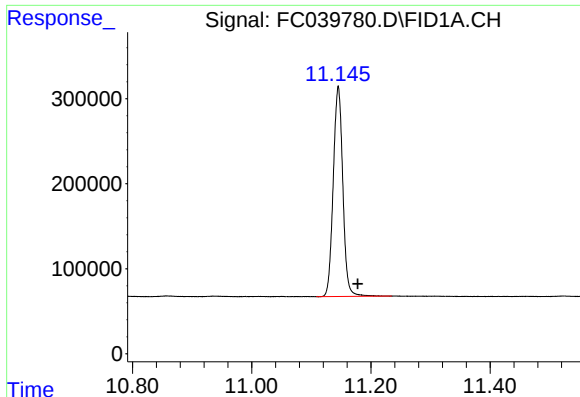

#9 ortho-Terphenyl (SURR)


R.T.: 11.145 min
Delta R.T.: -0.033 min
Response: 2757837
Conc: 16.40 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-5RE

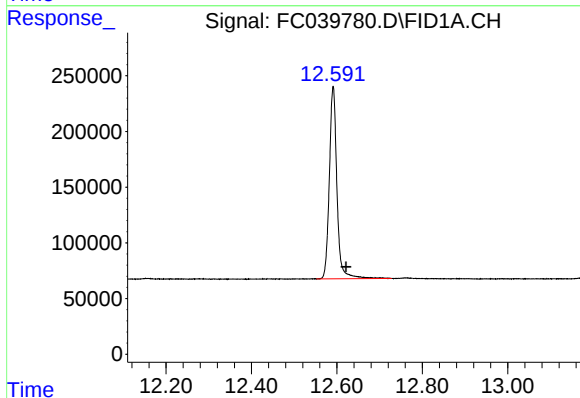


#12 1-chlorooctadecane (SURR)

R.T.: 12.591 min
Delta R.T.: -0.030 min
Response: 2130111
Conc: 16.89 ug/ml

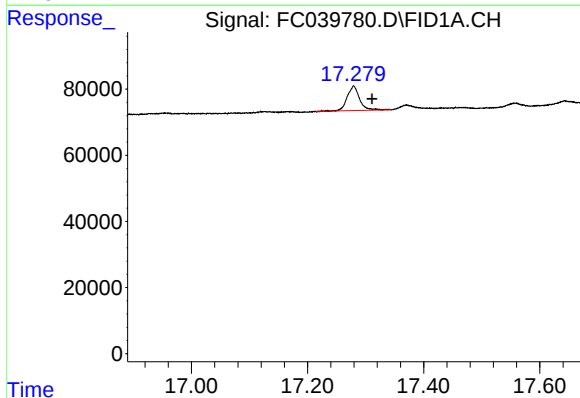


#17 n-Tricontane (C30)

R.T.: 17.279 min
Delta R.T.: -0.032 min
Response: 109168
Conc: 0.74 ug/ml

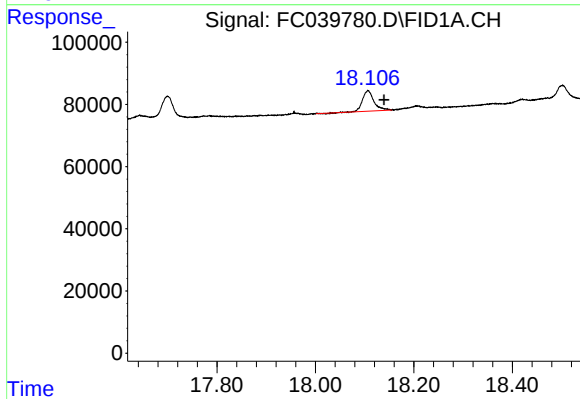

#18 n-Dotriacontane (C32)


R.T.: 18.107 min
Delta R.T.: -0.032 min
Response: 104843
Conc: 0.78 ug/ml

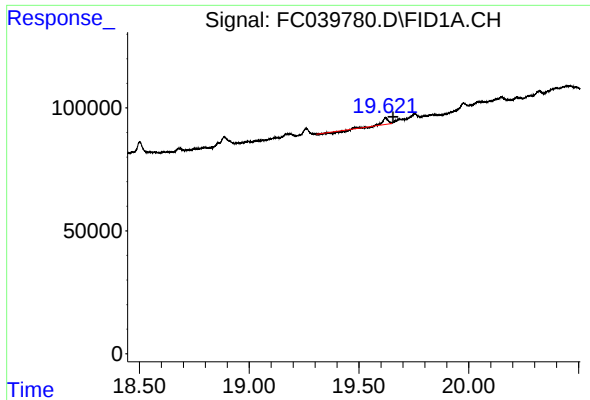

#20 n-Hexatriacontane (C36)

R.T.: 19.621 min
Delta R.T.: -0.034 min
Response: 26269
Conc: 0.27 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-5RE

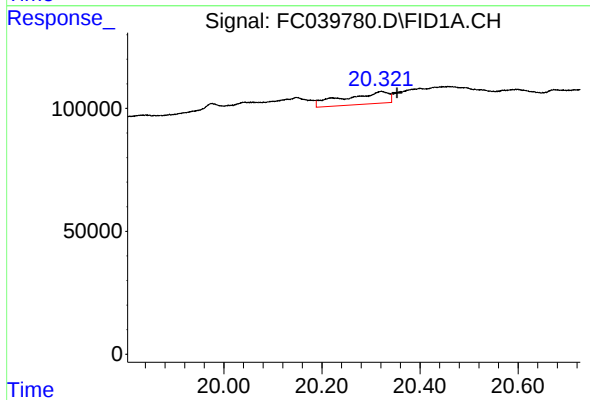

#21 n-Octatriacontane (C38)

R.T.: 20.321 min
Delta R.T.: -0.032 min
Response: 310034
Conc: 3.38 ug/ml