

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031319AL\
 Data File : FC039818.D
 Signal(s) : FID1A.CH
 Acq On : 14 Mar 2019 2:48
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 14 07:06:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 25 18:21:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.137	128347	0.955 ug/ml
19) T	n-Tetratriacontane (C34)	18.890	54455	0.479 ug/ml
20) T	n-Hexatriacontane (C36)	19.685	446655	4.631 ug/ml
21) T	n-Octatriacontane (C38)	20.354	1217421	13.259 ug/ml
22) T	n-Tetracontane (C40)	21.129	145487	1.603 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031319AL\
Data File : FC039818.D
Signal(s) : FID1A.CH
Acq On : 14 Mar 2019 2:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 14 07:06:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
Quant Title : GC Extractables
QLast Update : Mon Feb 25 18:21:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

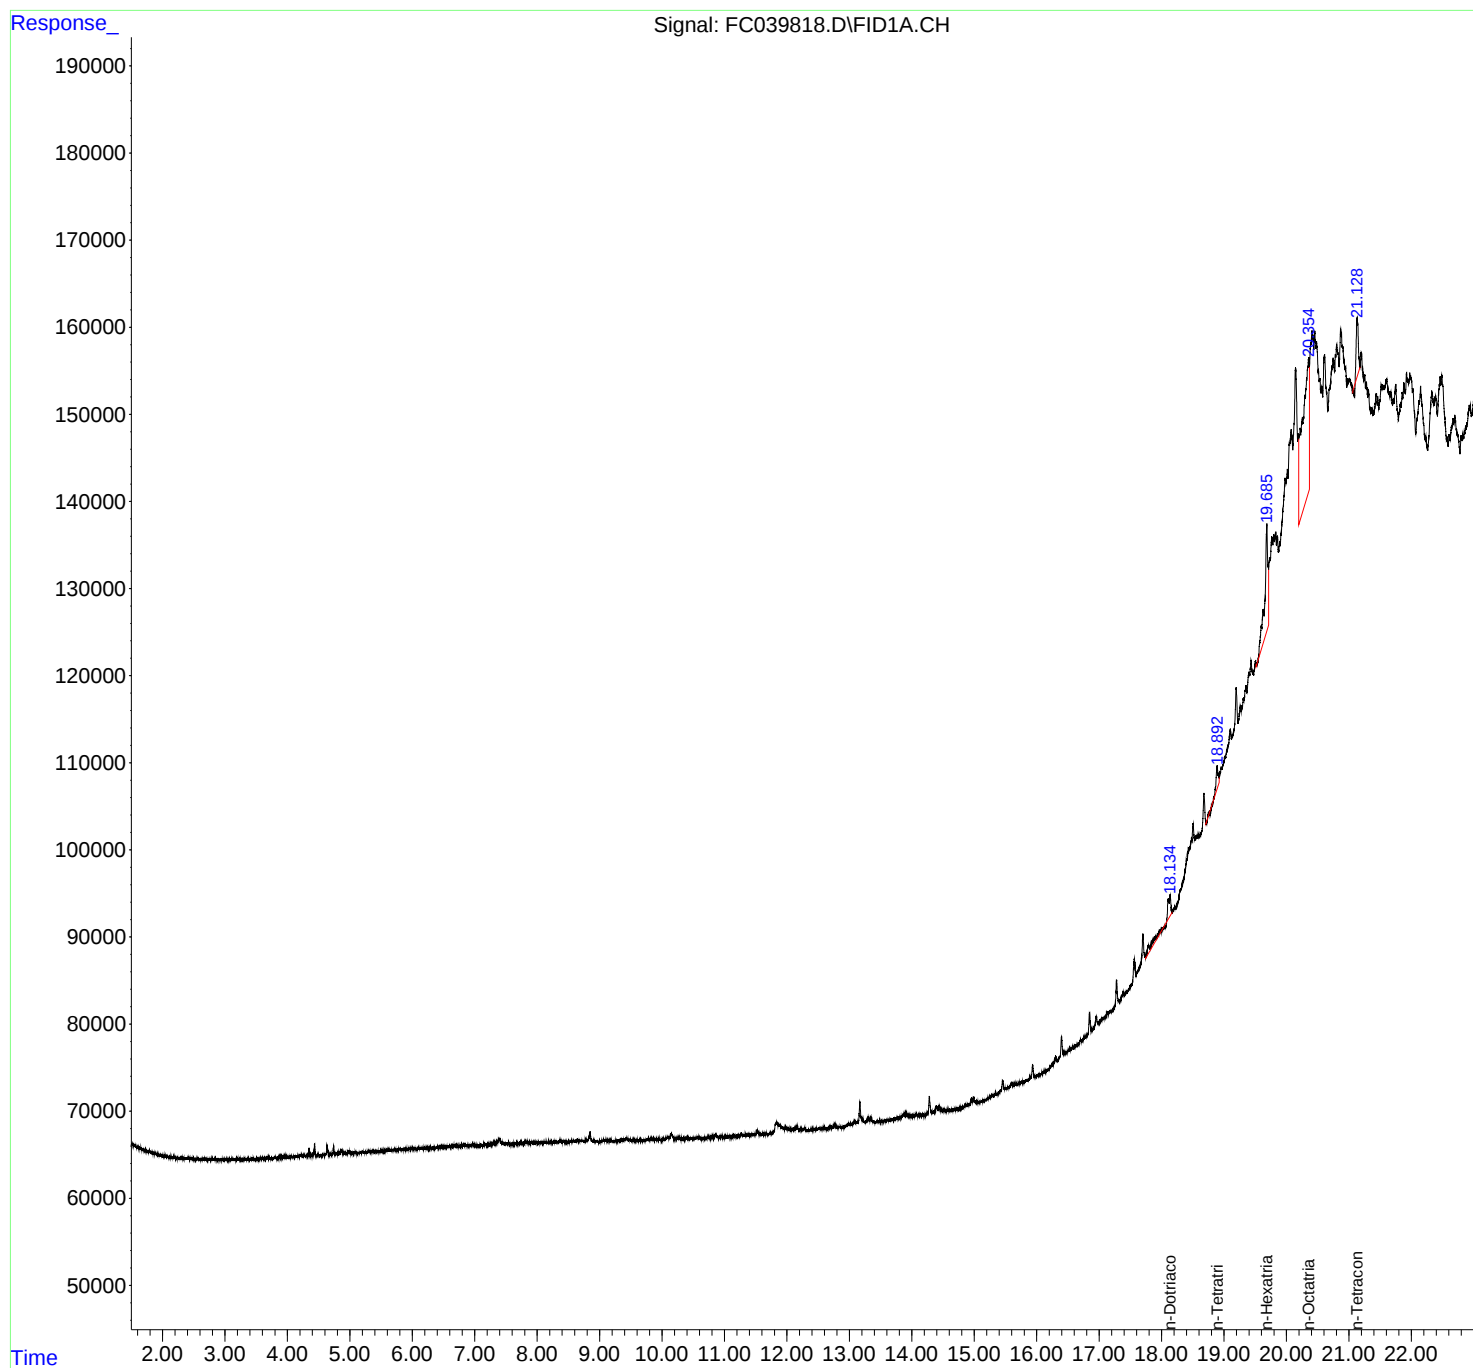


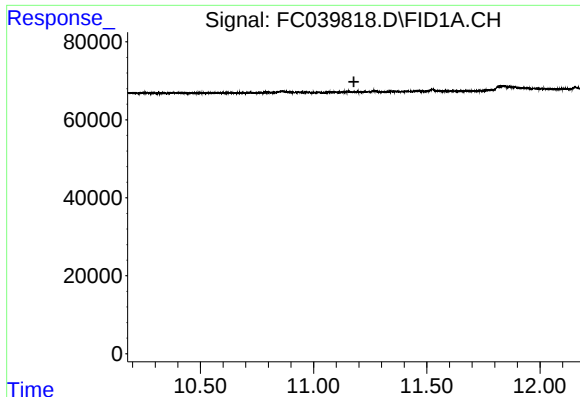

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.178 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

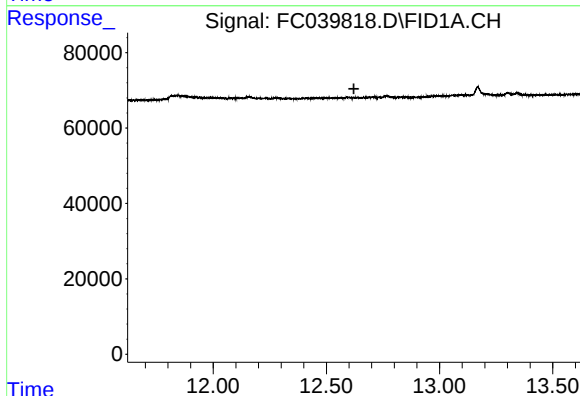


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.621 min
Response: 0
Conc: N.D.

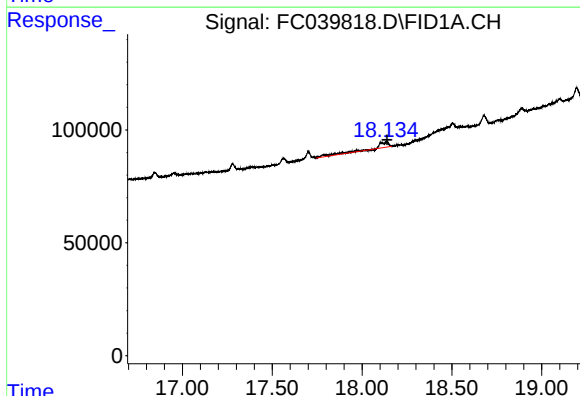


#18 n-Dotriacontane (C32)

R.T.: 18.137 min
Delta R.T.: -0.002 min
Response: 128347
Conc: 0.96 ug/ml

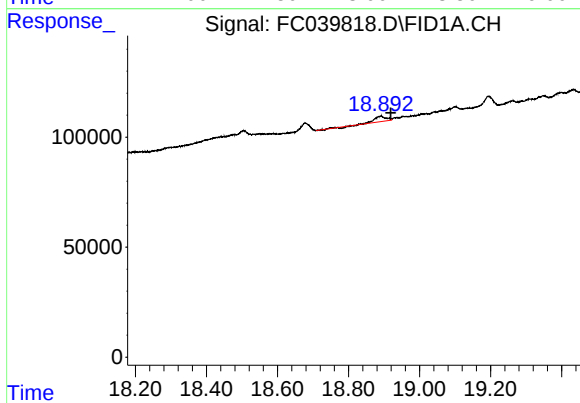

#19 n-Tetratriacontane (C34)


R.T.: 18.890 min
Delta R.T.: -0.028 min
Response: 54455
Conc: 0.48 ug/ml

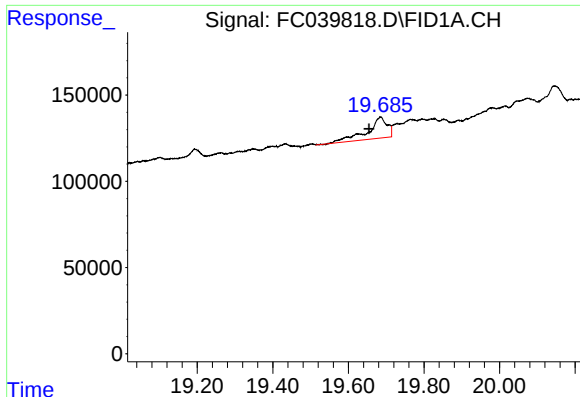

#20 n-Hexatriacontane (C36)


R.T.: 19.685 min
Delta R.T.: 0.030 min
Response: 446655
Conc: 4.63 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK

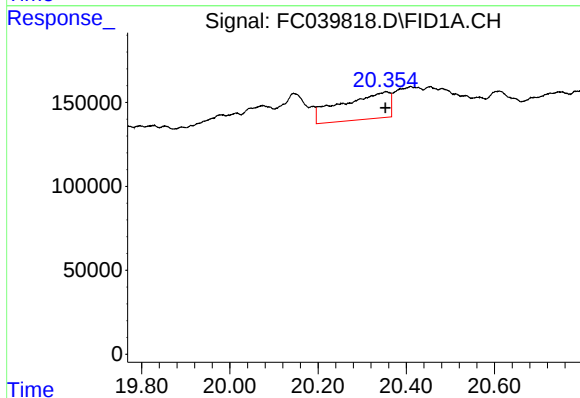

#21 n-Octatriacontane (C38)

R.T.: 20.354 min
Delta R.T.: 0.001 min
Response: 1217421
Conc: 13.26 ug/ml

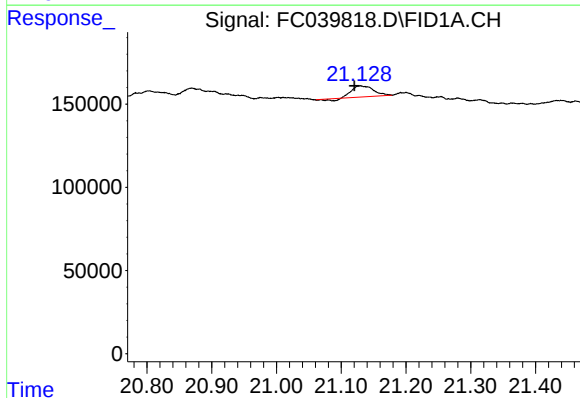

#22 n-Tetracontane (C40)

R.T.: 21.129 min
Delta R.T.: 0.009 min
Response: 145487
Conc: 1.60 ug/ml