

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031519AL\
 Data File : FC039930.D
 Signal(s) : FID1A.CH
 Acq On : 17 Mar 2019 5:03
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 18 00:50:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 25 18:21:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	17.274	72384	0.493 ug/ml
18) T	n-Dotriacontane (C32)	18.101	121034	0.901 ug/ml
19) T	n-Tetratriacontane (C34)	18.884	187520	1.649 ug/ml
20) T	n-Hexatriacontane (C36)	19.619	231216	2.397 ug/ml
21) T	n-Octatriacontane (C38)	20.385	1351027	14.714 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031519AL\
Data File : FC039930.D
Signal(s) : FID1A.CH
Acq On : 17 Mar 2019 5:03
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 18 00:50:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 022219.M
Quant Title : GC Extractables
QLast Update : Mon Feb 25 18:21:16 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

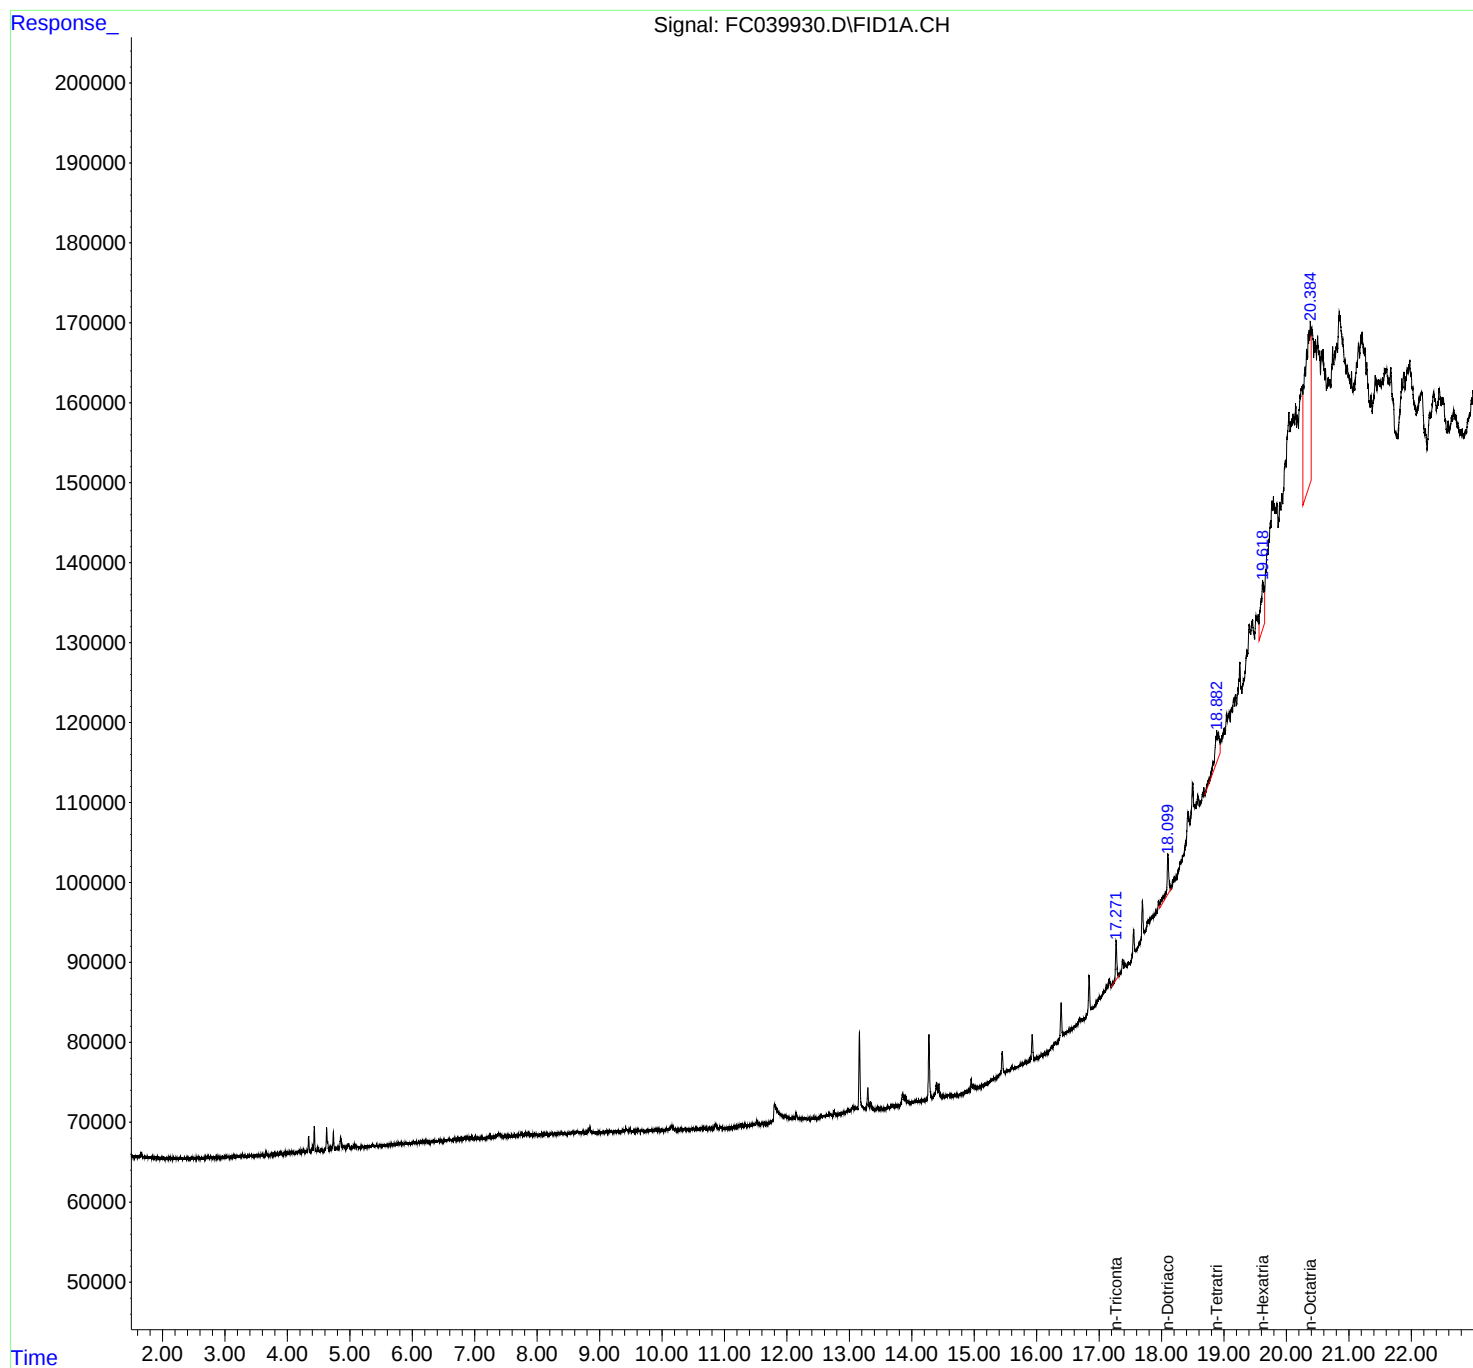


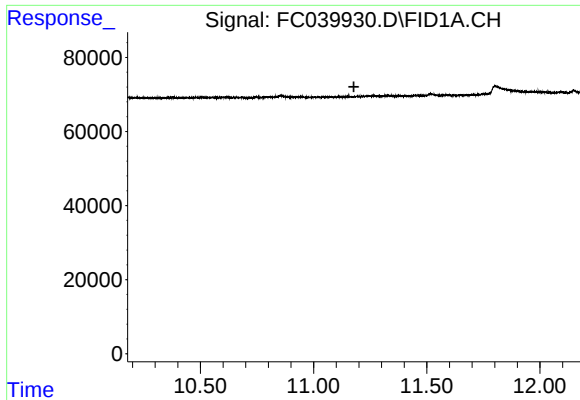

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.178 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

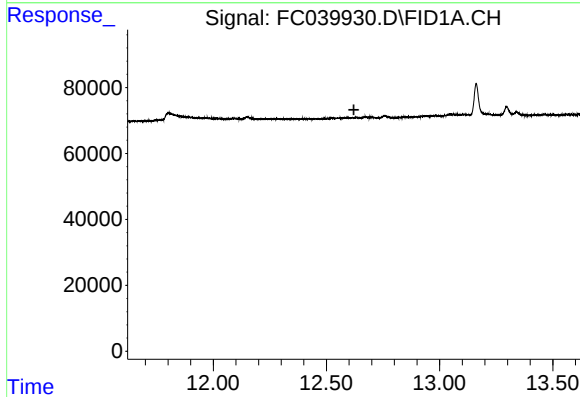


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.621 min
Response: 0
Conc: N.D.

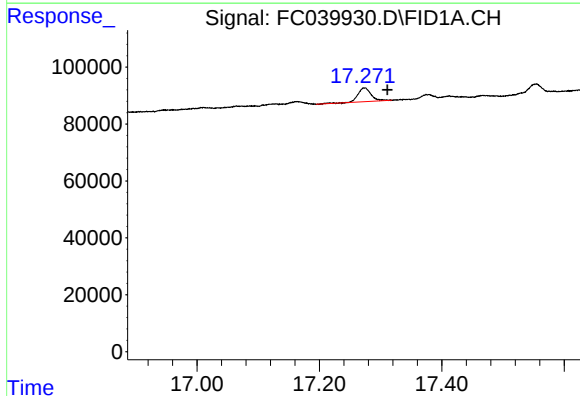


#17 n-Tricontane (C30)

R.T.: 17.274 min
Delta R.T.: -0.038 min
Response: 72384
Conc: 0.49 ug/ml

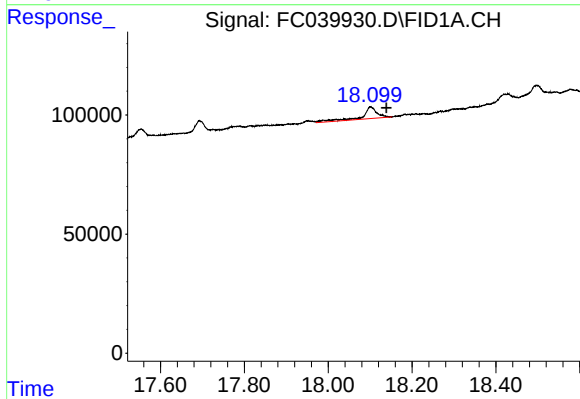

#18 n-Dotriacontane (C32)


R.T.: 18.101 min
Delta R.T.: -0.038 min
Response: 121034
Conc: 0.90 ug/ml

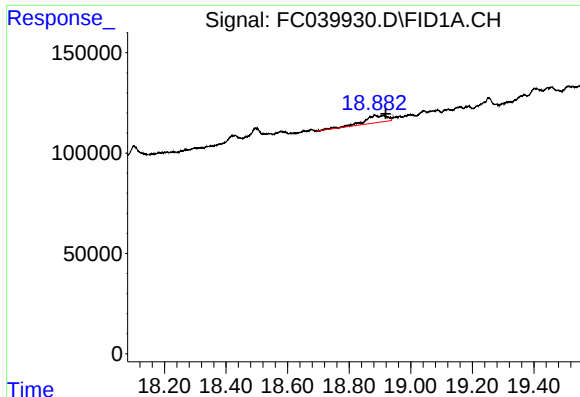

#19 n-Tetratriacontane (C34)


R.T.: 18.884 min
Delta R.T.: -0.035 min
Response: 187520
Conc: 1.65 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK

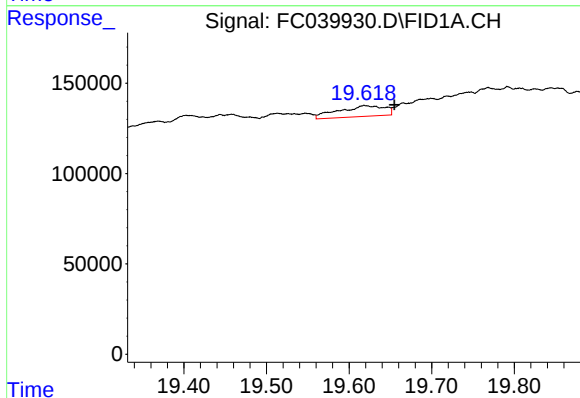

#20 n-Hexatriacontane (C36)

R.T.: 19.619 min
Delta R.T.: -0.036 min
Response: 231216
Conc: 2.40 ug/ml

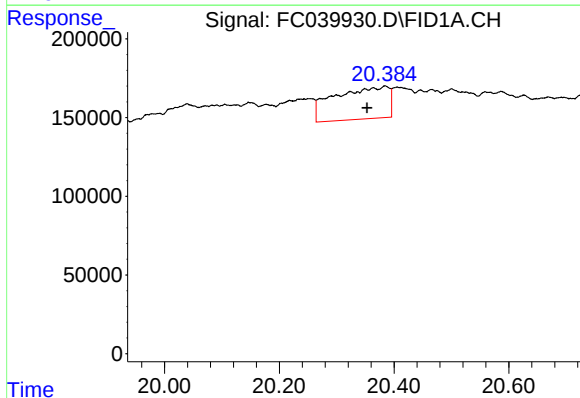

#21 n-Octatriacontane (C38)

R.T.: 20.385 min
Delta R.T.: 0.032 min
Response: 1351027
Conc: 14.71 ug/ml