

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
 Data File : FC052429.D
 Signal(s) : FID1A.CH
 Acq On : 15 Mar 2021 15:01
 Operator : DD\AJ
 Sample : M1652-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 16 01:31:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 04 03:56:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.044	2277474	21.899 ug/ml
Spiked Amount 50.000		Recovery =	43.80%
Target Compounds			
14) T n-Tetracosane (C24)	14.900	146813	1.259 ug/ml
15) T n-Hexacosane (C26)	15.922	190083	1.730 ug/ml
16) T n-Octacosane (C28)	16.872	223710	2.183 ug/ml
17) T n-Tricontane (C30)	17.760	245667	2.610 ug/ml
18) T n-Dotriacontane (C32)	18.591	189295	2.217 ug/ml
19) T n-Tetratriacontane (C34)	19.376	115558	1.491 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
Data File : FC052429.D
Signal(s) : FID1A.CH
Acq On : 15 Mar 2021 15:01
Operator : DD\AJ
Sample : M1652-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 16 01:31:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
Quant Title : GC Extractables
QLast Update : Thu Mar 04 03:56:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

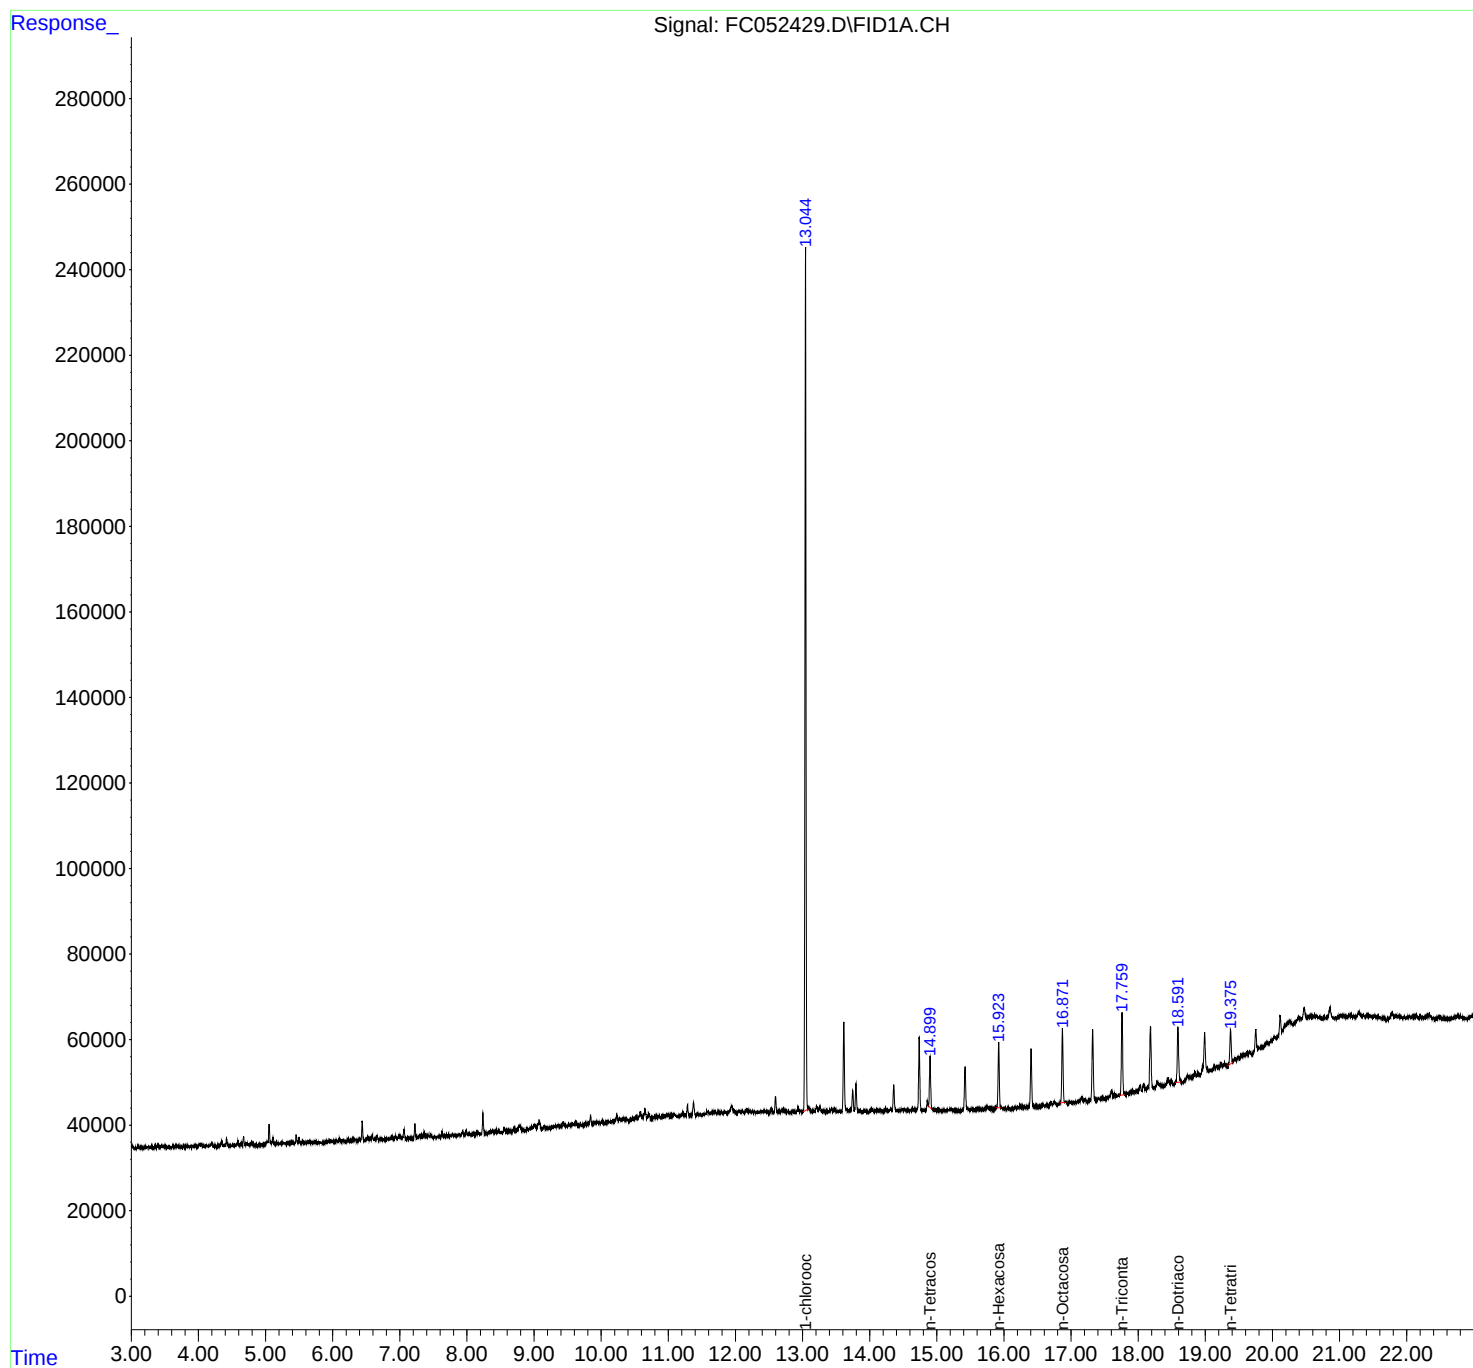


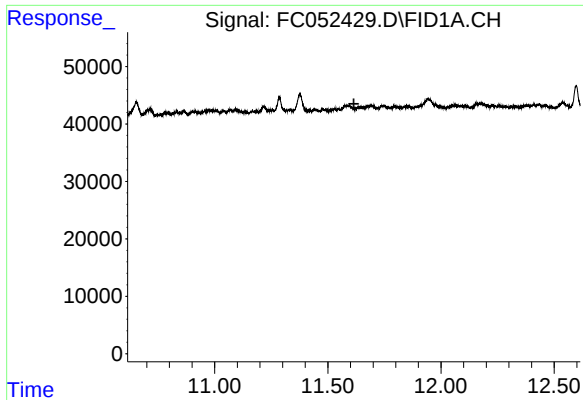

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.615 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

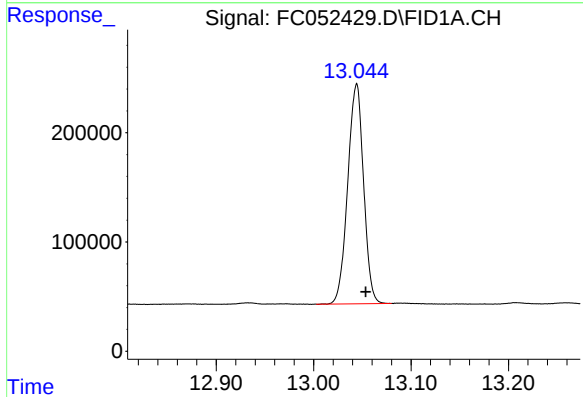


#12 1-chlorooctadecane (SURR)

R.T.: 13.044 min
Delta R.T.: -0.009 min
Response: 2277474
Conc: 21.90 ug/ml

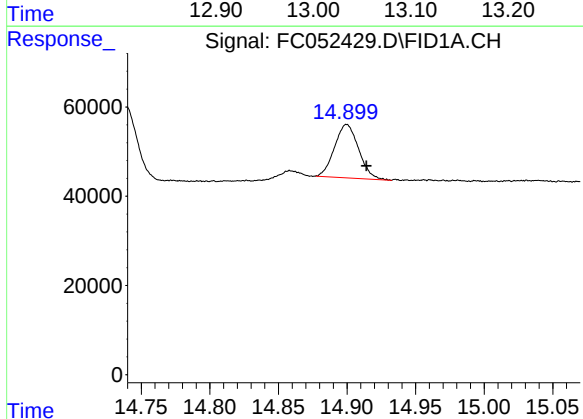


#14 n-Tetracosane (C24)

R.T.: 14.900 min
Delta R.T.: -0.014 min
Response: 146813
Conc: 1.26 ug/ml

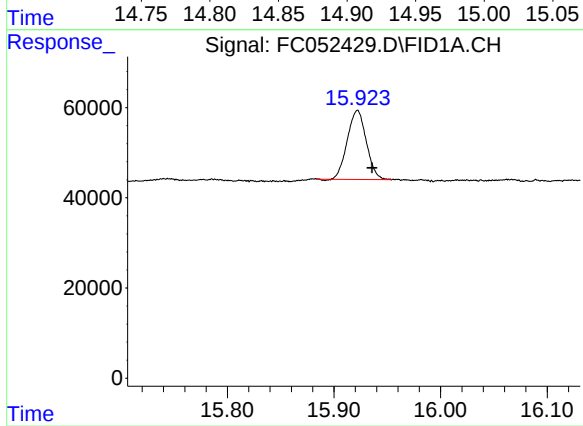

#15 n-Hexacosane (C26)


R.T.: 15.922 min
Delta R.T.: -0.014 min
Response: 190083
Conc: 1.73 ug/ml

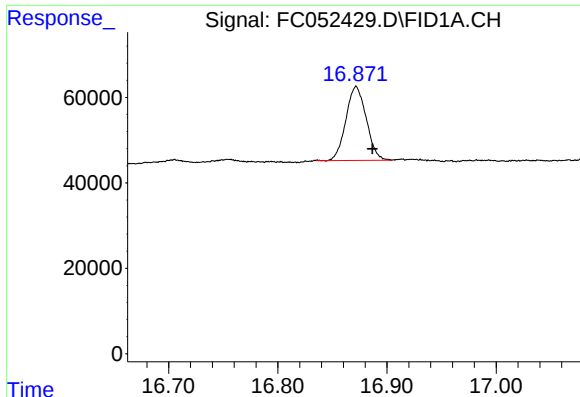

#16 n-Octacosane (C28)


R.T.: 16.872 min
Delta R.T.: -0.015 min
Response: 223710
Conc: 2.18 ug/ml

Instrument :
FID_C
ClientSampleId :

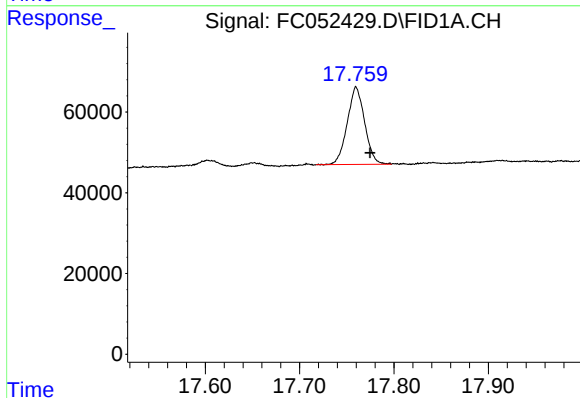


#17 n-Tricontane (C30)

R.T.: 17.760 min
Delta R.T.: -0.015 min
Response: 245667
Conc: 2.61 ug/ml

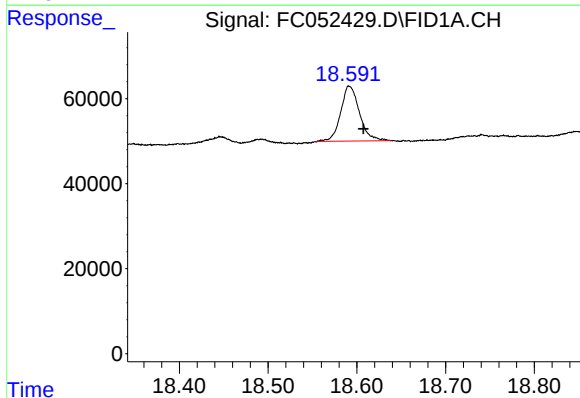

#18 n-Dotriacontane (C32)

R.T.: 18.591 min
Delta R.T.: -0.016 min
Response: 189295
Conc: 2.22 ug/ml

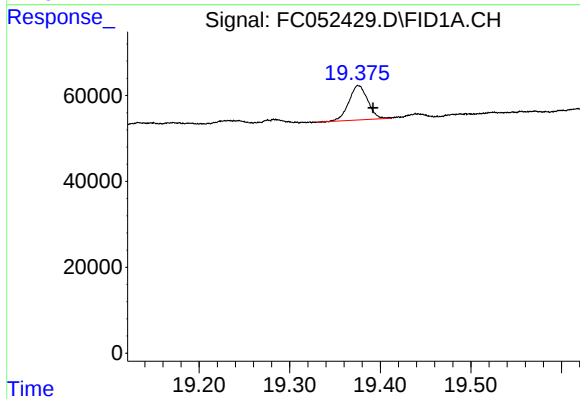

#19 n-Tetratriacontane (C34)

R.T.: 19.376 min
Delta R.T.: -0.016 min
Response: 115558
Conc: 1.49 ug/ml