

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
 Data File : FC052430.D
 Signal(s) : FID1A.CH
 Acq On : 15 Mar 2021 15:40
 Operator : DD\AJ
 Sample : M1652-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 16 01:31:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 04 03:56:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.043	1838970	17.682 ug/ml
Spiked Amount 50.000		Recovery =	35.36%
Target Compounds			
14) T n-Tetracosane (C24)	14.899	108938	0.934 ug/ml
15) T n-Hexacosane (C26)	15.922	99768	0.908 ug/ml
16) T n-Octacosane (C28)	16.873	110696	1.080 ug/ml
17) T n-Tricontane (C30)	17.758	123258	1.309 ug/ml
18) T n-Dotriacontane (C32)	18.591	97084	1.137 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
Data File : FC052430.D
Signal(s) : FID1A.CH
Acq On : 15 Mar 2021 15:40
Operator : DD\AJ
Sample : M1652-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 16 01:31:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
Quant Title : GC Extractables
QLast Update : Thu Mar 04 03:56:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

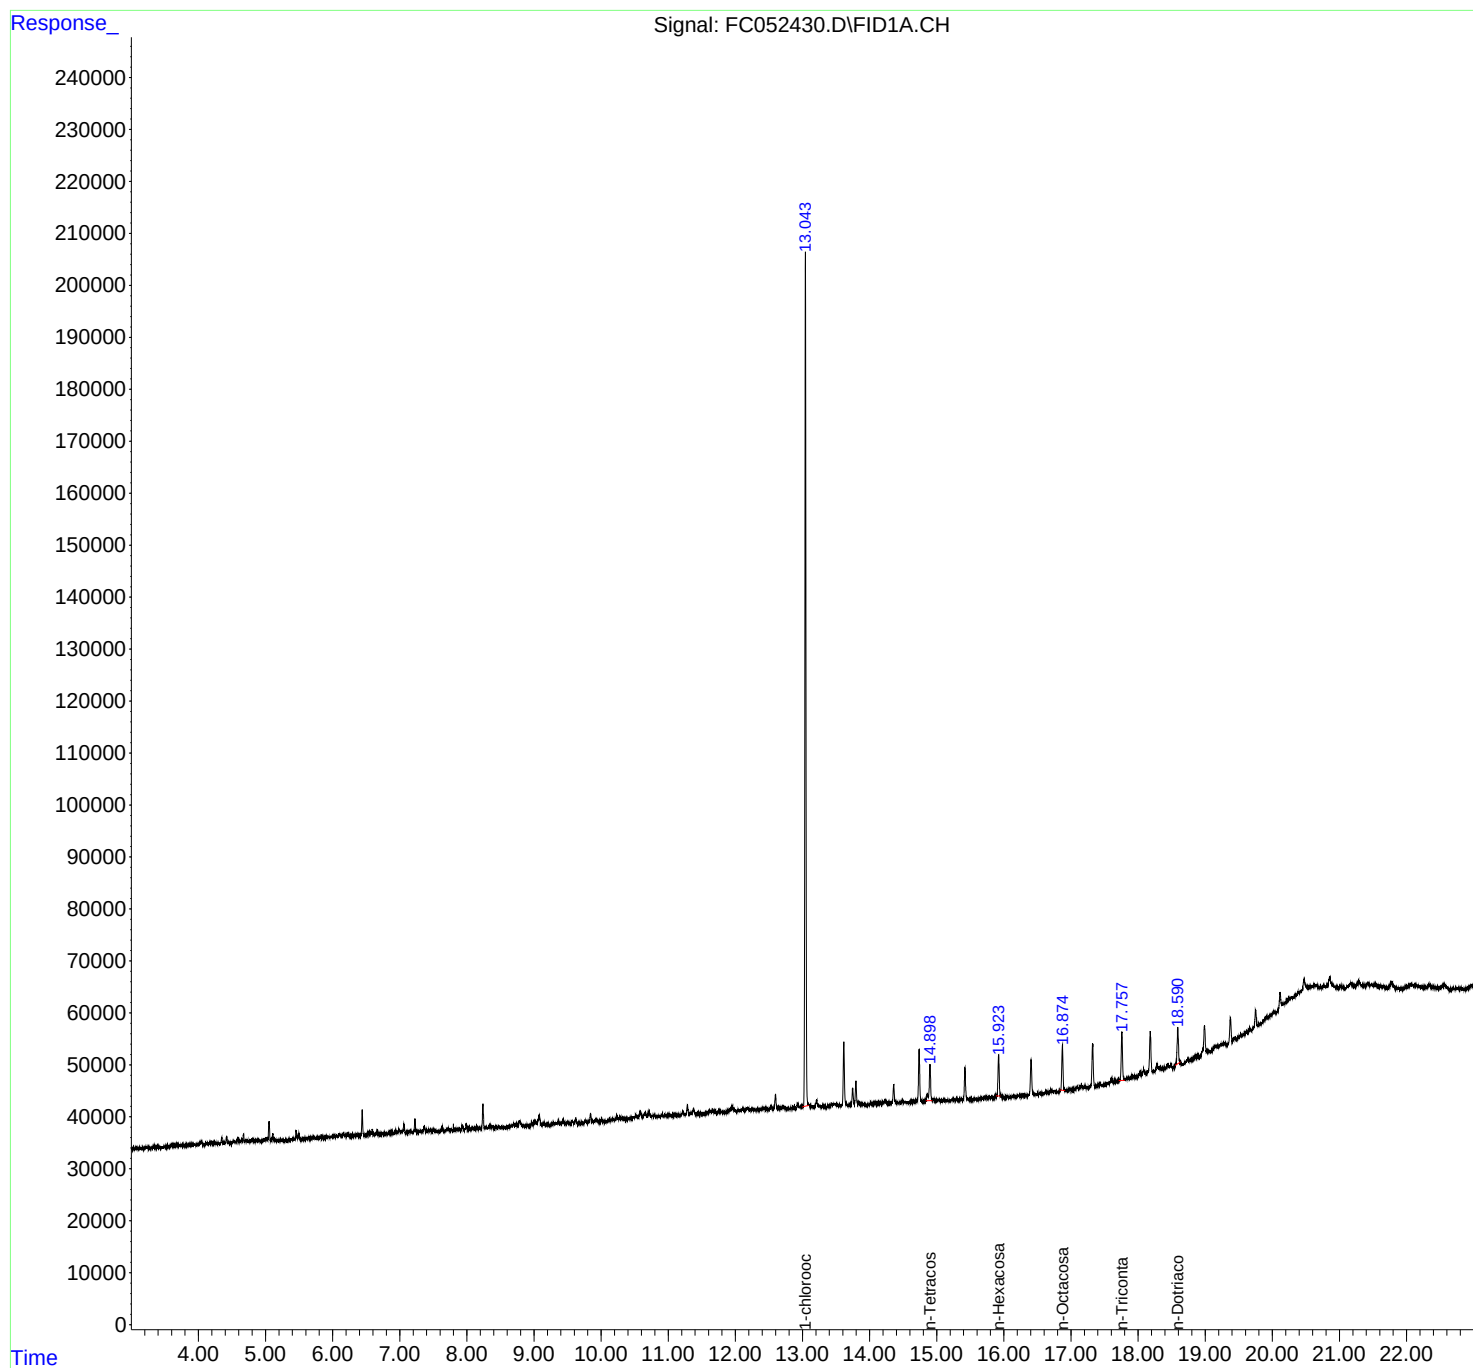


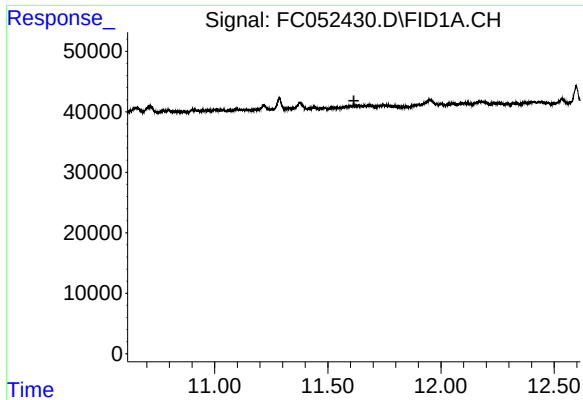

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.615 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

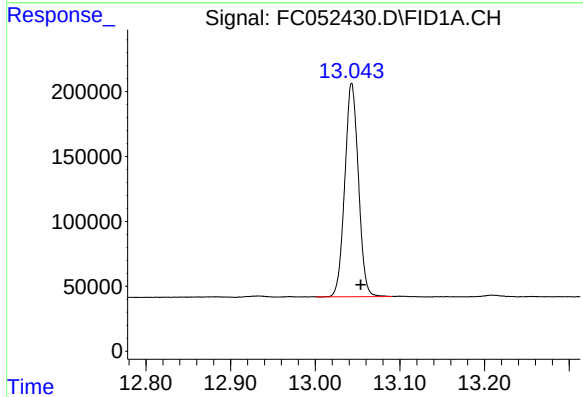


#12 1-chlorooctadecane (SURR)

R.T.: 13.043 min
Delta R.T.: -0.011 min
Response: 1838970
Conc: 17.68 ug/ml

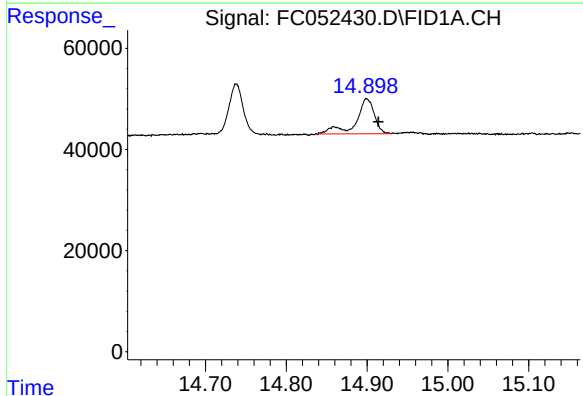


#14 n-Tetracosane (C24)

R.T.: 14.899 min
Delta R.T.: -0.015 min
Response: 108938
Conc: 0.93 ug/ml

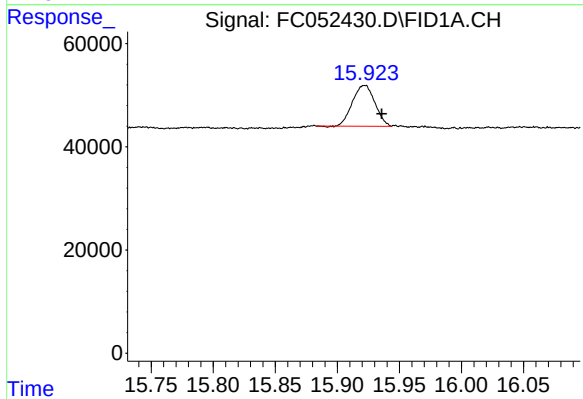

#15 n-Hexacosane (C26)


R.T.: 15.922 min
Delta R.T.: -0.014 min
Response: 99768
Conc: 0.91 ug/ml

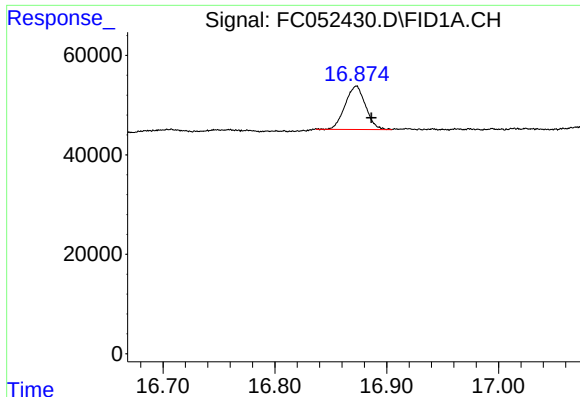

#16 n-Octacosane (C28)


R.T.: 16.873 min
Delta R.T.: -0.014 min
Response: 110696
Conc: 1.08 ug/ml

Instrument :
FID_C
ClientSampleId :

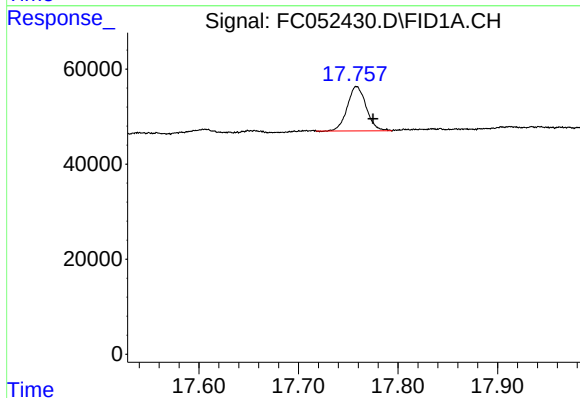

#17 n-Tricontane (C30)

R.T.: 17.758 min
Delta R.T.: -0.016 min
Response: 123258
Conc: 1.31 ug/ml

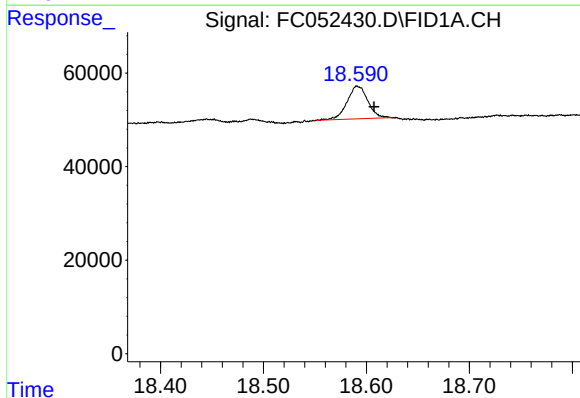

#18 n-Dotriacontane (C32)

R.T.: 18.591 min
Delta R.T.: -0.016 min
Response: 97084
Conc: 1.14 ug/ml