

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
 Data File : FC052431.D
 Signal(s) : FID1A.CH
 Acq On : 15 Mar 2021 16:19
 Operator : DD\AJ
 Sample : M1652-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 16 01:32:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 04 03:56:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.045	2392937	23.009 ug/ml
Spiked Amount 50.000		Recovery =	46.02%
Target Compounds			
4) T n-Dodecane (C12)	6.441	67485	0.558 ug/ml
6) T n-Tetradecane (C14)	8.240	70680	0.583 ug/ml
14) T n-Tetracosane (C24)	14.900	134839	1.157 ug/ml
15) T n-Hexacosane (C26)	15.923	179820	1.637 ug/ml
16) T n-Octacosane (C28)	16.872	195167	1.904 ug/ml
17) T n-Tricontane (C30)	17.760	201875	2.144 ug/ml
18) T n-Dotriacontane (C32)	18.591	164292	1.924 ug/ml
19) T n-Tetratriacontane (C34)	19.375	100177	1.292 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
Data File : FC052431.D
Signal(s) : FID1A.CH
Acq On : 15 Mar 2021 16:19
Operator : DD\AJ
Sample : M1652-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 16 01:32:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
Quant Title : GC Extractables
QLast Update : Thu Mar 04 03:56:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

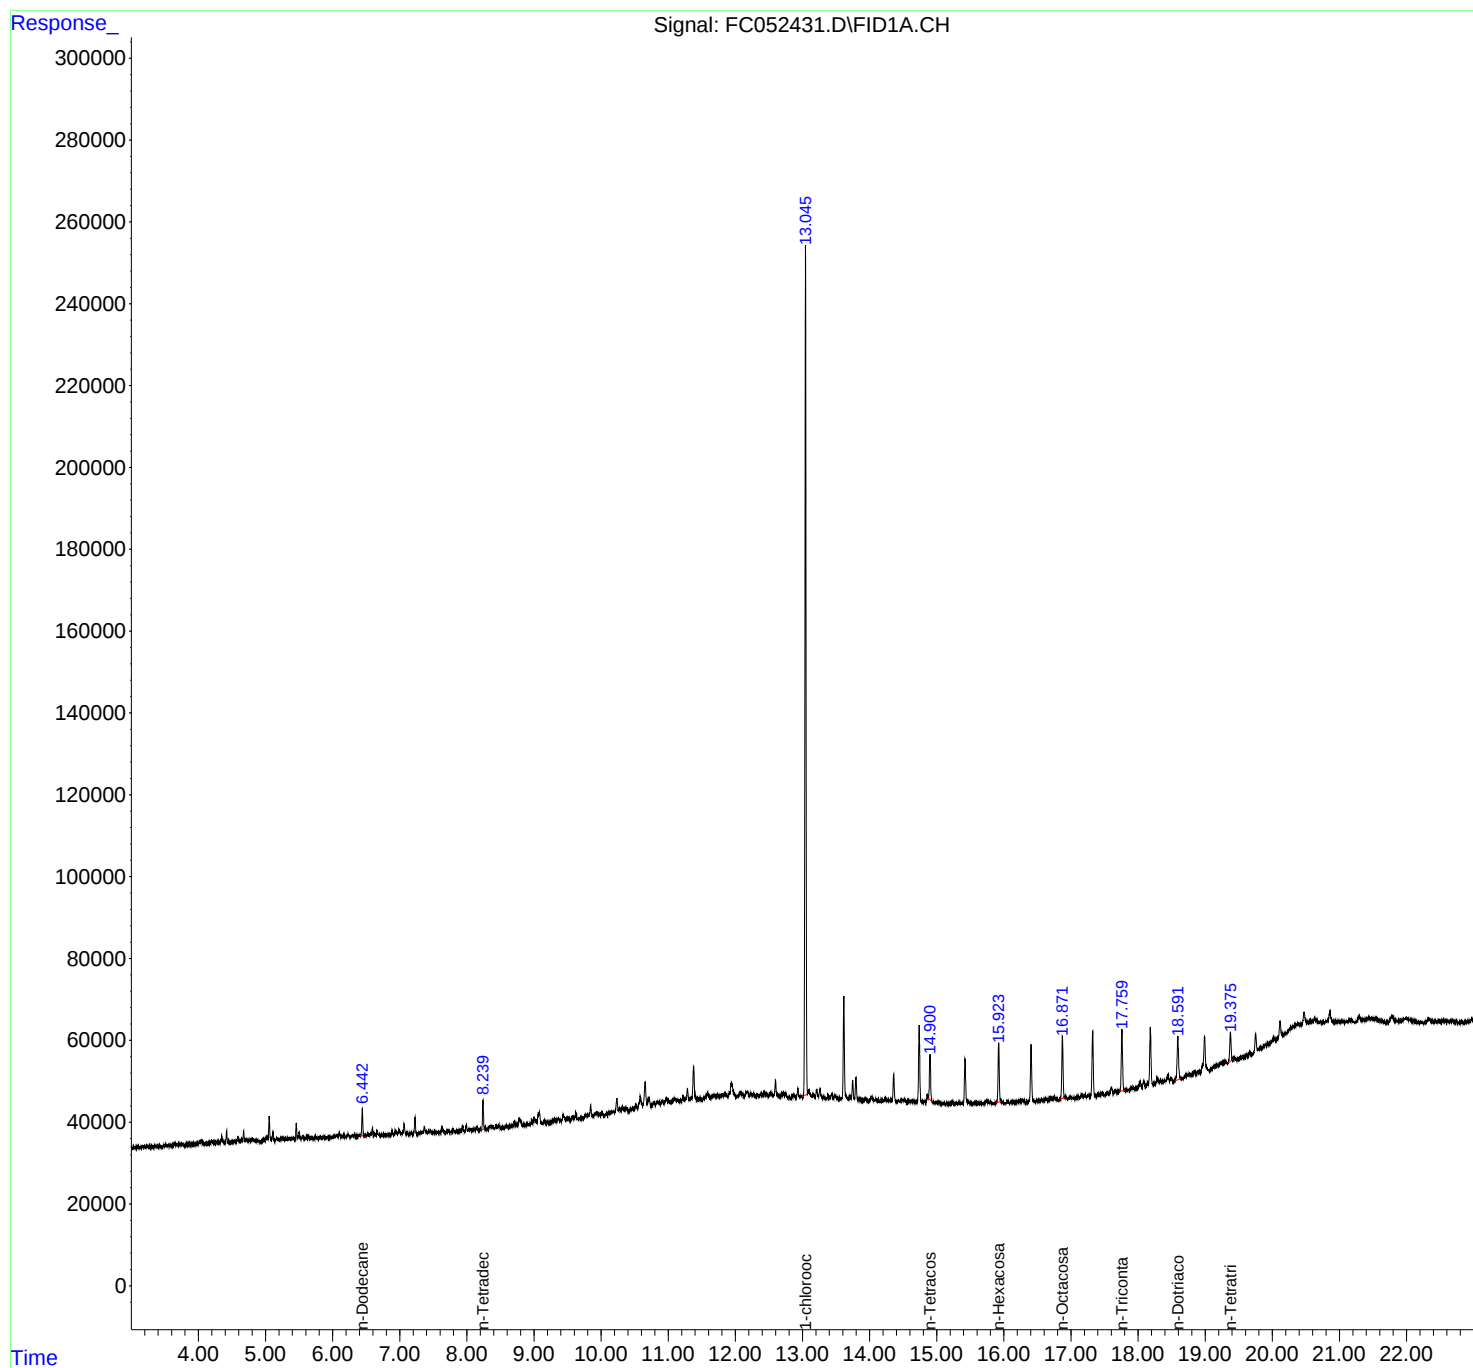


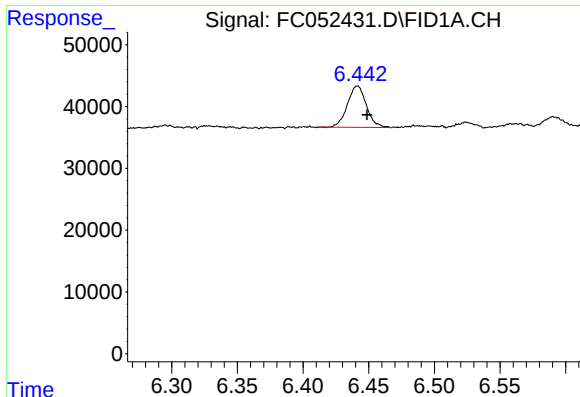

#4 n-Dodecane (C12)


R.T.: 6.441 min
Delta R.T.: -0.007 min
Response: 67485
Conc: 0.56 ug/ml

Instrument :
FID_C
ClientSampleId :

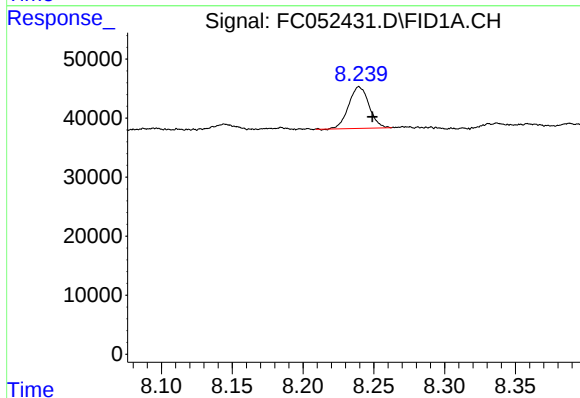


#6 n-Tetradecane (C14)

R.T.: 8.240 min
Delta R.T.: -0.009 min
Response: 70680
Conc: 0.58 ug/ml

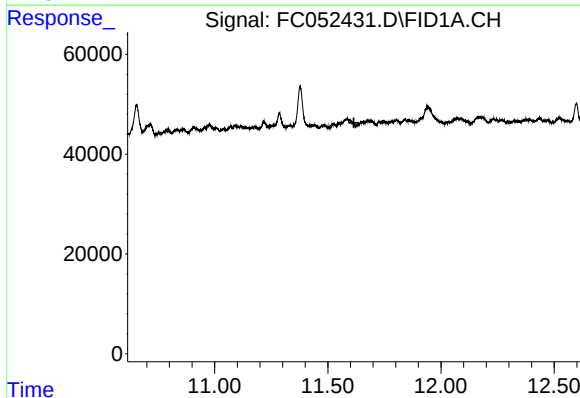


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.615 min
Response: 0
Conc: N.D.

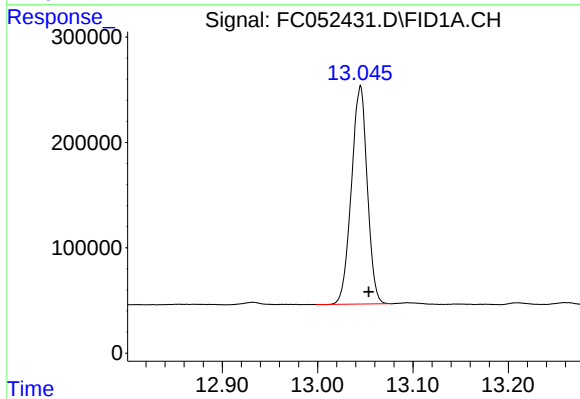

#12 1-chlorooctadecane (SURR)


R.T.: 13.045 min
Delta R.T.: -0.009 min
Response: 2392937
Conc: 23.01 ug/ml

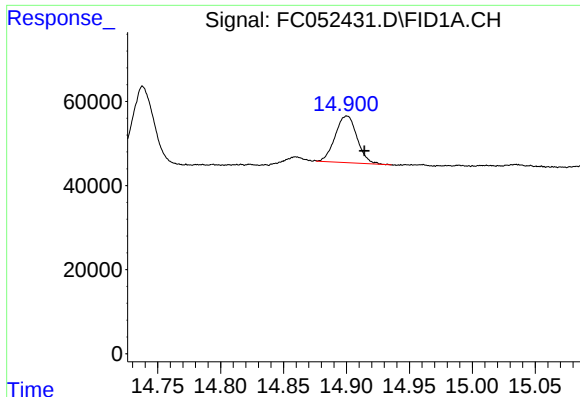

#14 n-Tetracosane (C24)


R.T.: 14.900 min
Delta R.T.: -0.014 min
Response: 134839
Conc: 1.16 ug/ml

Instrument :
FID_C
ClientSampleId :

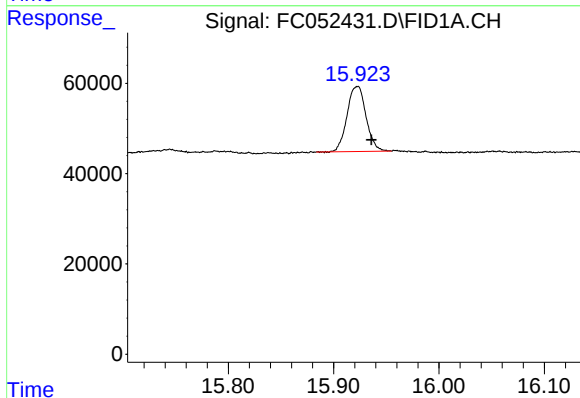


#15 n-Hexacosane (C26)

R.T.: 15.923 min
Delta R.T.: -0.013 min
Response: 179820
Conc: 1.64 ug/ml

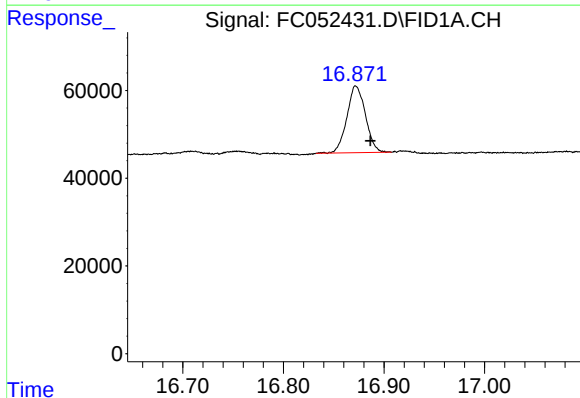


#16 n-Octacosane (C28)

R.T.: 16.872 min
Delta R.T.: -0.014 min
Response: 195167
Conc: 1.90 ug/ml

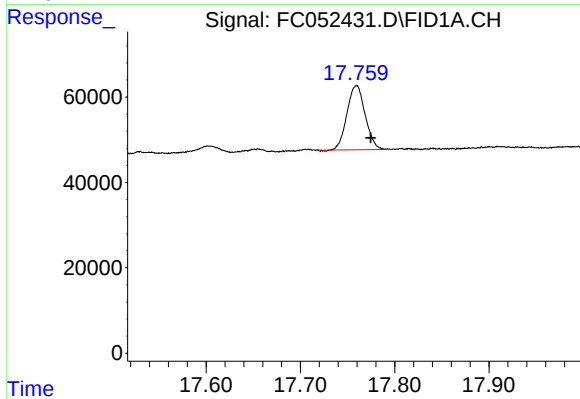

#17 n-Tricontane (C30)


R.T.: 17.760 min
Delta R.T.: -0.015 min
Response: 201875
Conc: 2.14 ug/ml

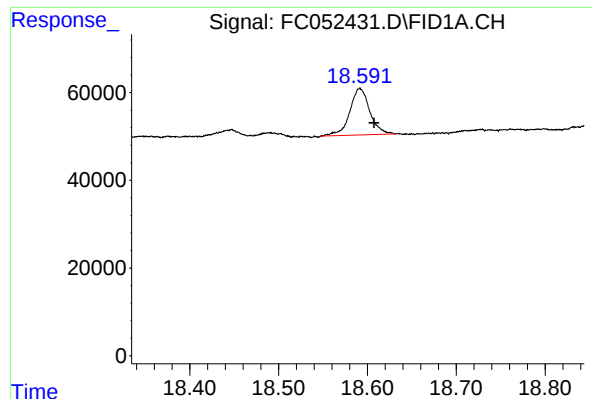

#18 n-Dotriacontane (C32)

R.T.: 18.591 min
Delta R.T.: -0.016 min
Response: 164292
Conc: 1.92 ug/ml

Instrument :
FID_C
ClientSampleId :

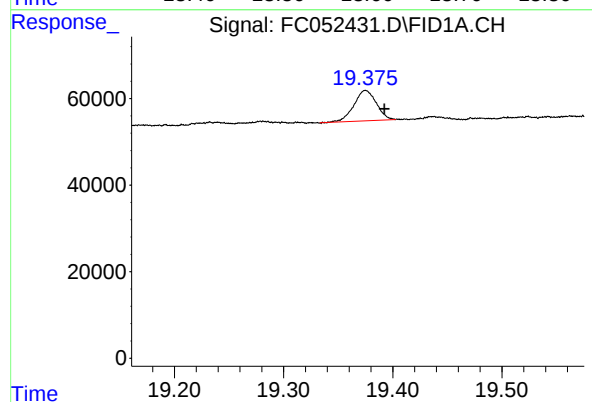

#19 n-Tetratriacontane (C34)

R.T.: 19.375 min
Delta R.T.: -0.017 min
Response: 100177
Conc: 1.29 ug/ml