

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
 Data File : FC052432.D
 Signal(s) : FID1A.CH
 Acq On : 15 Mar 2021 16:59
 Operator : DD\AJ
 Sample : M1652-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 16 01:32:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 04 03:56:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.045	2726609	26.217 ug/ml
Spiked Amount 50.000		Recovery =	52.43%
Target Compounds			
13) T n-Docosane (C22)	13.797	83712	0.696 ug/ml
14) T n-Tetracosane (C24)	14.900	153600	1.318 ug/ml
15) T n-Hexacosane (C26)	15.922	207461	1.889 ug/ml
16) T n-Octacosane (C28)	16.873	231899	2.262 ug/ml
17) T n-Tricontane (C30)	17.760	231056	2.454 ug/ml
18) T n-Dotriacontane (C32)	18.593	174894	2.048 ug/ml
19) T n-Tetratriacontane (C34)	19.376	108367	1.398 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031521AL\
Data File : FC052432.D
Signal(s) : FID1A.CH
Acq On : 15 Mar 2021 16:59
Operator : DD\AJ
Sample : M1652-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 16 01:32:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 030321.M
Quant Title : GC Extractables
QLast Update : Thu Mar 04 03:56:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

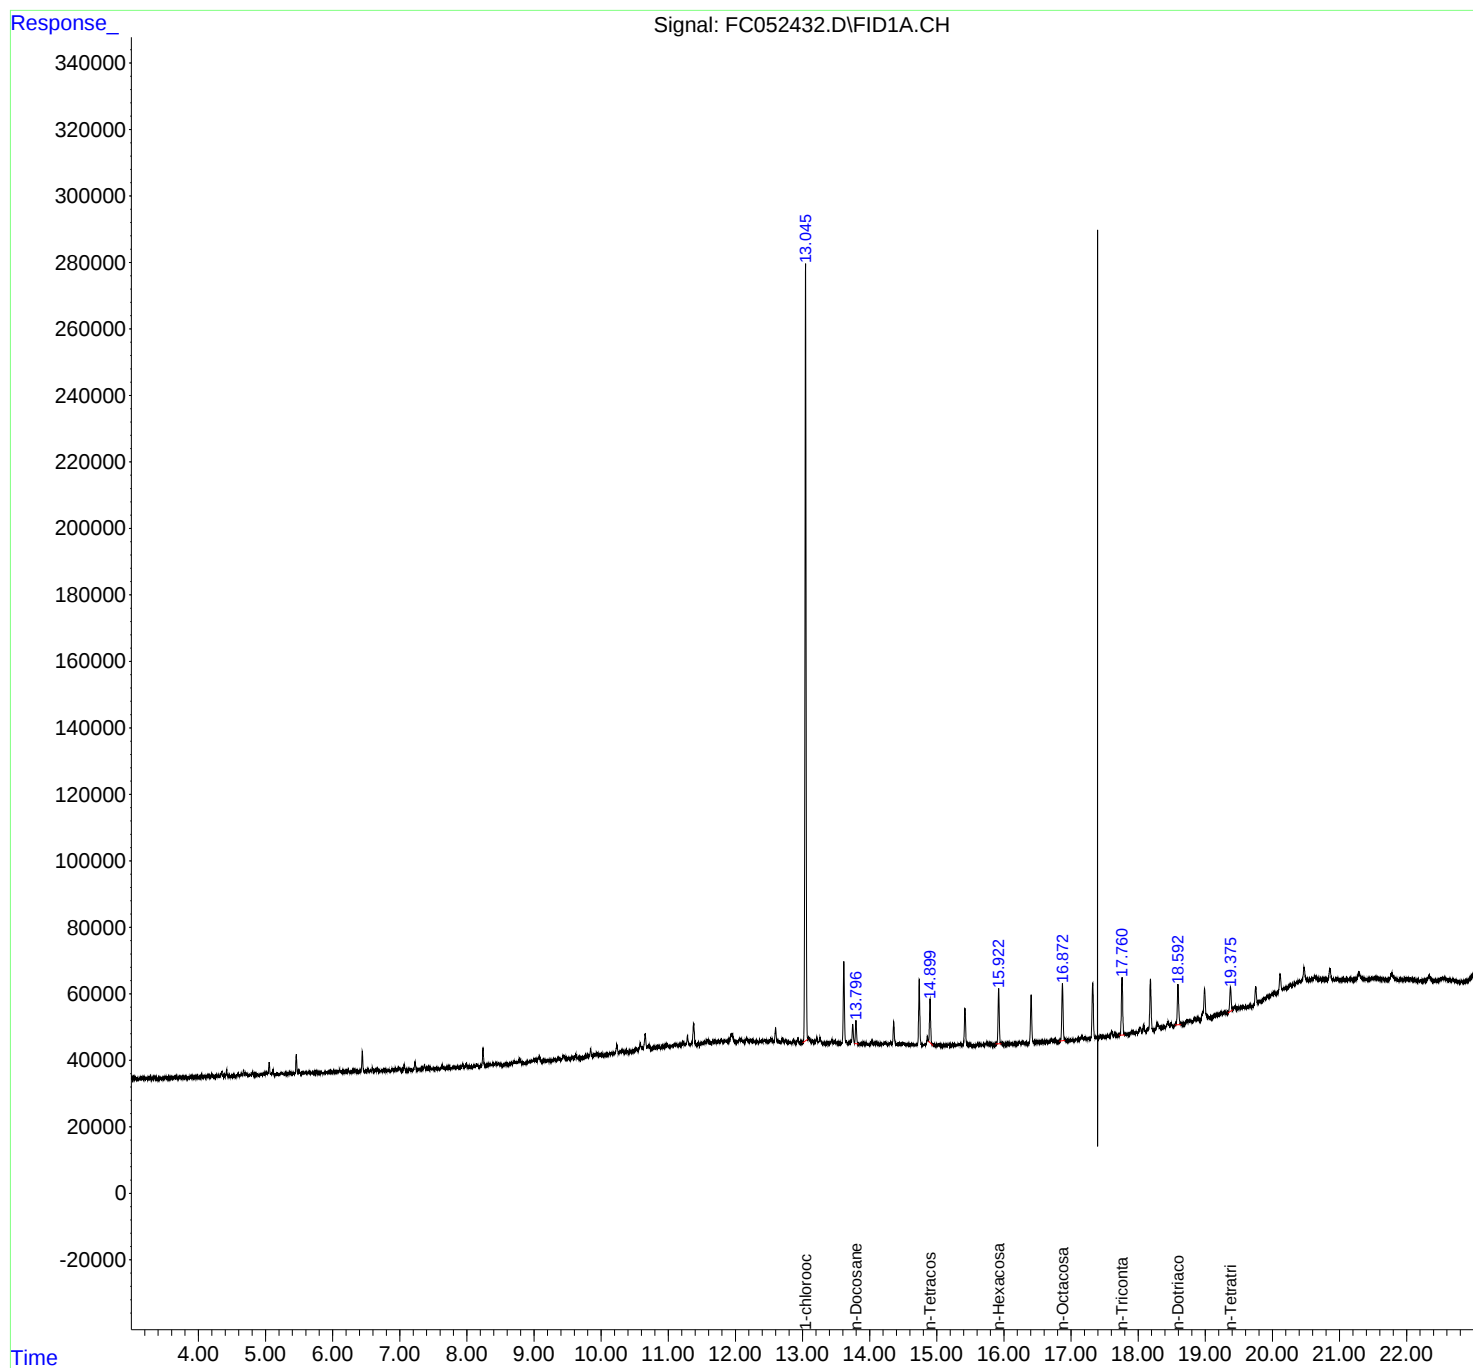


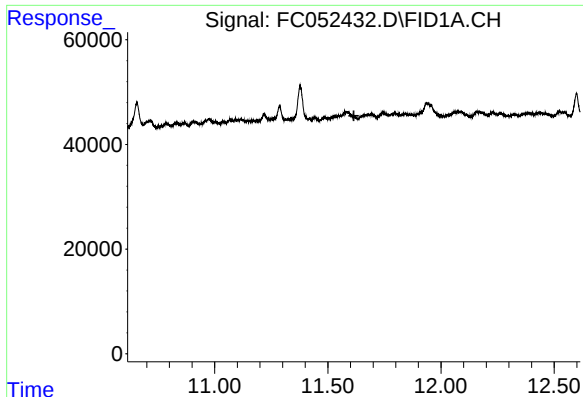

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.615 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

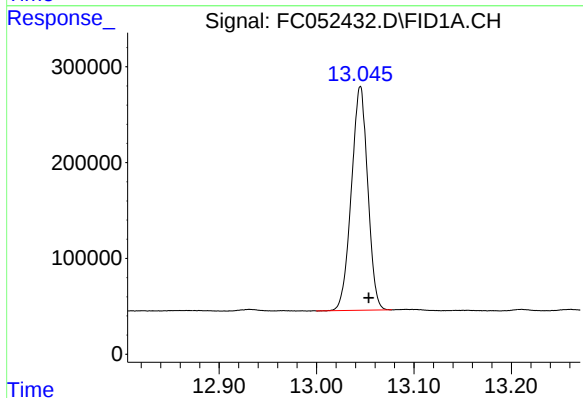


#12 1-chlorooctadecane (SURR)

R.T.: 13.045 min
Delta R.T.: -0.009 min
Response: 2726609
Conc: 26.22 ug/ml

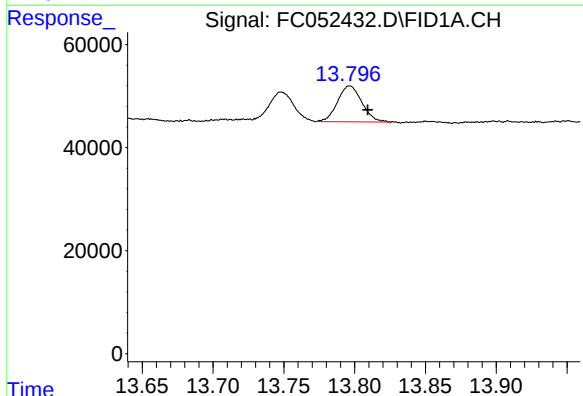


#13 n-Docosane (C22)

R.T.: 13.797 min
Delta R.T.: -0.013 min
Response: 83712
Conc: 0.70 ug/ml

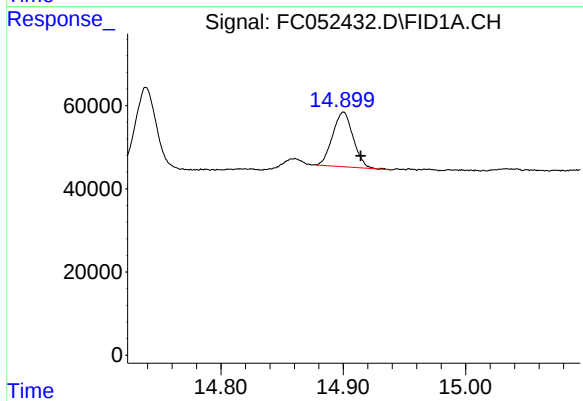

#14 n-Tetracosane (C24)


R.T.: 14.900 min
Delta R.T.: -0.014 min
Response: 153600
Conc: 1.32 ug/ml

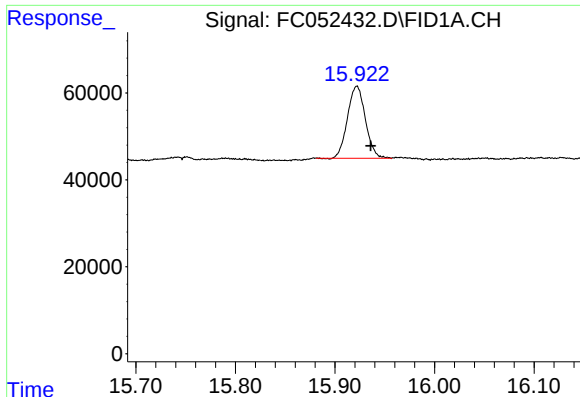

#15 n-Hexacosane (C26)


R.T.: 15.922 min
Delta R.T.: -0.014 min
Response: 207461
Conc: 1.89 ug/ml

Instrument :
FID_C
ClientSampleId :

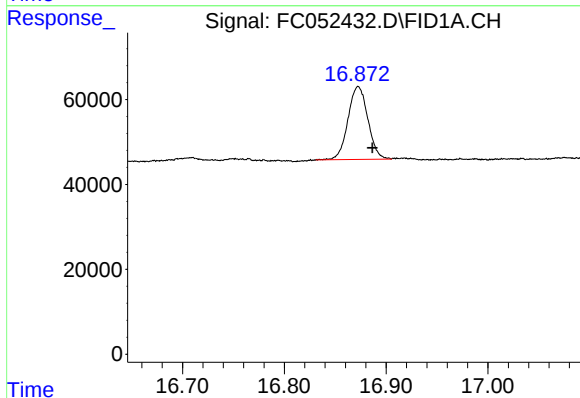


#16 n-Octacosane (C28)

R.T.: 16.873 min
Delta R.T.: -0.014 min
Response: 231899
Conc: 2.26 ug/ml

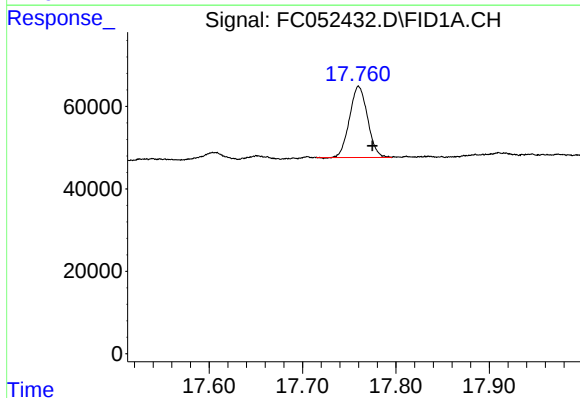


#17 n-Tricontane (C30)

R.T.: 17.760 min
Delta R.T.: -0.015 min
Response: 231056
Conc: 2.45 ug/ml

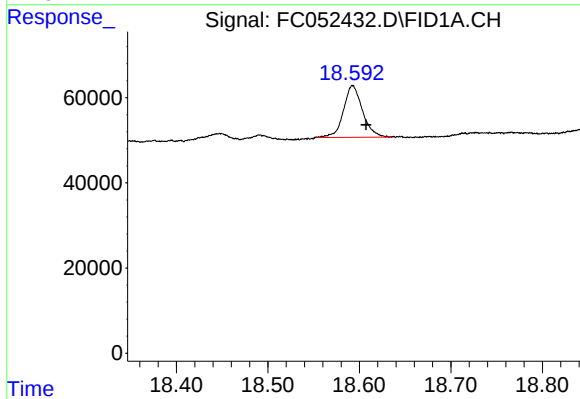

#18 n-Dotriacontane (C32)

R.T.: 18.593 min
Delta R.T.: -0.015 min
Response: 174894
Conc: 2.05 ug/ml

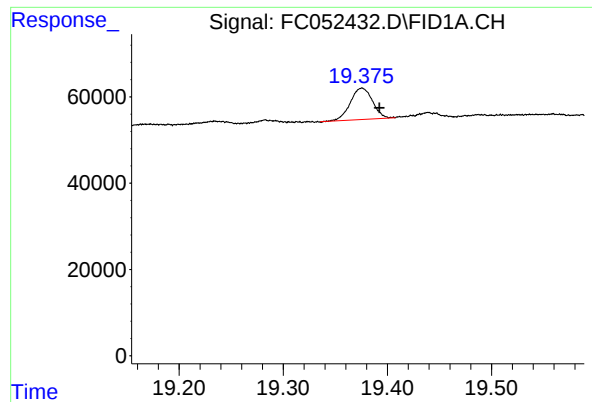

#19 n-Tetratriacontane (C34)

R.T.: 19.376 min
Delta R.T.: -0.017 min
Response: 108367
Conc: 1.40 ug/ml

Instrument :
FID_C
ClientSampleId :