

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC031721AL\  
 Data File : FC052496.D  
 Signal(s) : FID1A.CH  
 Acq On : 18 Mar 2021 5:57  
 Operator : DD\AJ  
 Sample : M1555-04  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Mar 18 07:49:00 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Alaphatic EPH 031721.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Mar 17 03:47:28 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.007 | 5329032    | 49.408 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 98.82%       |
| Target Compounds               |        |            |              |
| 4) T n-Dodecane (C12)          | 6.412  | 85889      | 0.715 ug/ml  |
| 6) T n-Tetradecane (C14)       | 8.208  | 121076     | 1.001 ug/ml  |
| 7) T n-Hexadecane (C16)        | 9.808  | 86230      | 0.717 ug/ml  |
| 19) T n-Tetratriacontane (C34) | 19.332 | 205440     | 2.235 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC031721AL\  
Data File : FC052496.D  
Signal(s) : FID1A.CH  
Acq On : 18 Mar 2021 5:57  
Operator : DD\AJ  
Sample : M1555-04  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Mar 18 07:49:00 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 031721.M  
Quant Title : GC Extractables  
QLast Update : Wed Mar 17 03:47:28 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

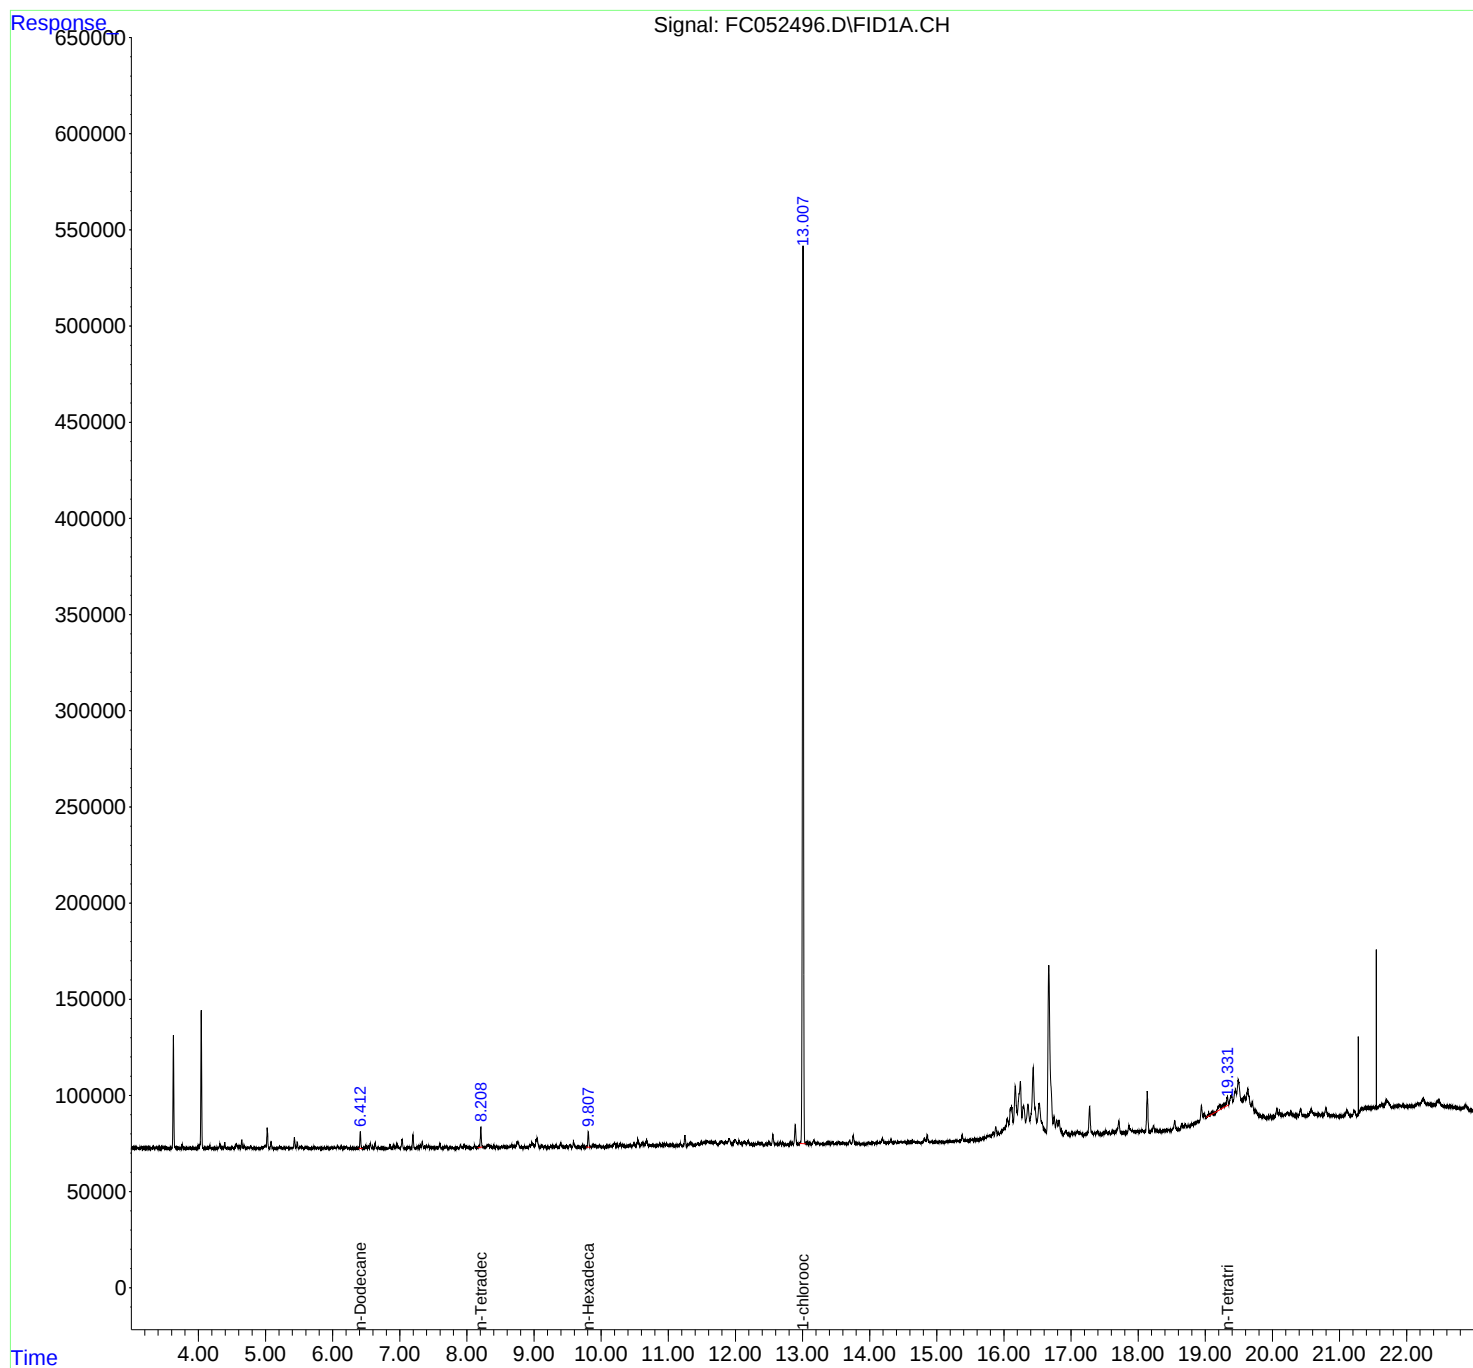


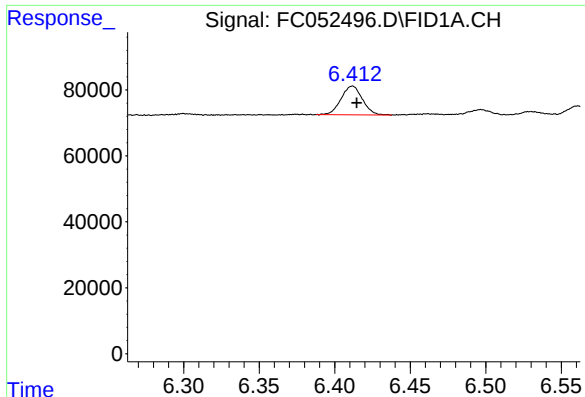

#4 n-Dodecane (C12)


R.T.: 6.412 min  
Delta R.T.: -0.003 min  
Response: 85889  
Conc: 0.72 ug/ml

Instrument :  
FID\_C  
ClientSampleId :

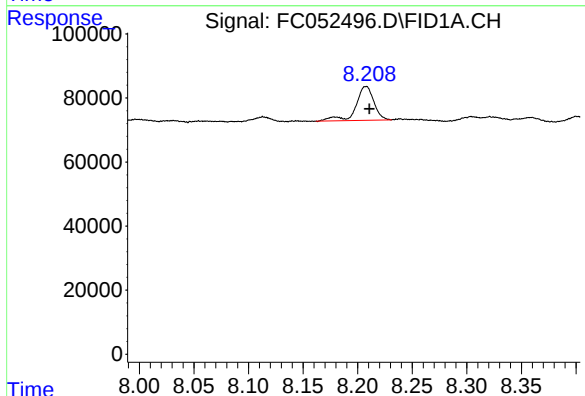


#6 n-Tetradecane (C14)

R.T.: 8.208 min  
Delta R.T.: -0.003 min  
Response: 121076  
Conc: 1.00 ug/ml

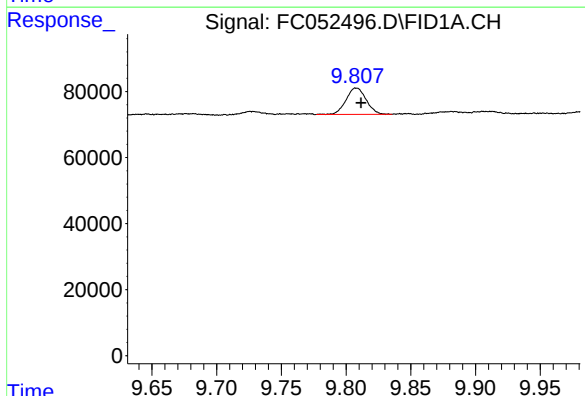


#7 n-Hexadecane (C16)

R.T.: 9.808 min  
Delta R.T.: -0.004 min  
Response: 86230  
Conc: 0.72 ug/ml

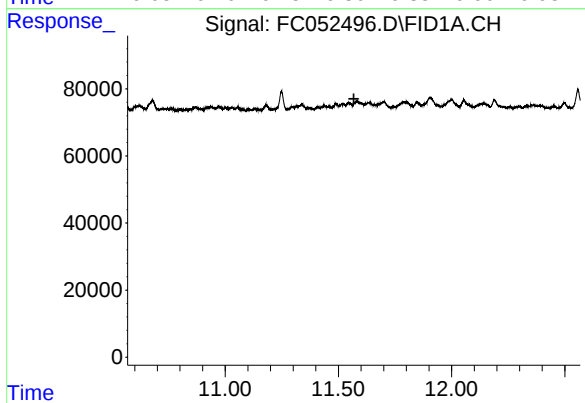

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 11.568 min  
Response: 0  
Conc: N.D.

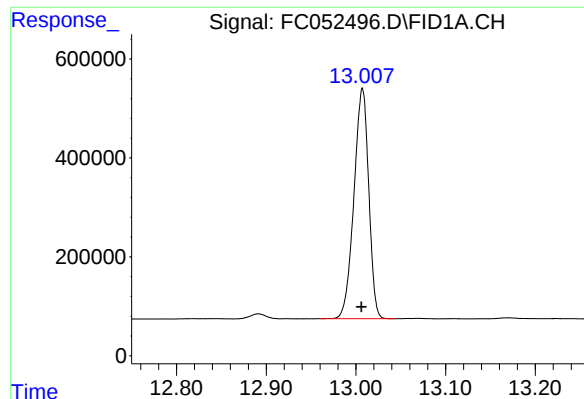

#12 1-chlorooctadecane (SURR)

R.T.: 13.007 min  
Delta R.T.: 0.001 min  
Response: 5329032  
Conc: 49.41 ug/ml

Instrument :  
FID\_C  
ClientSampleId :

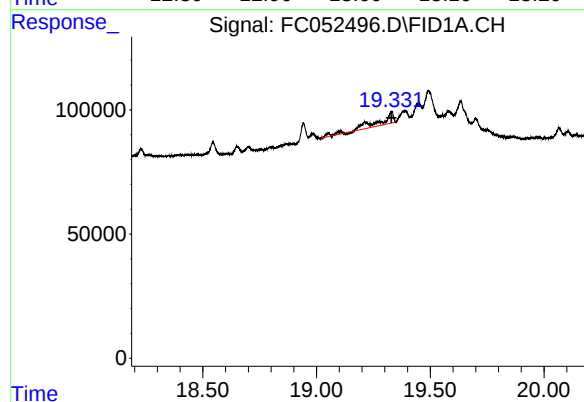

#19 n-Tetratriacontane (C34)

R.T.: 19.332 min  
Delta R.T.: 0.002 min  
Response: 205440  
Conc: 2.24 ug/ml