

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031821AL\
 Data File : FC052514.D
 Signal(s) : FID1A.CH
 Acq On : 18 Mar 2021 17:50
 Operator : DD\AJ
 Sample : M1687-01DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 AUD-1052-1053DL

Manual Integrations
 APPROVED

Ankita
 3/19/2021 11:09:32 AM

Integration File: autoint1.e
 Quant Time: Mar 19 01:40:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 03:47:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.005	677343	6.280 ug/mlm
Spiked Amount 50.000		Recovery =	12.56%
Target Compounds			

(f)=RT Delta > 1/2 Window		(m)=manual int.	

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031821AL\
Data File : FC052514.D
Signal(s) : FID1A.CH
Acq On : 18 Mar 2021 17:50
Operator : DD\AJ
Sample : M1687-01DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
AUD-1052-1053DL


Manual Integrations
APPROVED

Ankita
3/19/2021 11:09:32 AM

Integration File: autoint1.e
Quant Time: Mar 19 01:40:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 03:47:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

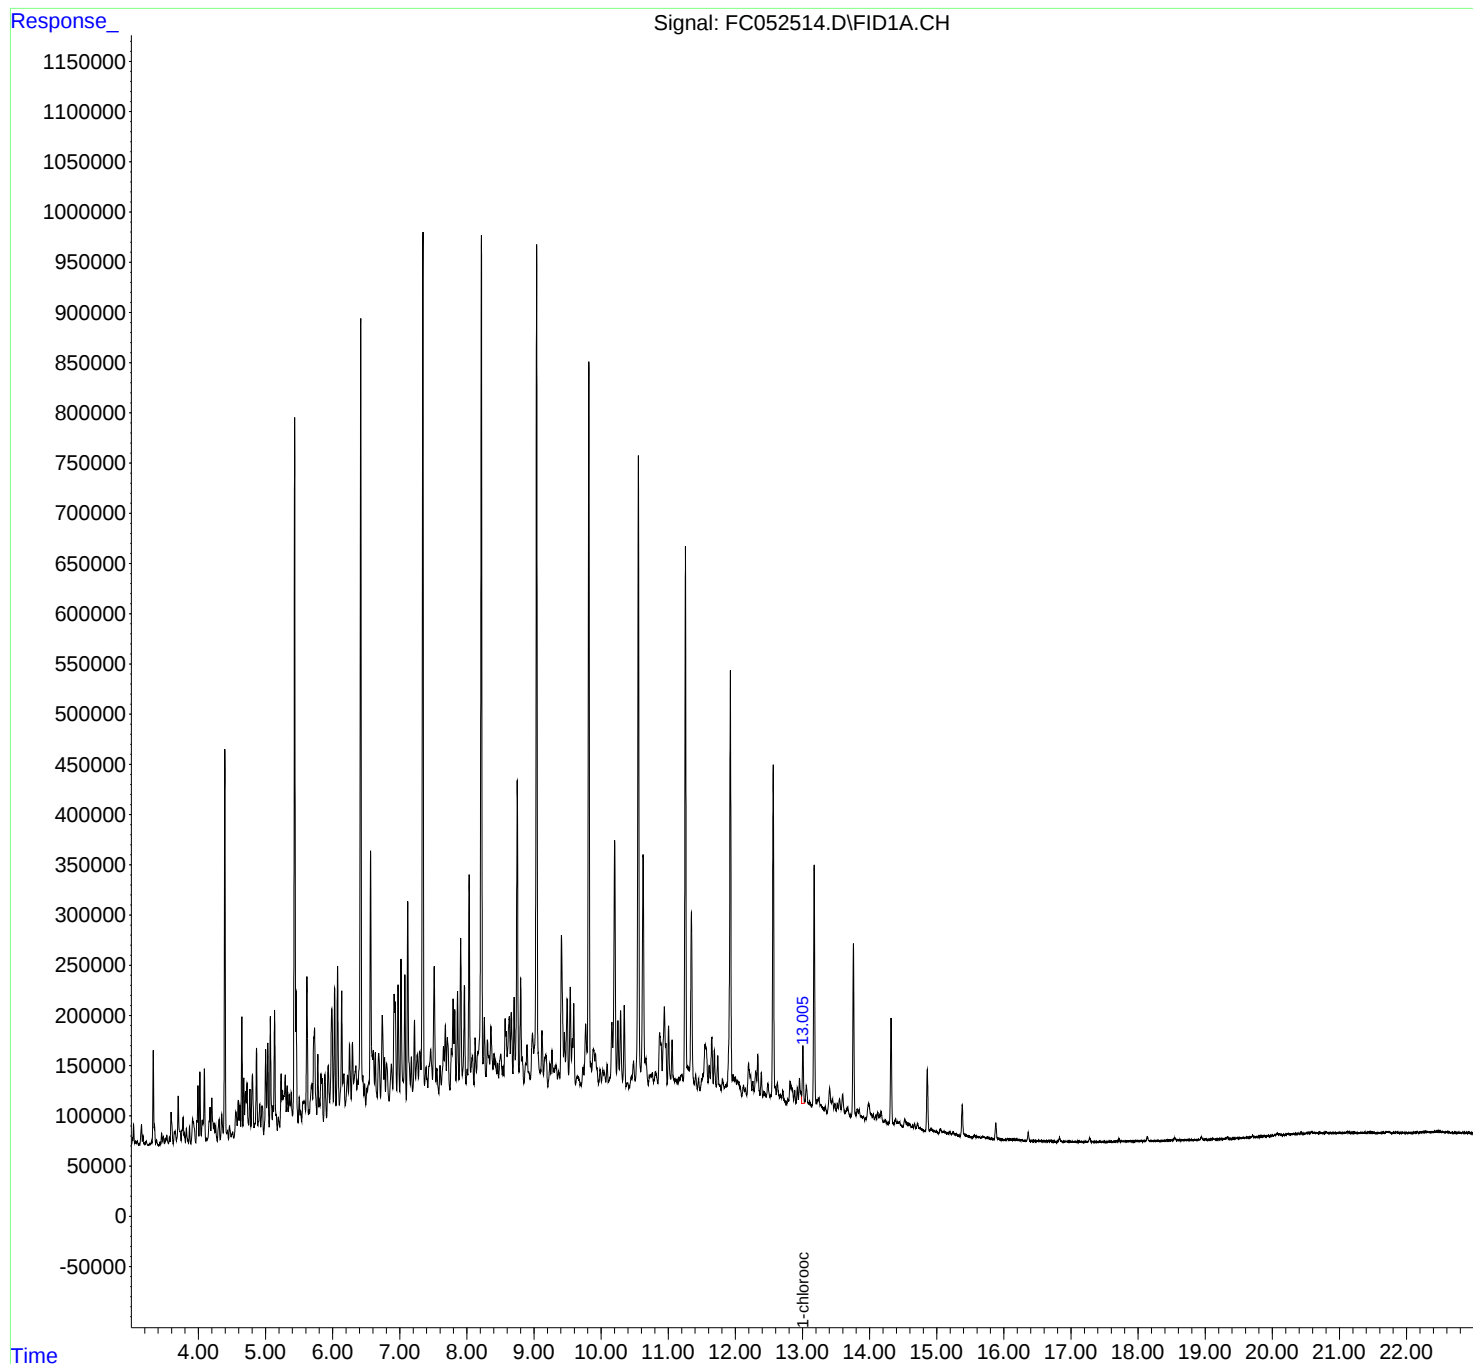

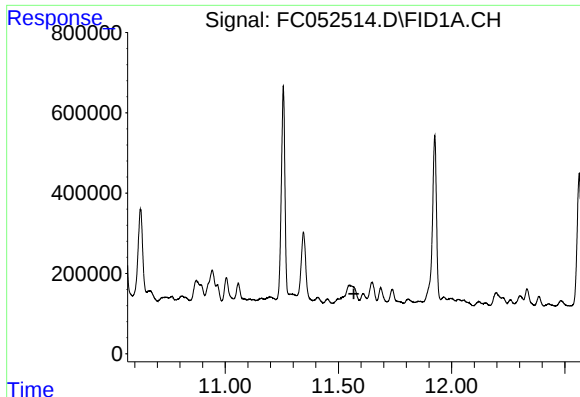


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.568 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
AUD-1052-1053DL

Manual Integrations
APPROVED

Ankita
3/19/2021 11:09:32 AM

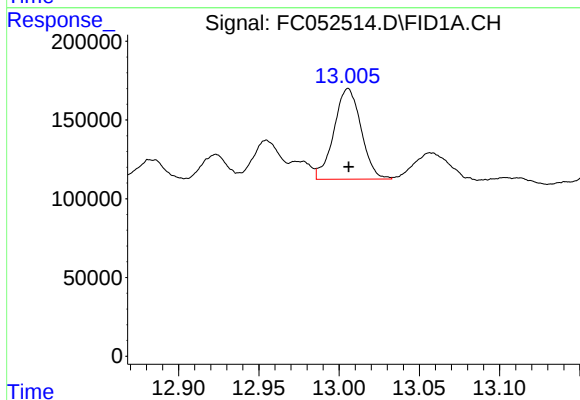

#12 1-chlorooctadecane (SURR)

R.T.: 13.005 min
Delta R.T.: 0.000 min
Response: 677343
Conc: 6.28 ug/ml m