

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031921AL\
 Data File : FC052559.D
 Signal(s) : FID1A.CH
 Acq On : 19 Mar 2021 21:54
 Operator : DD\AJ
 Sample : M1720-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 20 00:09:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 03:47:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.005	5719089	53.024 ug/ml
Spiked Amount 50.000		Recovery =	106.05%
Target Compounds			
4) T n-Dodecane (C12)	6.410	116359	0.969 ug/ml
6) T n-Tetradecane (C14)	8.212	1420522	11.745 ug/ml
7) T n-Hexadecane (C16)	9.806	96753	0.804 ug/ml
8) T n-Octadecane (C18)	11.247	85459	0.677 ug/ml
14) T n-Tetracosane (C24)	14.855	99169	0.794 ug/ml
15) T n-Hexacosane (C26)	15.876	96846	0.804 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC031921AL\
Data File : FC052559.D
Signal(s) : FID1A.CH
Acq On : 19 Mar 2021 21:54
Operator : DD\AJ
Sample : M1720-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 20 00:09:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 03:47:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

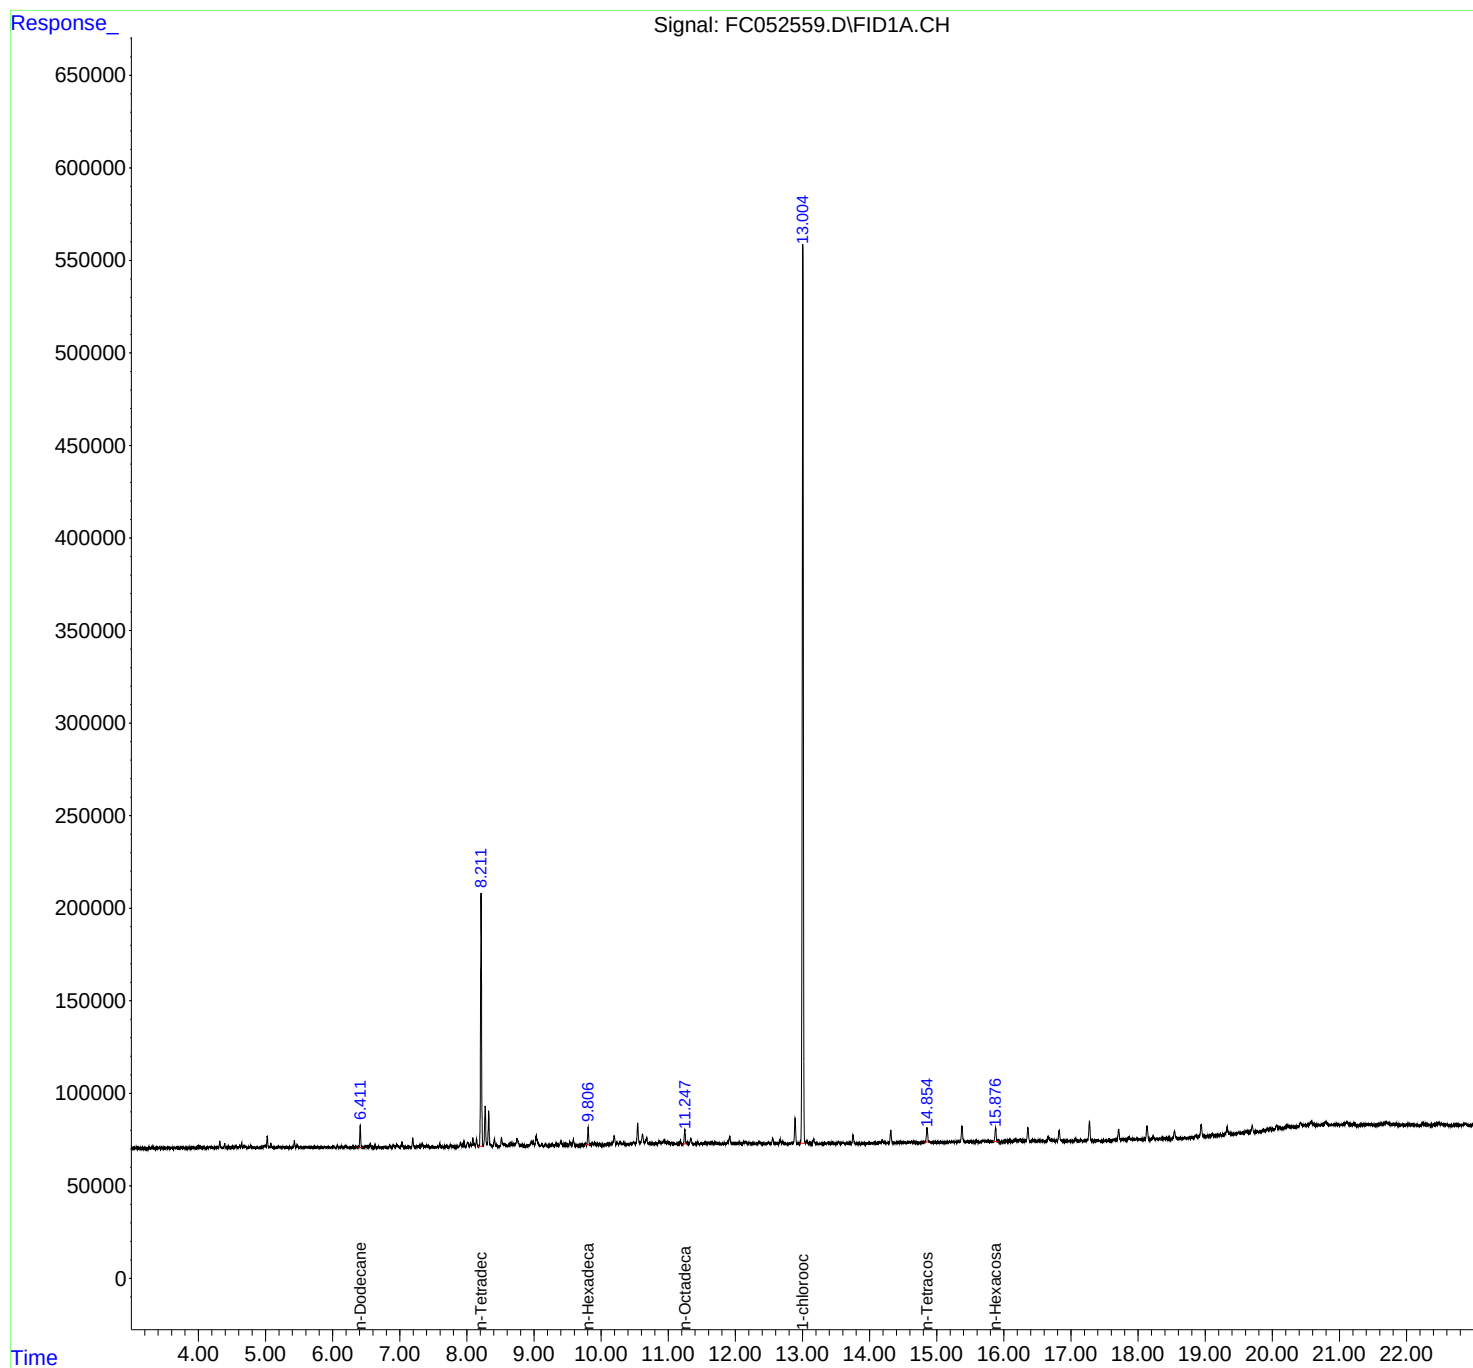


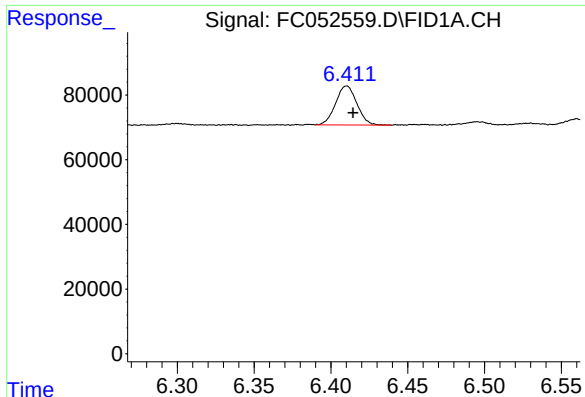

#4 n-Dodecane (C12)


R.T.: 6.410 min
Delta R.T.: -0.004 min
Response: 116359
Conc: 0.97 ug/ml

Instrument :
FID_C
ClientSampleId :

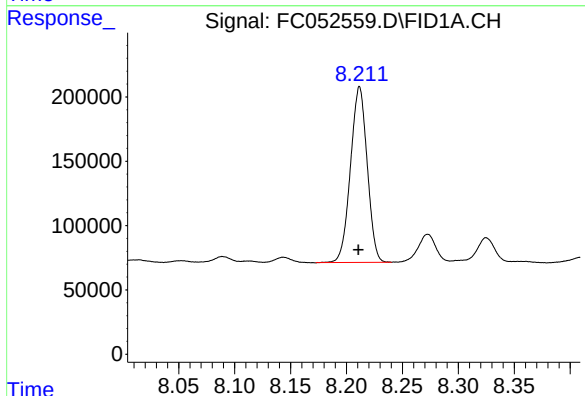


#6 n-Tetradecane (C14)

R.T.: 8.212 min
Delta R.T.: 0.001 min
Response: 1420522
Conc: 11.75 ug/ml

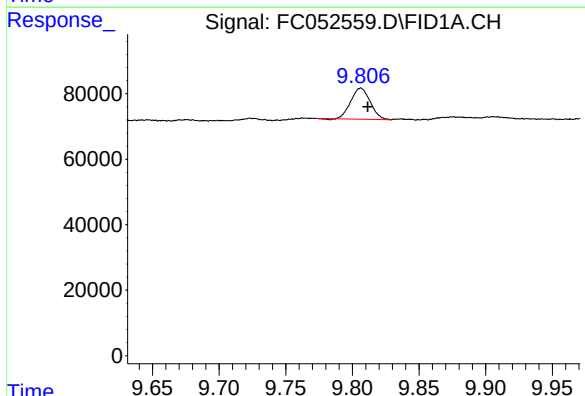


#7 n-Hexadecane (C16)

R.T.: 9.806 min
Delta R.T.: -0.005 min
Response: 96753
Conc: 0.80 ug/ml

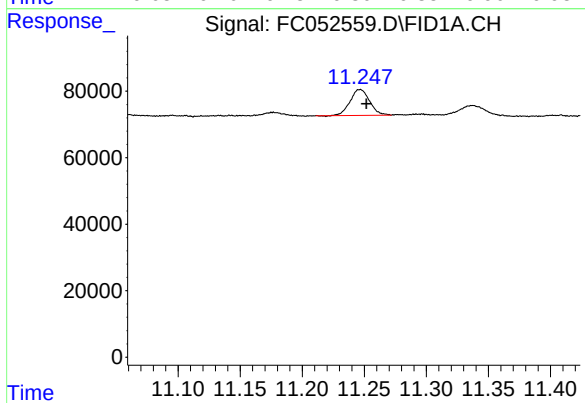

#8 n-Octadecane (C18)


R.T.: 11.247 min
Delta R.T.: -0.005 min
Response: 85459
Conc: 0.68 ug/ml

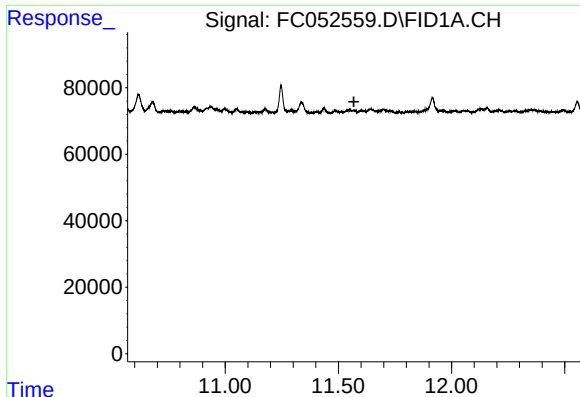

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.568 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

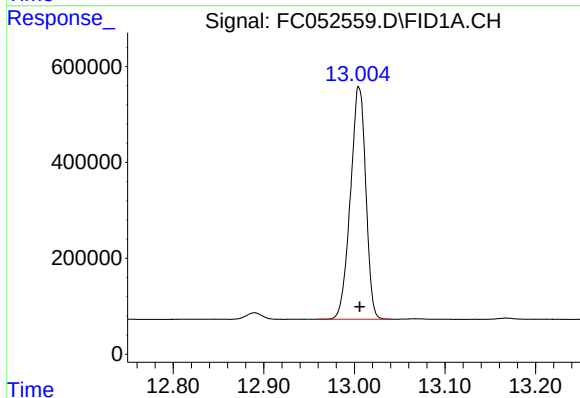


#12 1-chlorooctadecane (SURR)

R.T.: 13.005 min
Delta R.T.: 0.000 min
Response: 5719089
Conc: 53.02 ug/ml

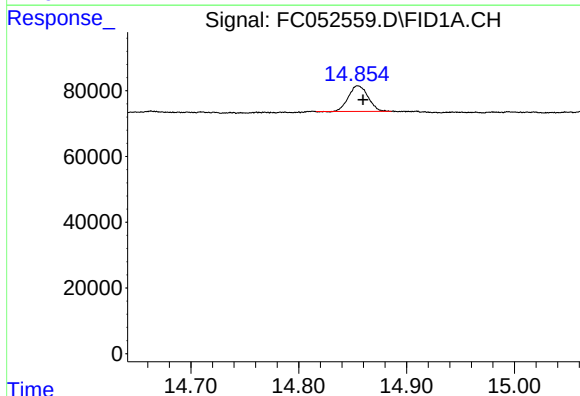

#14 n-Tetracosane (C24)

R.T.: 14.855 min
Delta R.T.: -0.005 min
Response: 99169
Conc: 0.79 ug/ml

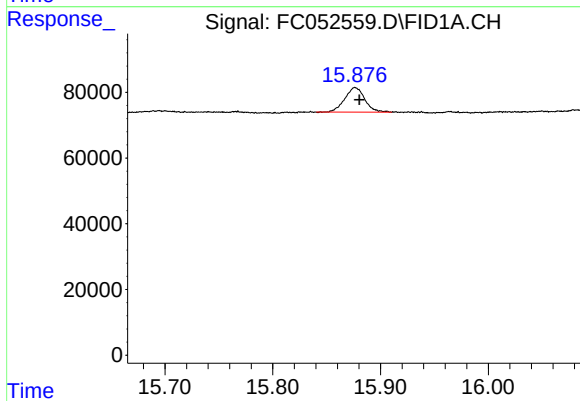

#15 n-Hexacosane (C26)

R.T.: 15.876 min
Delta R.T.: -0.004 min
Response: 96846
Conc: 0.80 ug/ml