

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032420AL\
 Data File : FC046476.D
 Signal(s) : FID1A.CH
 Acq On : 24 Mar 2020 16:16
 Operator : DD\AJ
 Sample : L2020-0D
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 25 00:53:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 032320.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 24 12:45:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.759	7340626	67.466 ug/ml
Spiked Amount 50.000		Recovery =	134.93%
12) S 1-chlorooctadecane (S...	13.176	5999945	69.623 ug/ml
Spiked Amount 50.000		Recovery =	139.25%
Target Compounds			
15) T n-Hexacosane (C26)	16.030	549551	5.356 ug/ml
16) T n-Octacosane (C28)	16.974	1462237	14.367 ug/ml
17) T n-Tricontane (C30)	17.859	1608209	16.415 ug/ml
18) T n-Dotriacontane (C32)	18.684	759362	9.057 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032420AL\
Data File : FC046476.D
Signal(s) : FID1A.CH
Acq On : 24 Mar 2020 16:16
Operator : DD\AJ
Sample : L2020-0D
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 25 00:53:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 032320.M
Quant Title : GC Extractables
QLast Update : Tue Mar 24 12:45:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

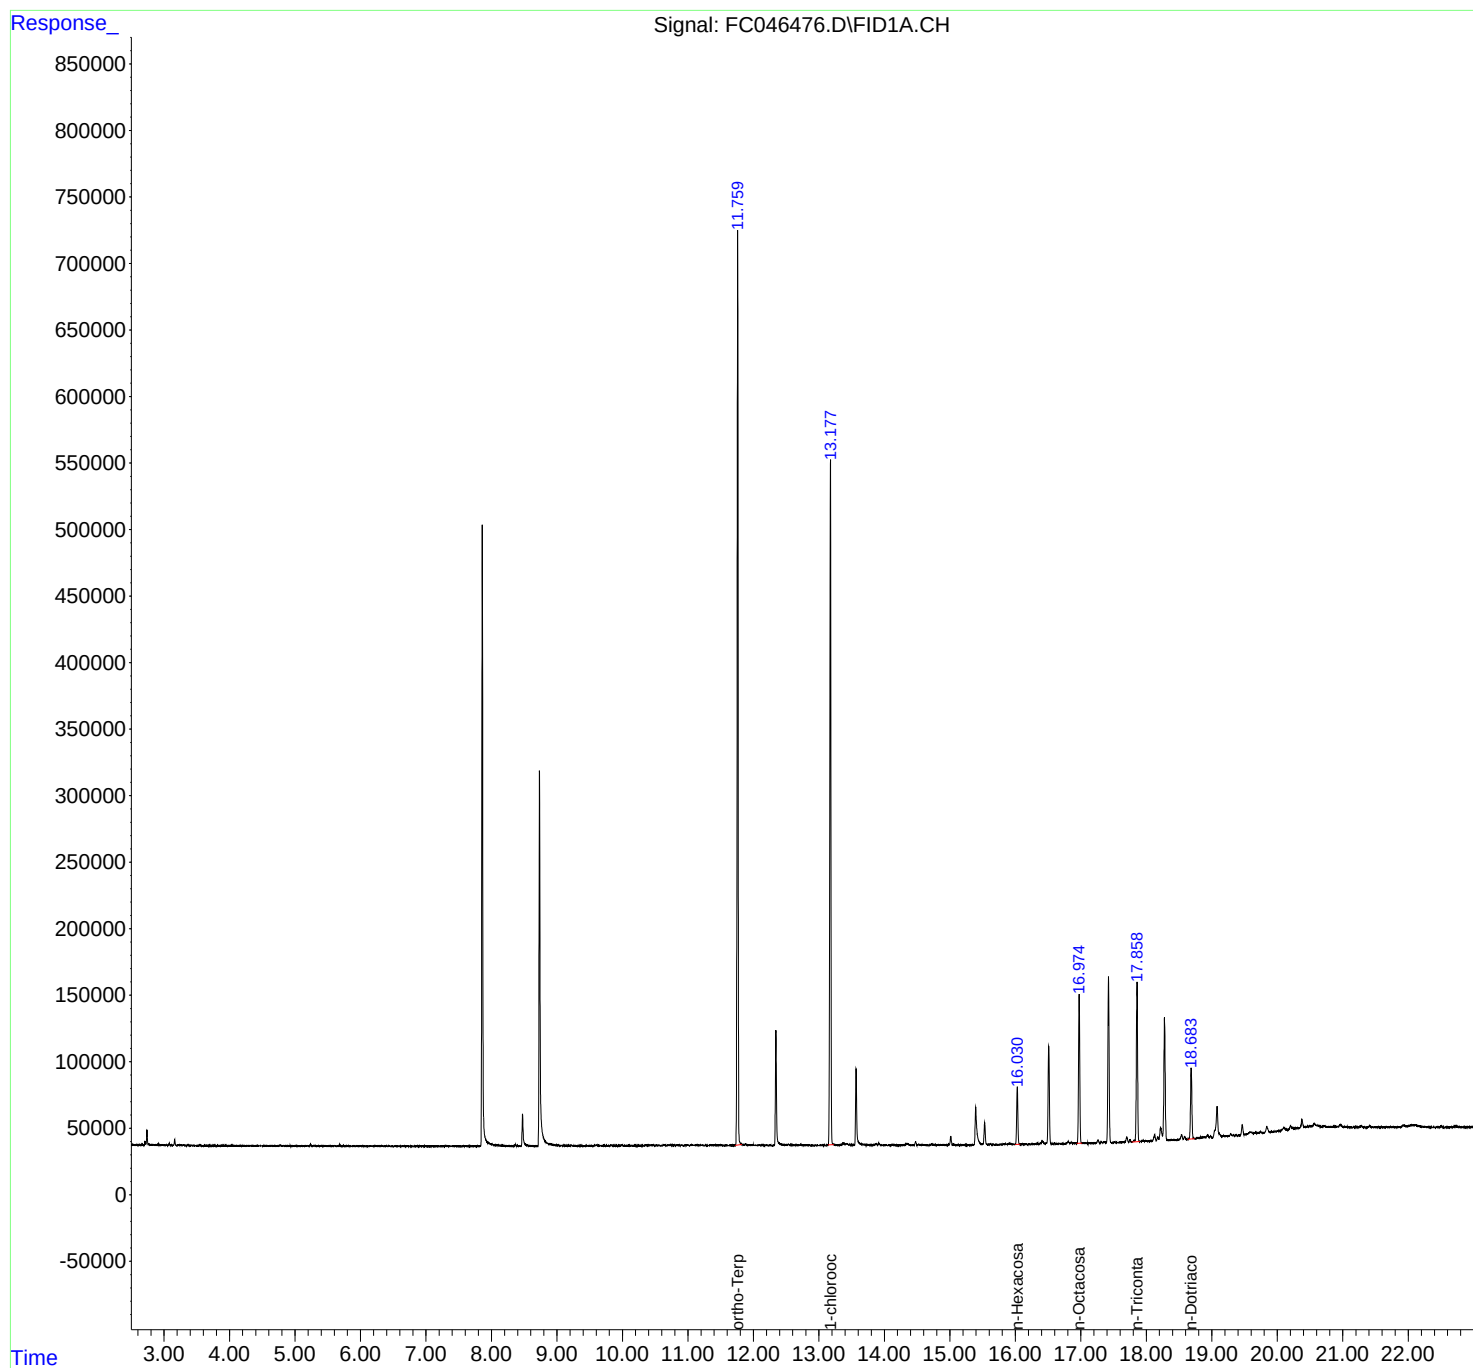


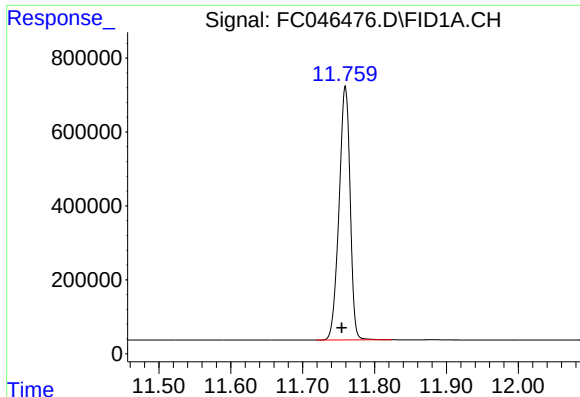

#9 ortho-Terphenyl (SURR)


R.T.: 11.759 min
Delta R.T.: 0.005 min
Response: 7340626
Conc: 67.47 ug/ml

Instrument :
FID_C
ClientSampleId :

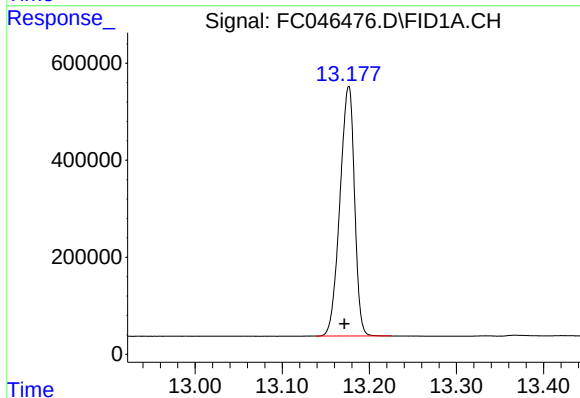


#12 1-chlorooctadecane (SURR)

R.T.: 13.176 min
Delta R.T.: 0.005 min
Response: 5999945
Conc: 69.62 ug/ml

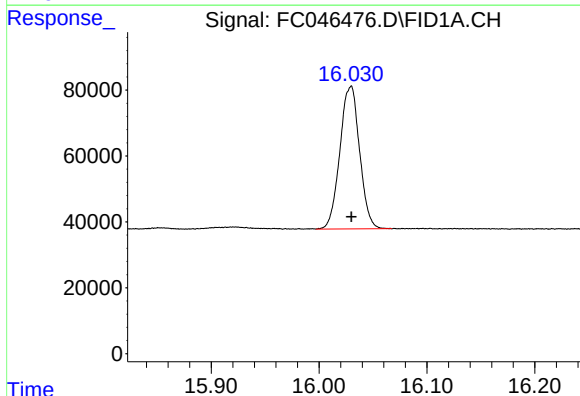


#15 n-Hexacosane (C26)

R.T.: 16.030 min
Delta R.T.: 0.000 min
Response: 549551
Conc: 5.36 ug/ml

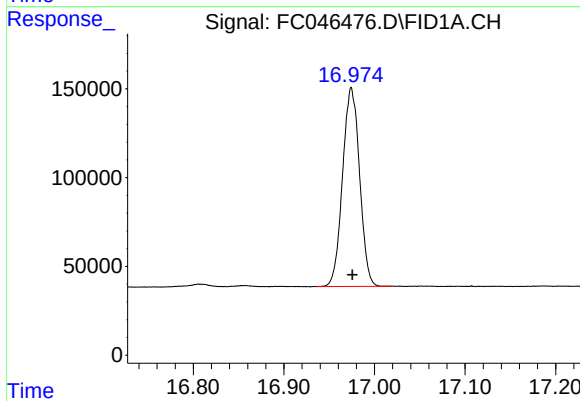

#16 n-Octacosane (C28)


R.T.: 16.974 min
Delta R.T.: -0.001 min
Response: 1462237
Conc: 14.37 ug/ml

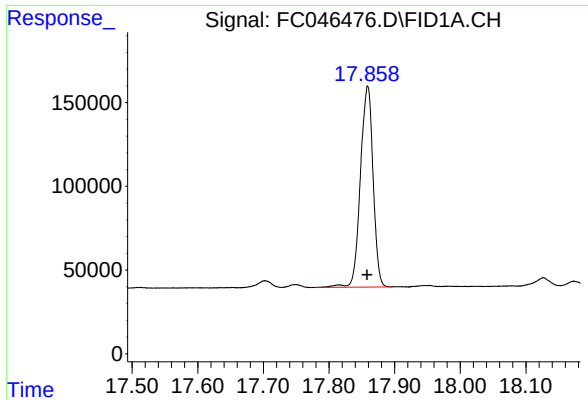

#17 n-Tricontane (C30)

R.T.: 17.859 min
Delta R.T.: 0.001 min
Response: 1608209
Conc: 16.41 ug/ml

Instrument :
FID_C
ClientSampleId :

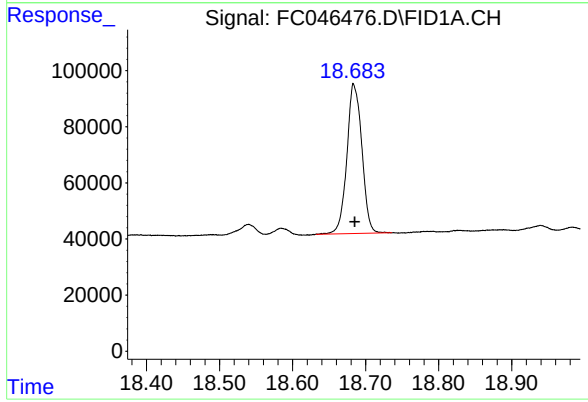

#18 n-Dotriacontane (C32)

R.T.: 18.684 min
Delta R.T.: -0.001 min
Response: 759362
Conc: 9.06 ug/ml