

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032521AL\
 Data File : FC052727.D
 Signal(s) : FID1A.CH
 Acq On : 25 Mar 2021 21:29
 Operator : DD\AJ
 Sample : M1773-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 26 01:07:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 031721.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 03:47:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.569	5048428	37.663 ug/ml
Spiked Amount 50.000		Recovery =	75.33%
12) S 1-chlorooctadecane (S...	13.006	3896826	36.129 ug/ml
Spiked Amount 50.000		Recovery =	72.26%
Target Compounds			
10) T n-Eicosane (C20)	12.616f	152968	1.198 ug/ml
14) T n-Tetracosane (C24)	14.833	81773	0.655 ug/ml
17) T n-Tricontane (C30)	17.718	132183	1.213 ug/ml
18) T n-Dotriacontane (C32)	18.543	185305	1.847 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032521AL\
Data File : FC052727.D
Signal(s) : FID1A.CH
Acq On : 25 Mar 2021 21:29
Operator : DD\AJ
Sample : M1773-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 01:07:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 031721.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 03:47:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

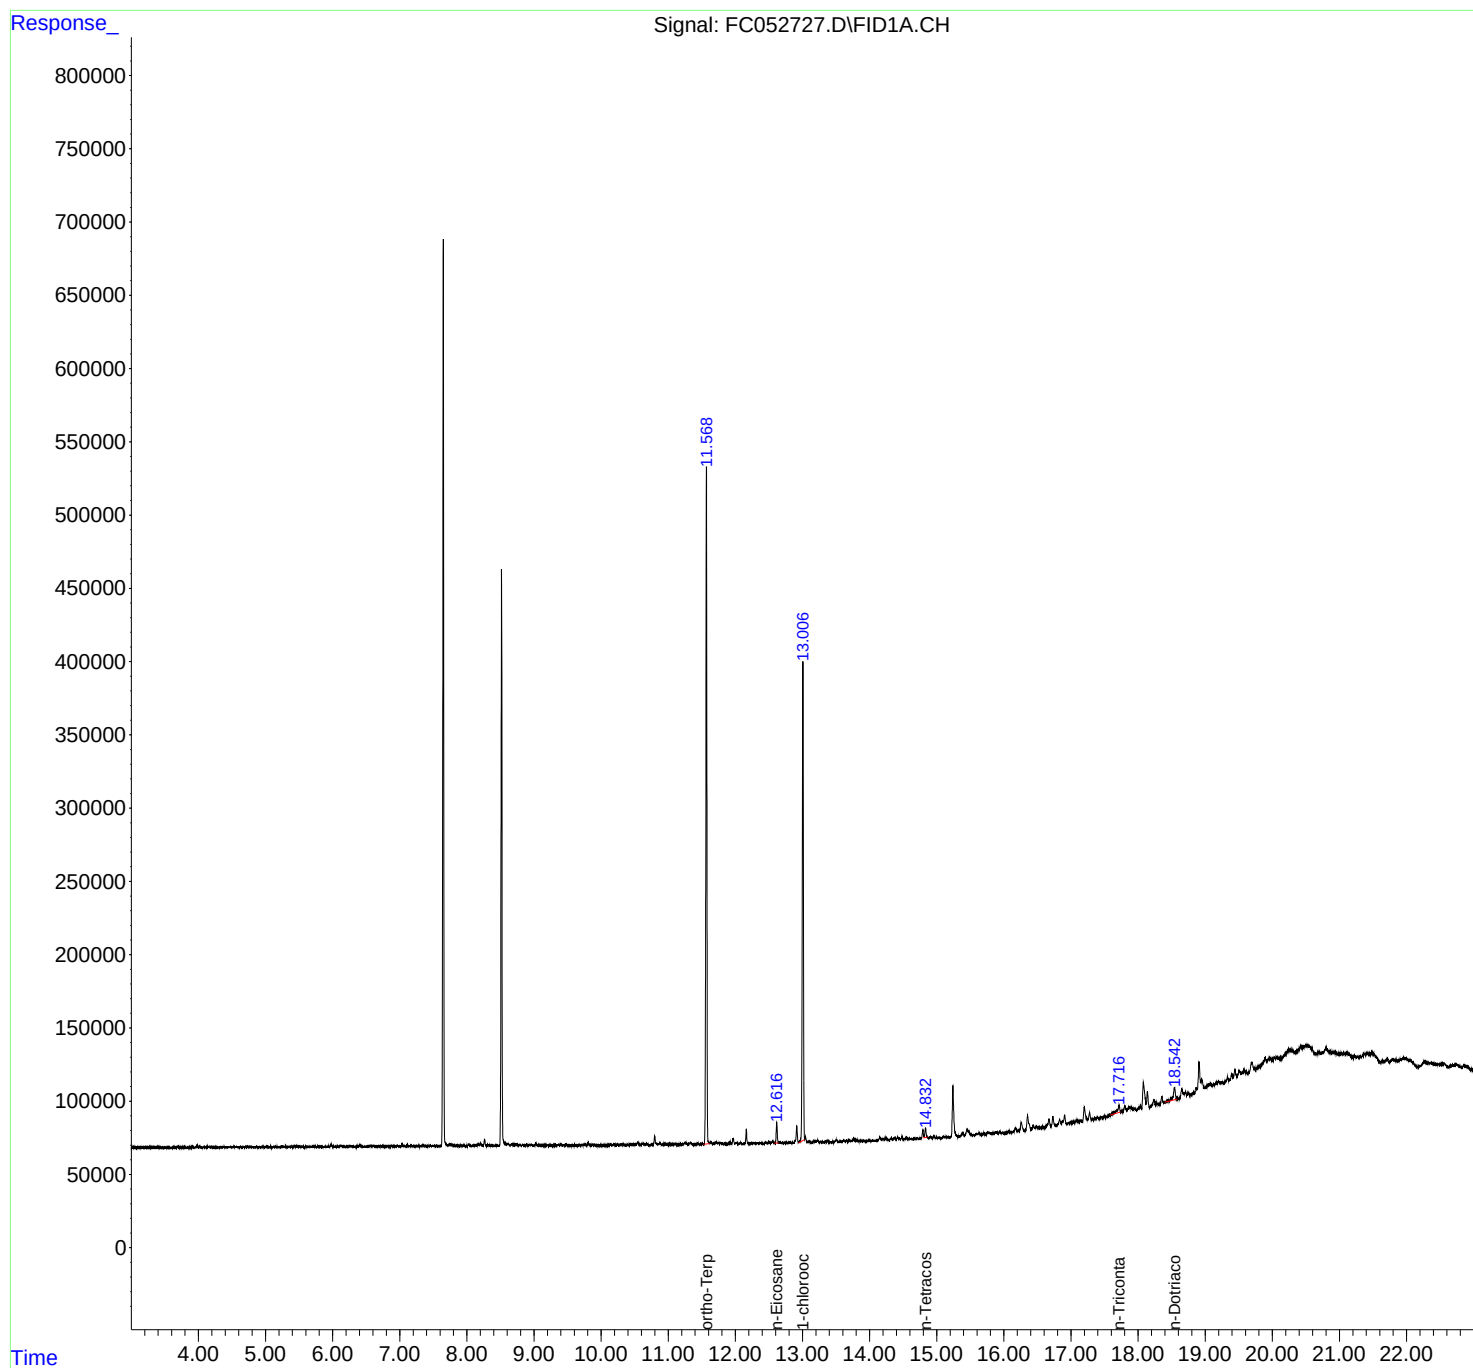


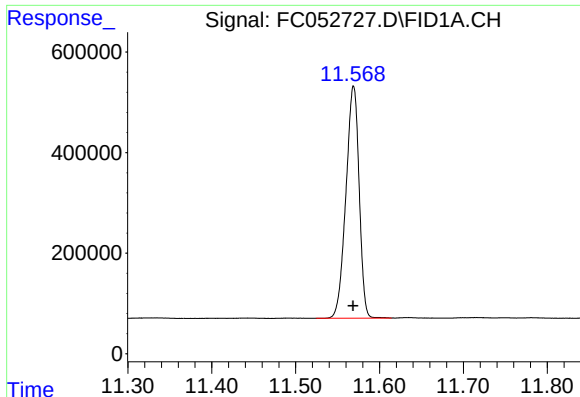

#9 ortho-Terphenyl (SURR)


R.T.: 11.569 min
Delta R.T.: 0.000 min
Response: 5048428
Conc: 37.66 ug/ml

Instrument :
FID_C
ClientSampleId :

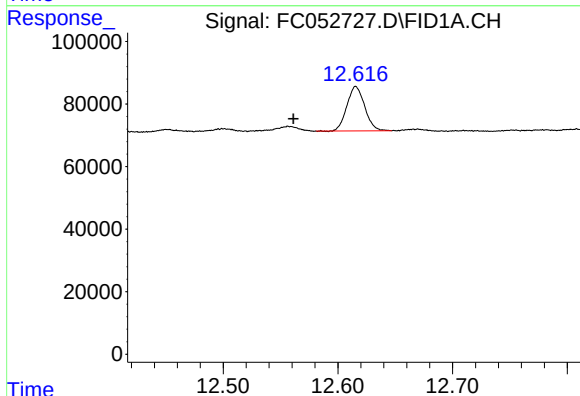


#10 n-Eicosane (C20)

R.T.: 12.616 min
Delta R.T.: 0.055 min
Response: 152968
Conc: 1.20 ug/ml

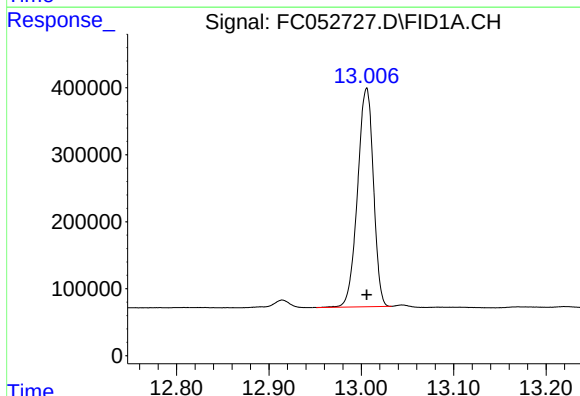


#12 1-chlorooctadecane (SURR)

R.T.: 13.006 min
Delta R.T.: 0.000 min
Response: 3896826
Conc: 36.13 ug/ml

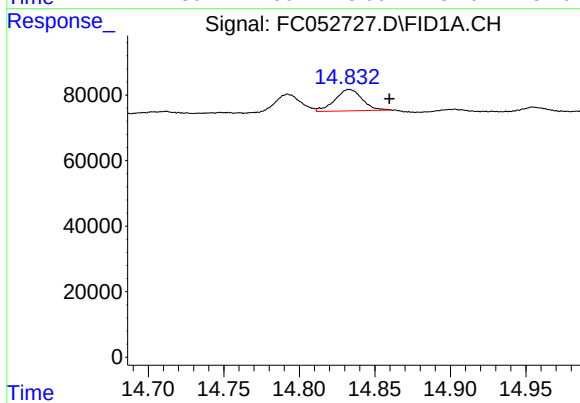

#14 n-Tetracosane (C24)


R.T.: 14.833 min
Delta R.T.: -0.027 min
Response: 81773
Conc: 0.65 ug/ml

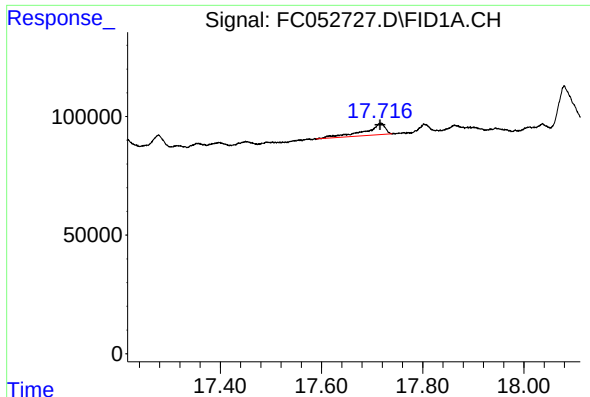

#17 n-Tricontane (C30)

R.T.: 17.718 min
Delta R.T.: 0.002 min
Response: 132183
Conc: 1.21 ug/ml

Instrument :
FID_C
ClientSampleId :

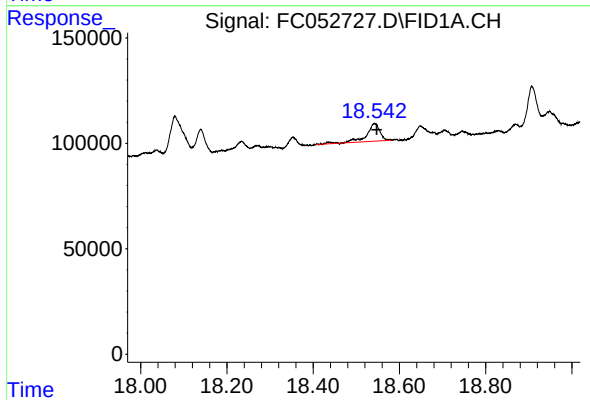

#18 n-Dotriacontane (C32)

R.T.: 18.543 min
Delta R.T.: -0.005 min
Response: 185305
Conc: 1.85 ug/ml