

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC032521AL\  
 Data File : FC052746.D  
 Signal(s) : FID1A.CH  
 Acq On : 26 Mar 2021 9:27  
 Operator : DD\AJ  
 Sample : M1802-01  
 Misc :  
 ALS Vial : 36 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 SB-1S-(0.5-1)

Integration File: autoint1.e  
 Quant Time: Mar 26 10:42:30 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Alaphatic EPH 031721.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Mar 17 03:47:28 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.006 | 3989749    | 36.991 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 73.98%       |
| Target Compounds               |        |            |              |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC032521AL\  
Data File : FC052746.D  
Signal(s) : FID1A.CH  
Acq On : 26 Mar 2021 9:27  
Operator : DD\AJ  
Sample : M1802-01  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
SB-1S-(0.5-1)

Integration File: autoint1.e  
Quant Time: Mar 26 10:42:30 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Alaphatic EPH 031721.M  
Quant Title : GC Extractables  
QLast Update : Wed Mar 17 03:47:28 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

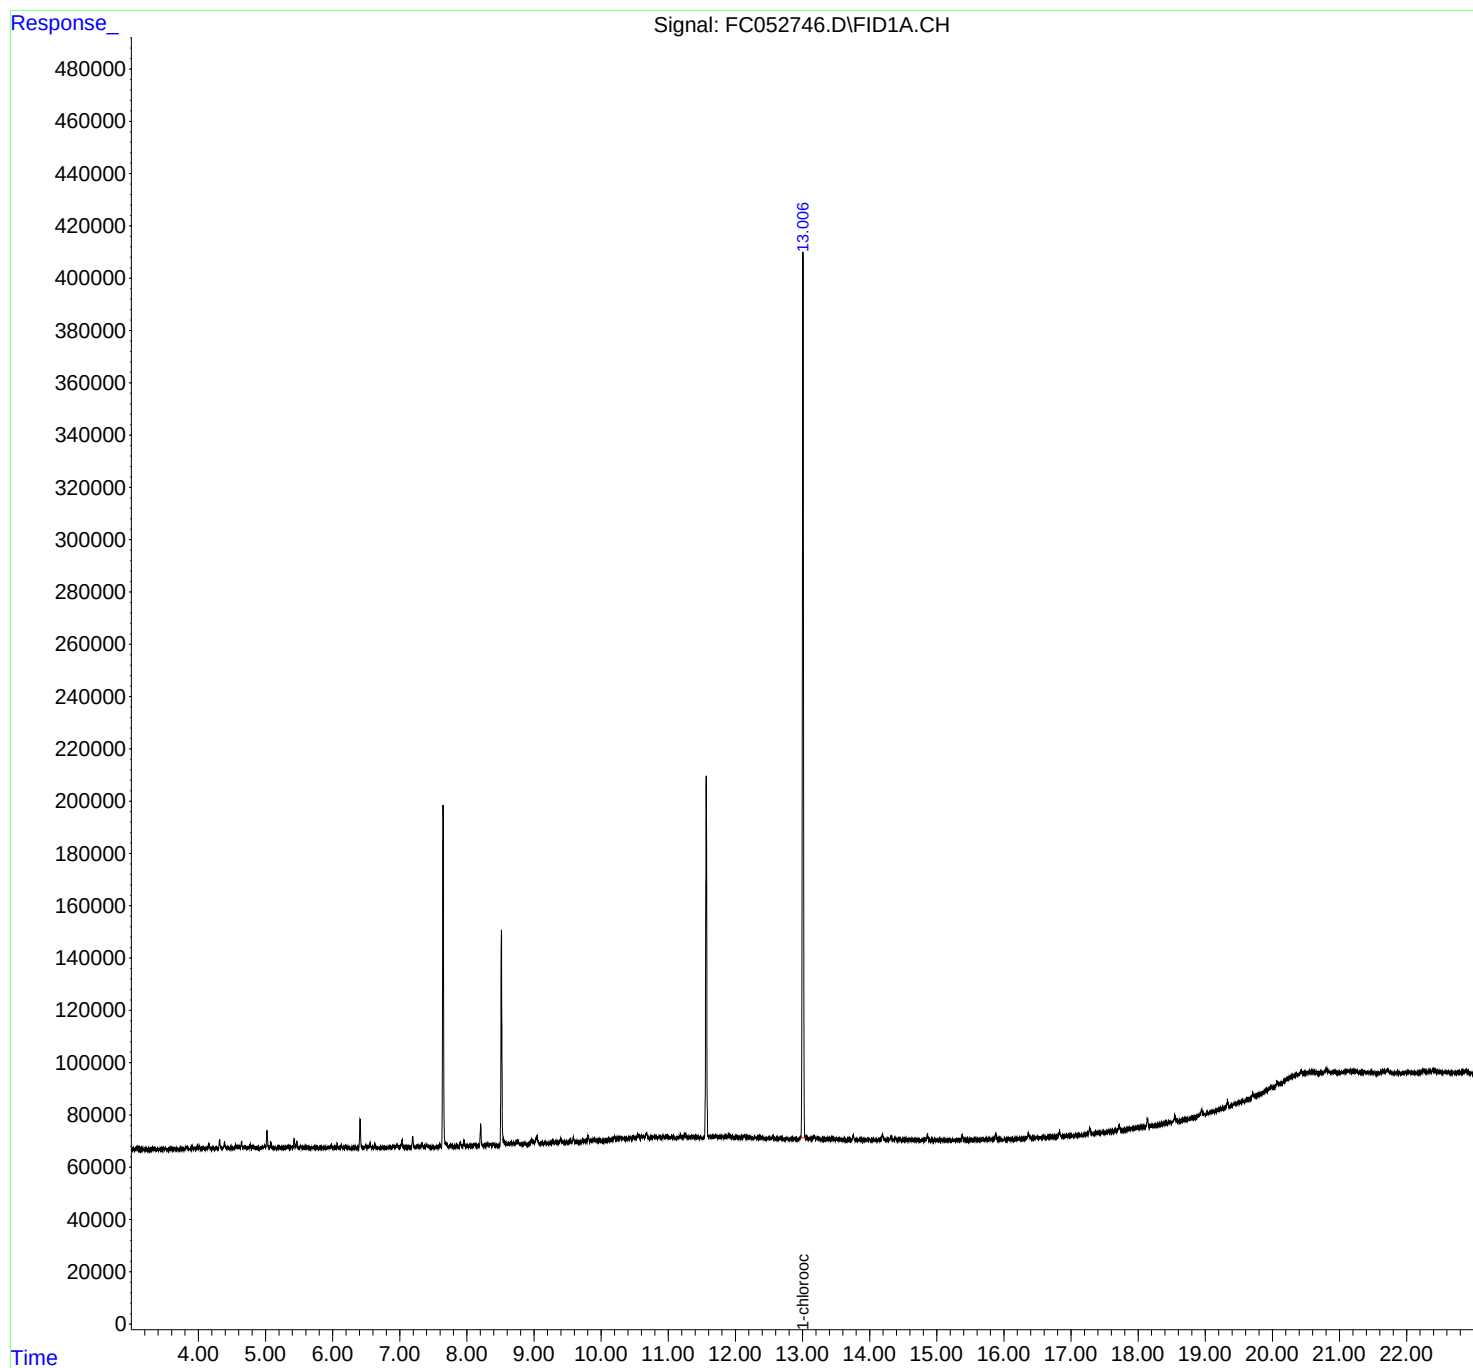


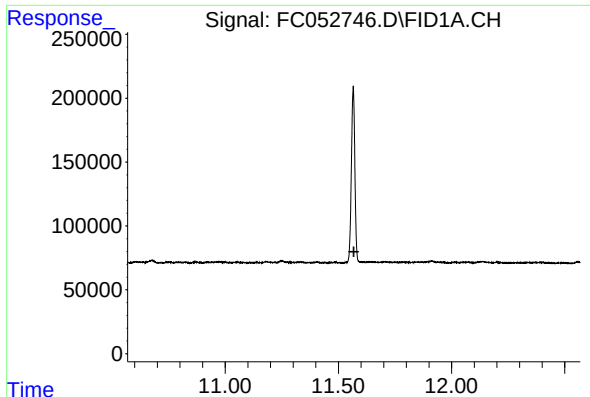

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.568 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :  
SB-1S-(0.5-1)

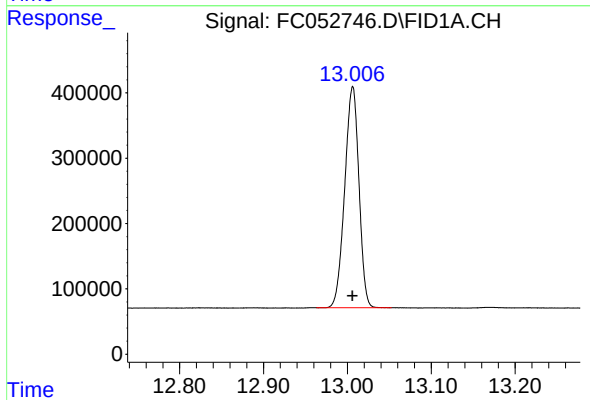

#12 1-chlorooctadecane (SURR)

R.T.: 13.006 min  
Delta R.T.: 0.000 min  
Response: 3989749  
Conc: 36.99 ug/ml