

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032522AL\
 Data File : FC058912.D
 Signal(s) : FID1A.CH
 Acq On : 27 Mar 2022 1:10
 Operator : UA/NP
 Sample : N2103-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 CHRT-20019

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
 Quant Time: Mar 27 03:43:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.101	5836681	40.509 ug/ml
Spiked Amount 50.000		Recovery =	81.02%
12) S 1-chlorooctadecane (S...	12.548	4344889	38.761 ug/mlm
Spiked Amount 50.000		Recovery =	77.52%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032522AL\
Data File : FC058912.D
Signal(s) : FID1A.CH
Acq On : 27 Mar 2022 1:10
Operator : UA/NP
Sample : N2103-09
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
CHRT-20019


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022

Integration File: autoint1.e
Quant Time: Mar 27 03:43:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

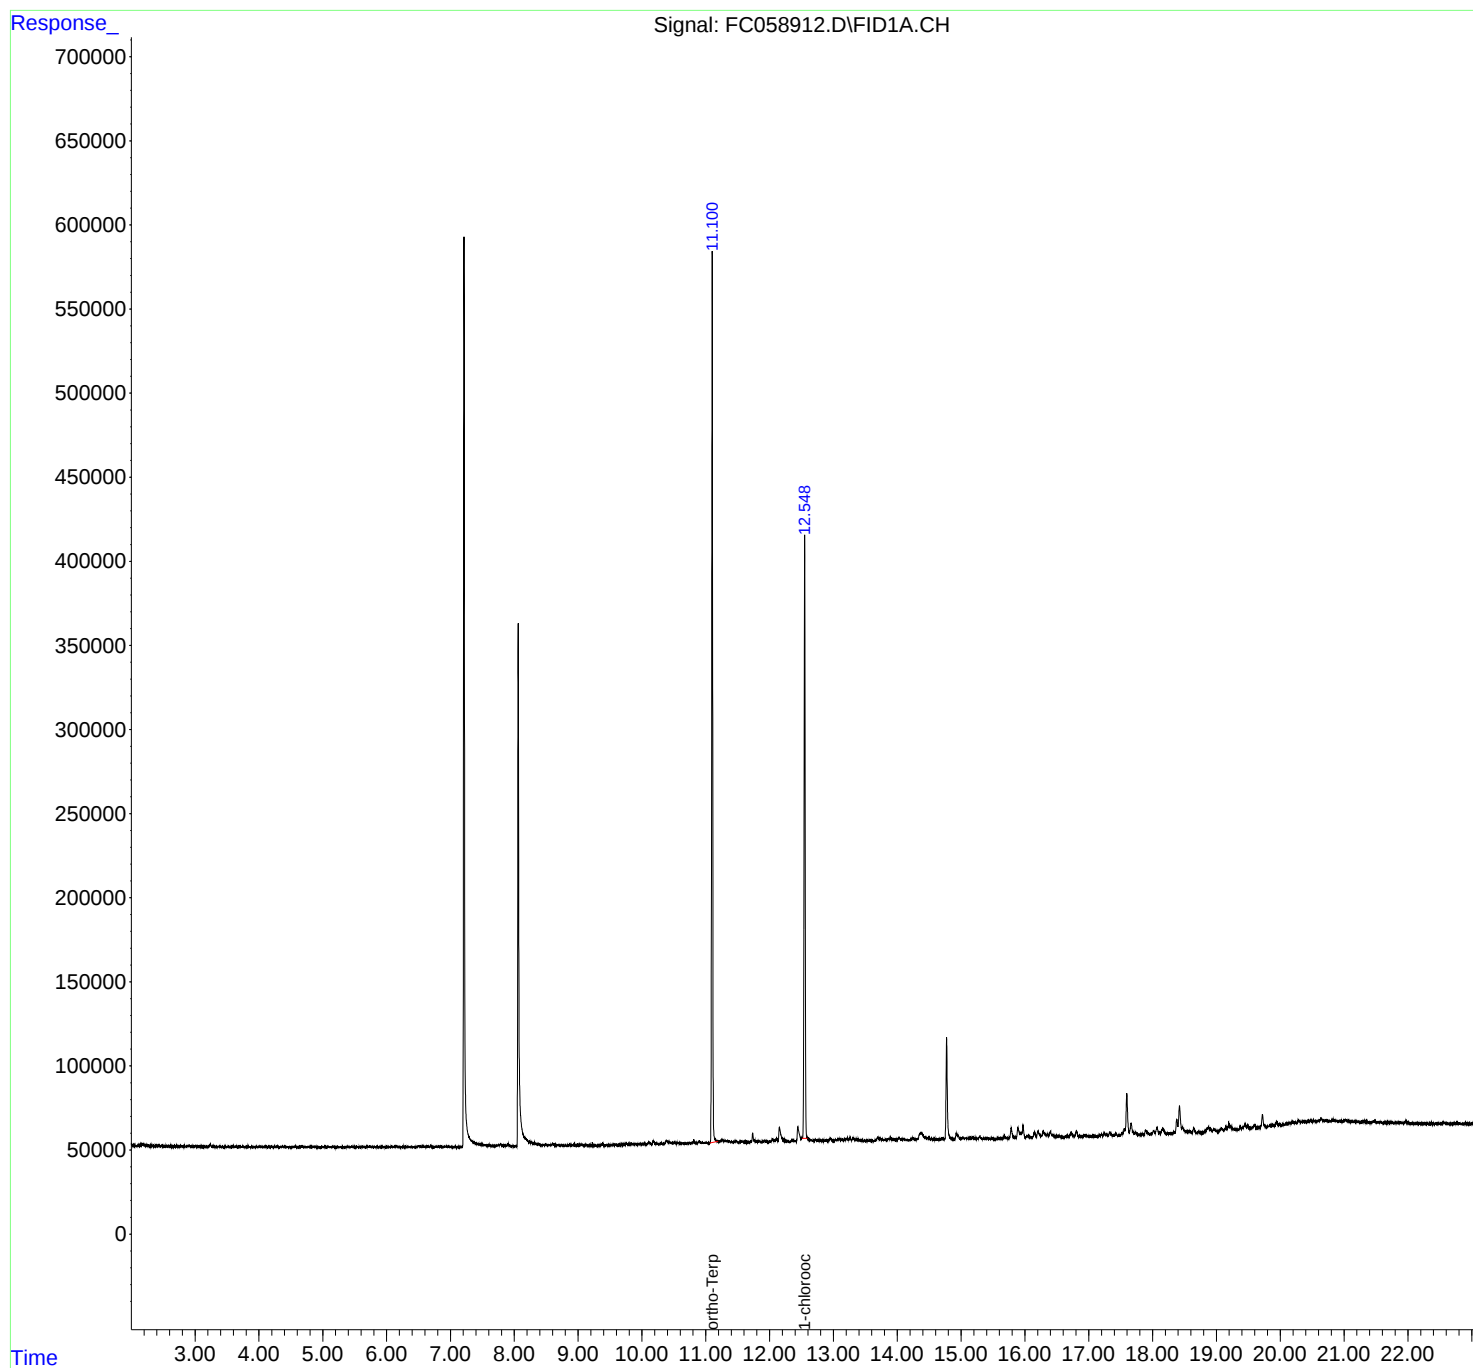

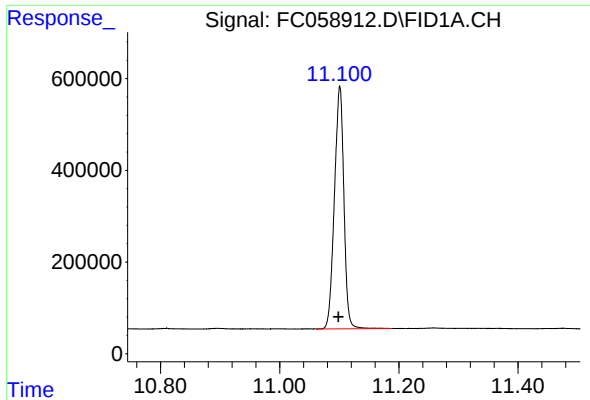


#9 ortho-Terphenyl (SURR)

R.T.: 11.101 min
Delta R.T.: 0.002 min
Response: 5836681
Conc: 40.51 ug/ml

Instrument :
FID_C
ClientSampleId :
CHRT-20019

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/30/2022

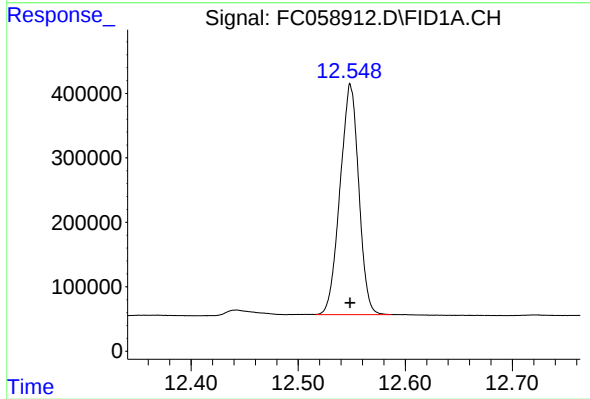

#12 1-chlorooctadecane (SURR)

R.T.: 12.548 min
Delta R.T.: 0.000 min
Response: 4344889
Conc: 38.76 ug/ml m