

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032824AL\
 Data File : FC066127.D
 Signal(s) : FID1A.ch
 Acq On : 28 Mar 2024 11:14
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 29 02:22:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 030424.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 04 13:09:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.455	20289	0.116 ug/ml
11) T	n-Heneicosane (C21)	13.064	41428	0.239 ug/ml
13) T	n-Docosane (C22)	13.645	27866	0.162 ug/ml
14) T	n-Tetracosane (C24)	14.739	32508	0.190 ug/ml
17) T	n-Tricontane (C30)	17.576	32321	0.189 ug/ml
18) T	n-Dotriacontane (C32)	18.402	38122	0.226 ug/ml
20) T	n-Hexatriacontane (C36)	19.967	28311	0.178 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032824AL\
Data File : FC066127.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2024 11:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:22:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 030424.M
Quant Title : GC Extractables
QLast Update : Mon Mar 04 13:09:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

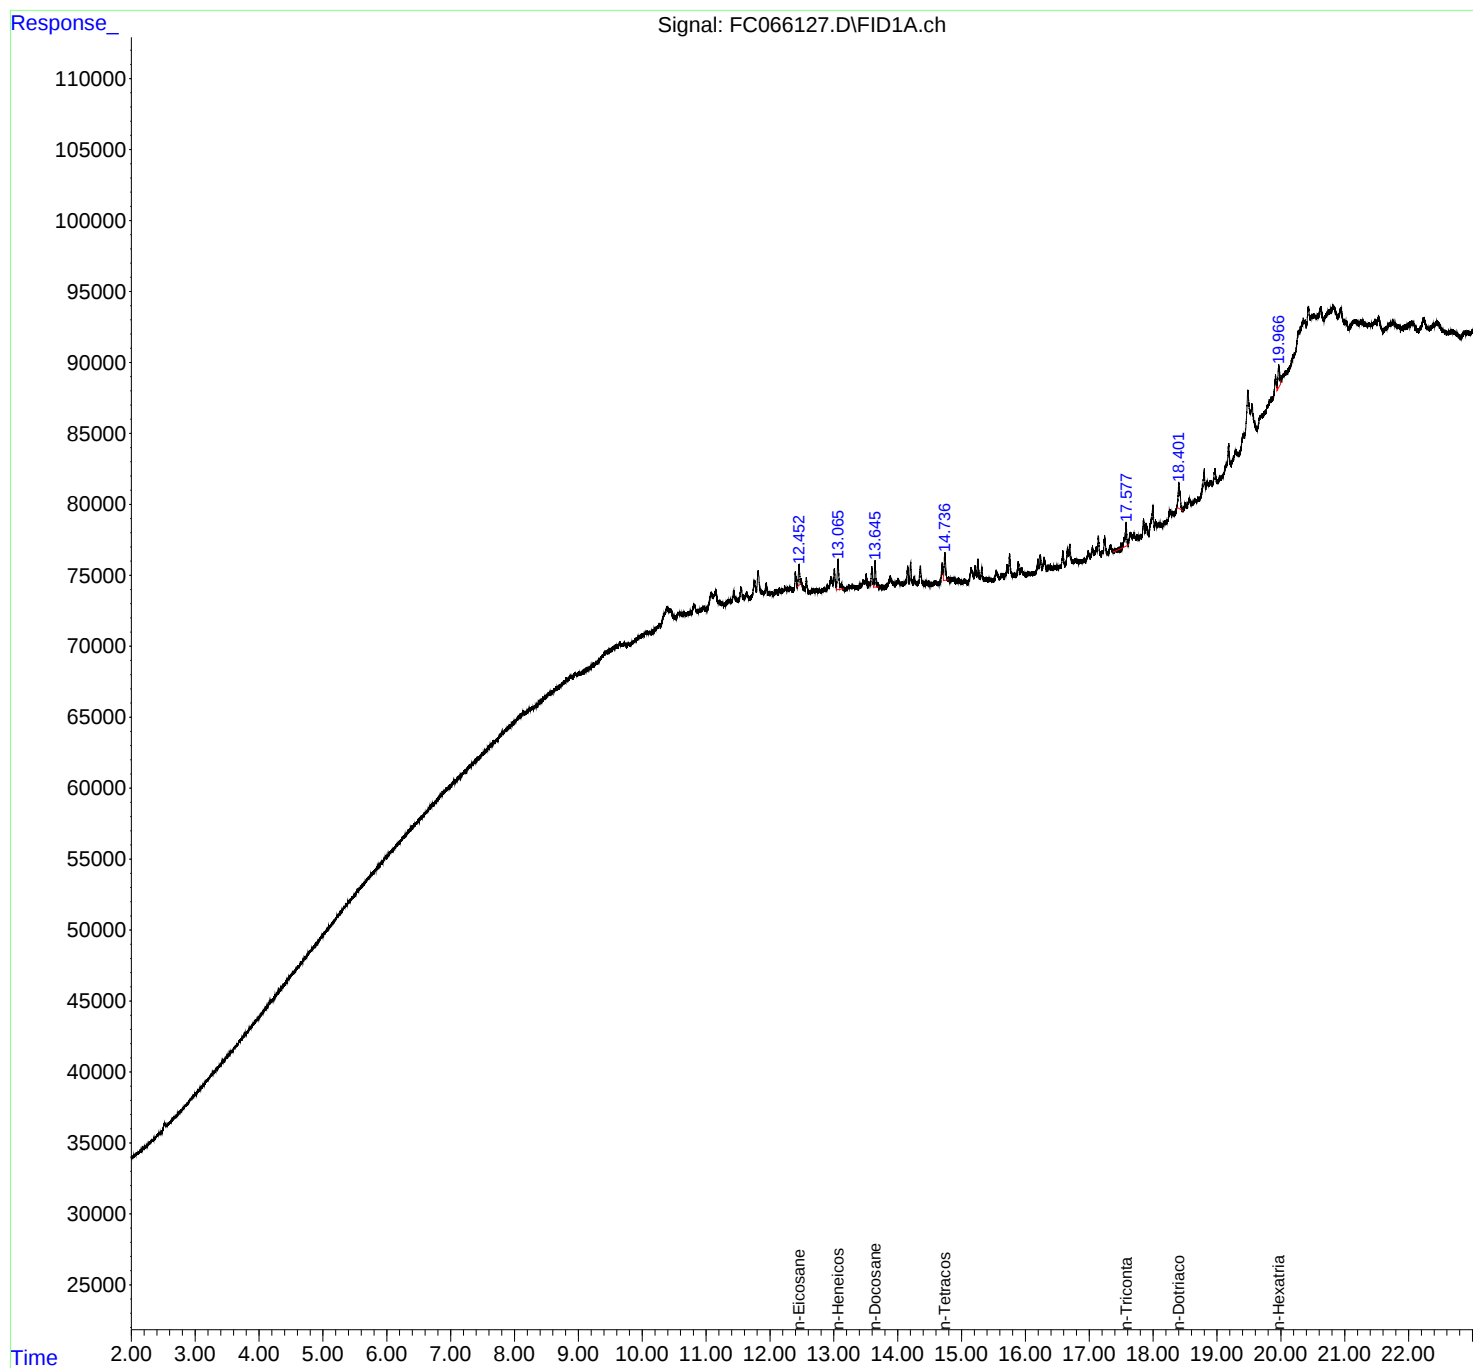


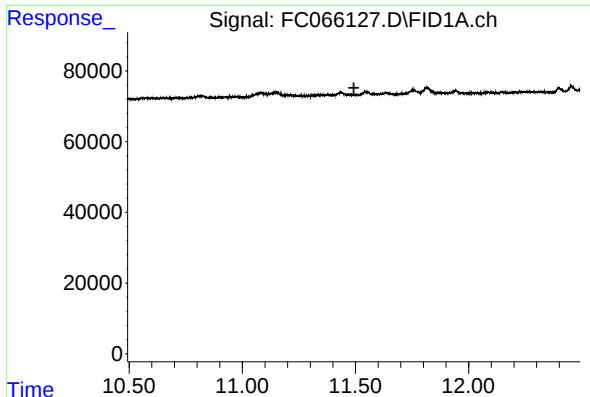

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.493 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

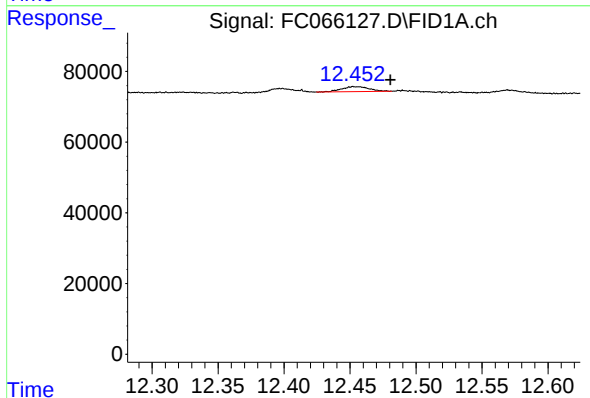


#10 n-Eicosane (C20)

R.T.: 12.455 min
Delta R.T.: -0.026 min
Response: 20289
Conc: 0.12 ug/ml

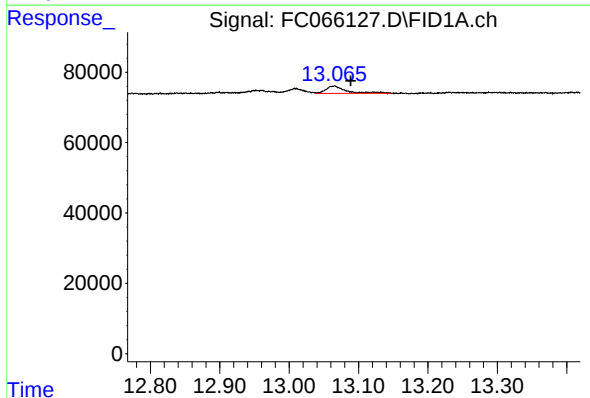


#11 n-Heneicosane (C21)

R.T.: 13.064 min
Delta R.T.: -0.024 min
Response: 41428
Conc: 0.24 ug/ml

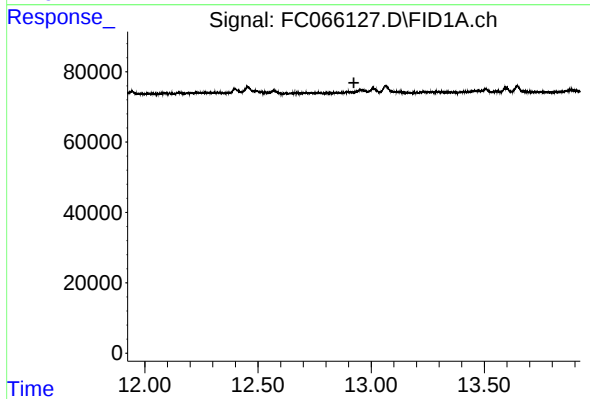

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.924 min
Response: 0
Conc: N.D.

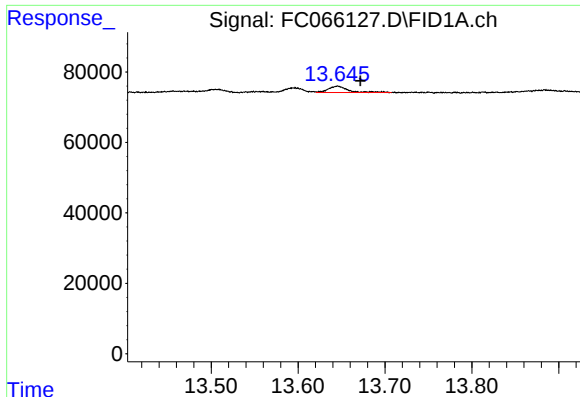

#13 n-Docosane (C22)


R.T.: 13.645 min
Delta R.T.: -0.026 min
Response: 27866
Conc: 0.16 ug/ml

Instrument :
FID_C
ClientSampleId :

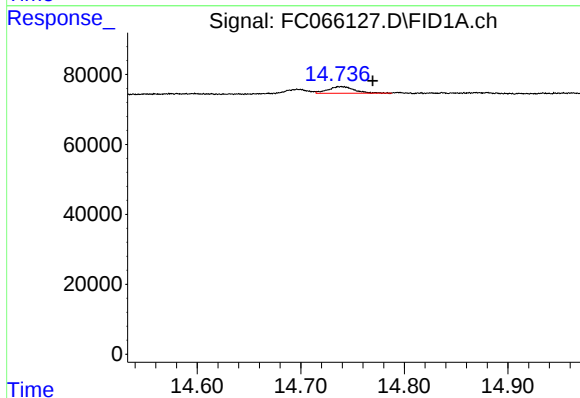


#14 n-Tetracosane (C24)

R.T.: 14.739 min
Delta R.T.: -0.030 min
Response: 32508
Conc: 0.19 ug/ml

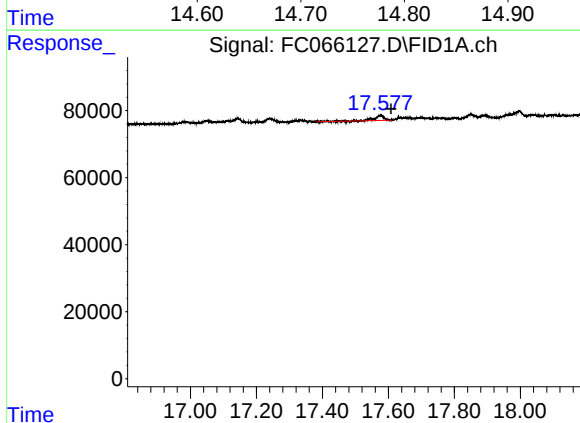


#17 n-Tricontane (C30)

R.T.: 17.576 min
Delta R.T.: -0.032 min
Response: 32321
Conc: 0.19 ug/ml

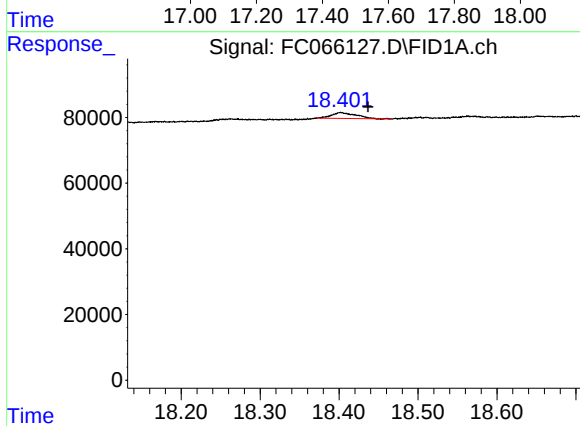

#18 n-Dotriacontane (C32)

R.T.: 18.402 min
Delta R.T.: -0.035 min
Response: 38122
Conc: 0.23 ug/ml

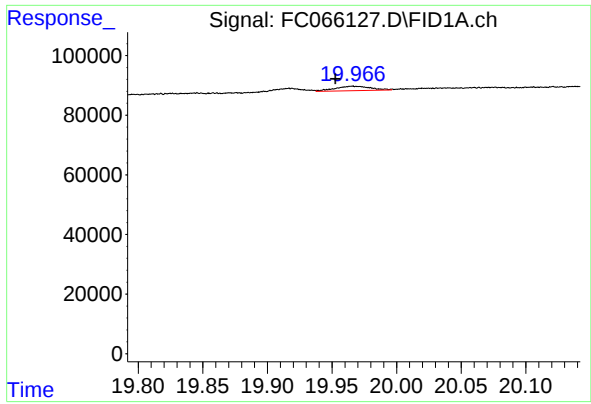

#20 n-Hexatriacontane (C36)

R.T.: 19.967 min
Delta R.T.: 0.014 min
Response: 28311
Conc: 0.18 ug/ml

Instrument :
FID_C
ClientSampleId :