

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032824AL\
Data File : FC066135.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2024 20:45
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:24:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 030424.M
Quant Title : GC Extractables
QLast Update : Mon Mar 04 13:09:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.587	56388	0.330 ug/ml
18) T	n-Dotriacontane (C32)	18.412	61034	0.362 ug/ml
20) T	n-Hexatriacontane (C36)	19.954	102153	0.642 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032824AL\
Data File : FC066135.D
Signal(s) : FID1A.ch
Acq On : 28 Mar 2024 20:45
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 29 02:24:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 030424.M
Quant Title : GC Extractables
QLast Update : Mon Mar 04 13:09:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

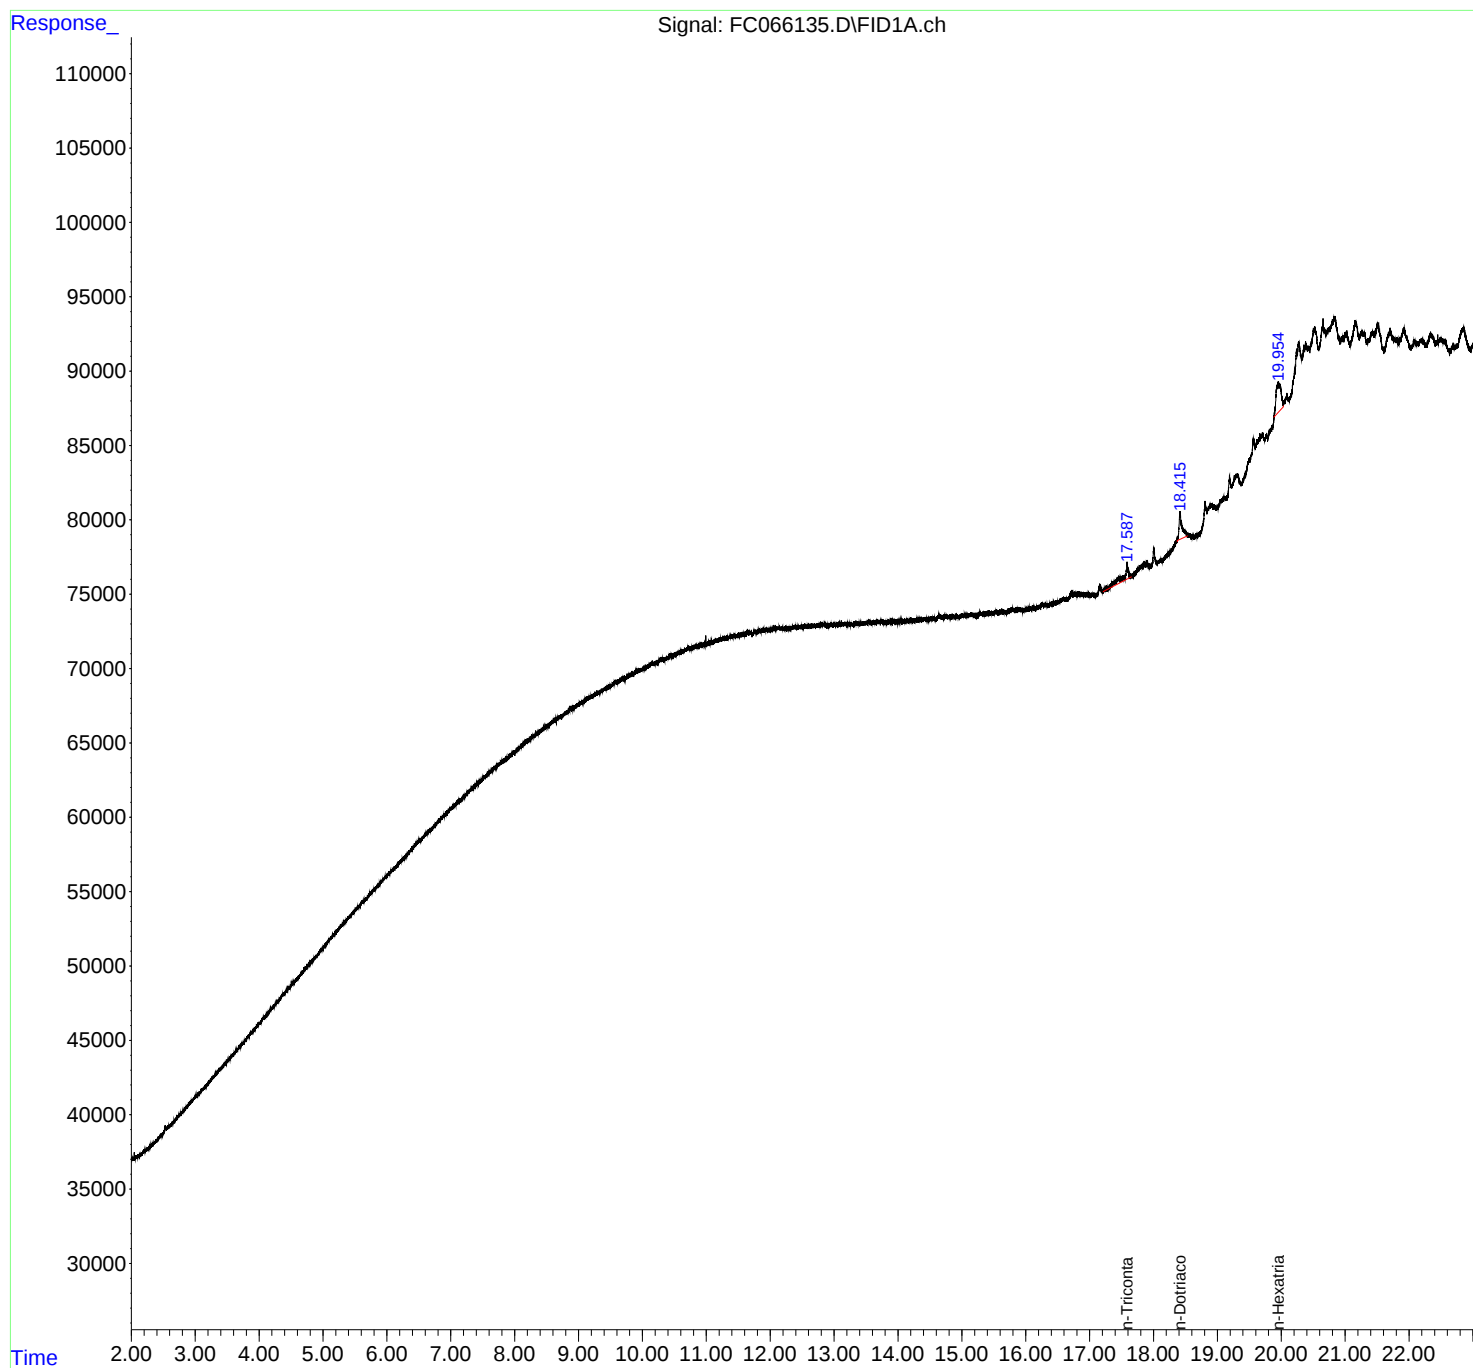


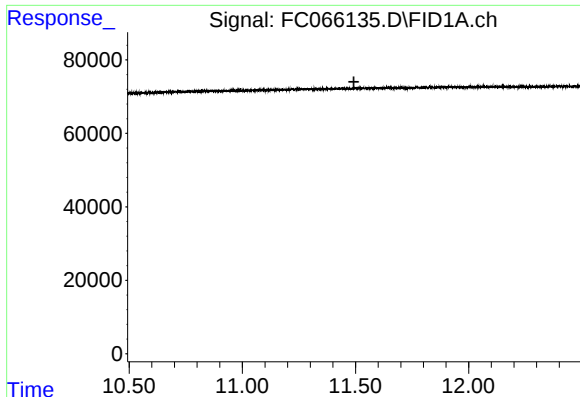

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.493 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

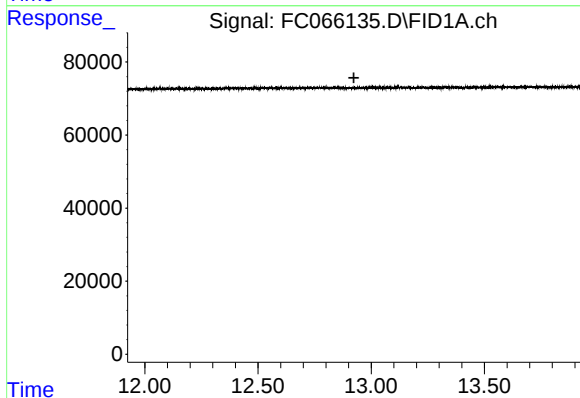


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.924 min
Response: 0
Conc: N.D.

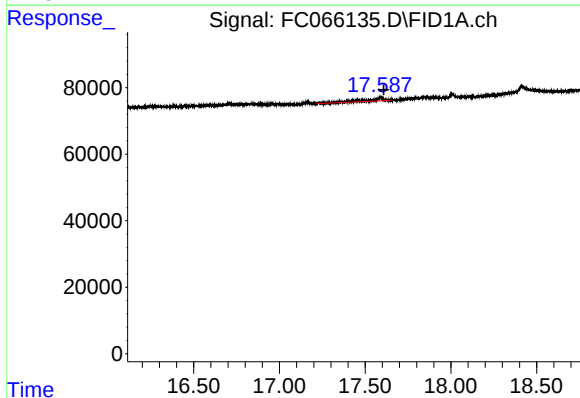


#17 n-Tricontane (C30)

R.T.: 17.587 min
Delta R.T.: -0.022 min
Response: 56388
Conc: 0.33 ug/ml

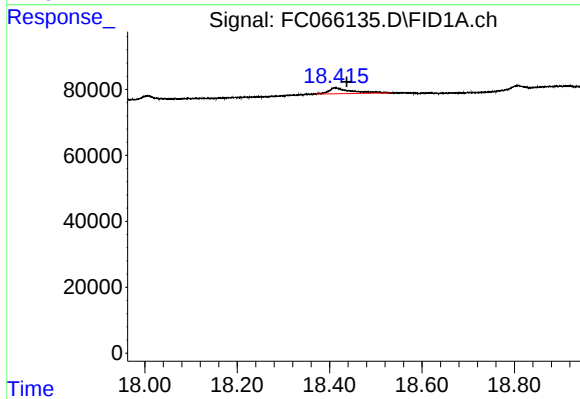

#18 n-Dotriacontane (C32)

R.T.: 18.412 min
Delta R.T.: -0.025 min
Response: 61034
Conc: 0.36 ug/ml

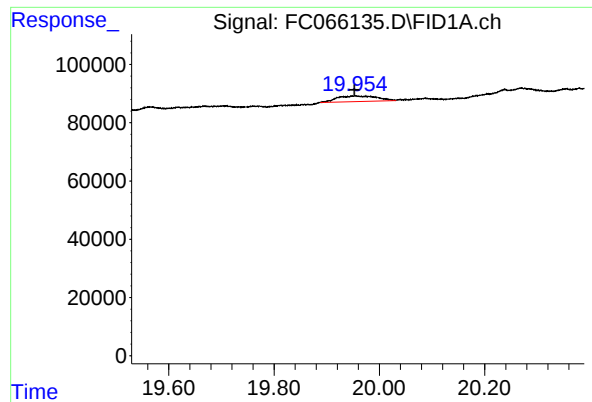

#20 n-Hexatriacontane (C36)

R.T.: 19.954 min
Delta R.T.: 0.002 min
Response: 102153
Conc: 0.64 ug/ml

Instrument :

FID_C

ClientSampleId :