

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032922AL\
 Data File : FC058952.D
 Signal(s) : FID1A.CH
 Acq On : 29 Mar 2022 21:31
 Operator : UA/NP
 Sample : N2155-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 30 03:23:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.544	5362815	47.842 ug/ml
Spiked Amount 50.000		Recovery =	95.68%
Target Compounds			
4) T n-Dodecane (C12)	5.997	169078	1.324 ug/ml
6) T n-Tetradecane (C14)	7.780	101710	0.782 ug/ml
15) T n-Hexacosane (C26)	15.408	88876	0.736 ug/ml
16) T n-Octacosane (C28)	16.354	168436	1.422 ug/ml
17) T n-Tricontane (C30)	17.237	97089	0.851 ug/ml
19) T n-Tetratriacontane (C34)	18.844	84908	0.840 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032922AL\
Data File : FC058952.D
Signal(s) : FID1A.CH
Acq On : 29 Mar 2022 21:31
Operator : UA/NP
Sample : N2155-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 30 03:23:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

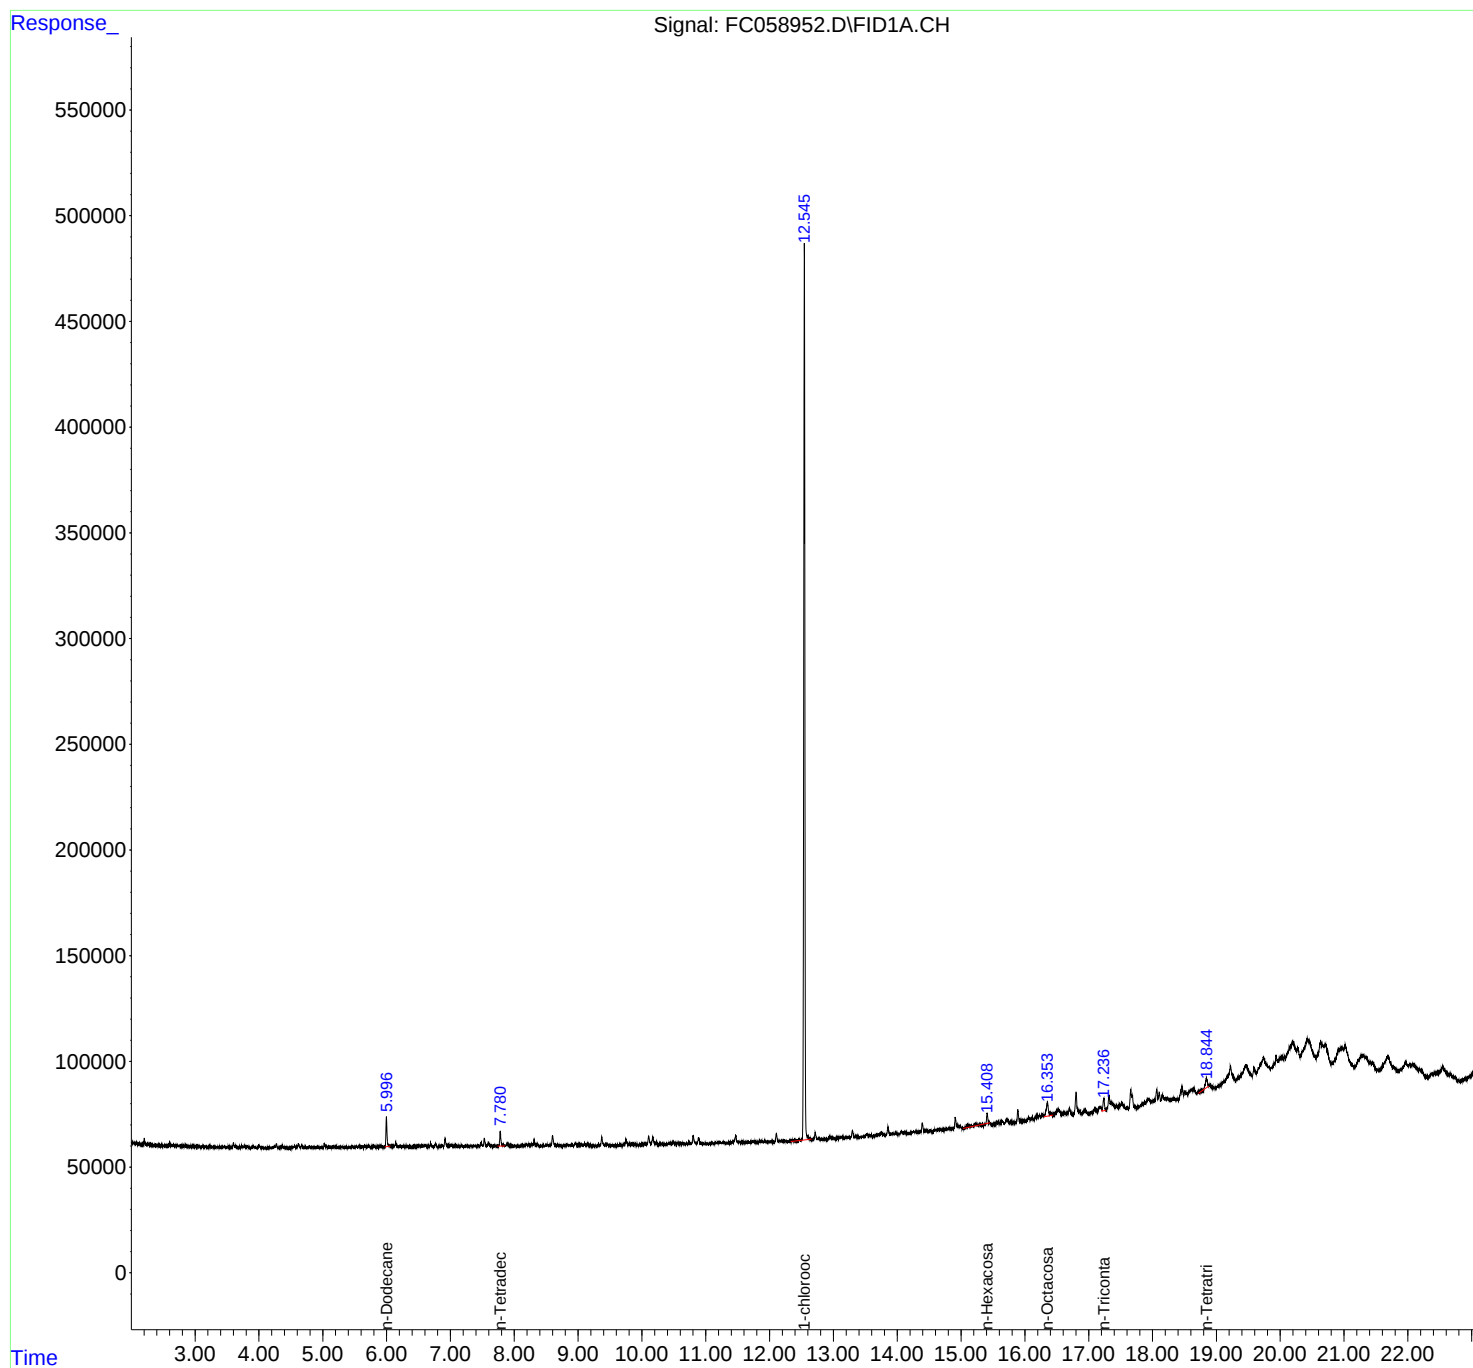


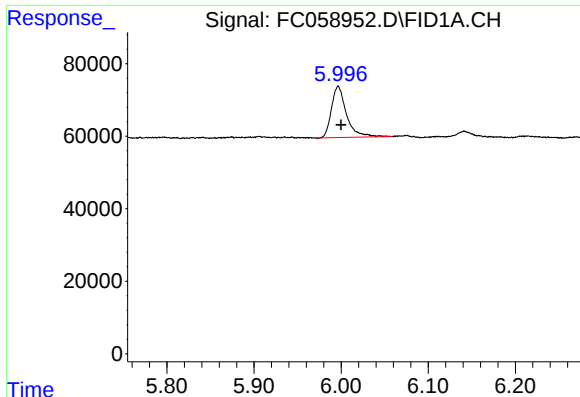

#4 n-Dodecane (C12)


R.T.: 5.997 min
Delta R.T.: -0.003 min
Response: 169078
Conc: 1.32 ug/ml

Instrument :
FID_C
ClientSampleId :

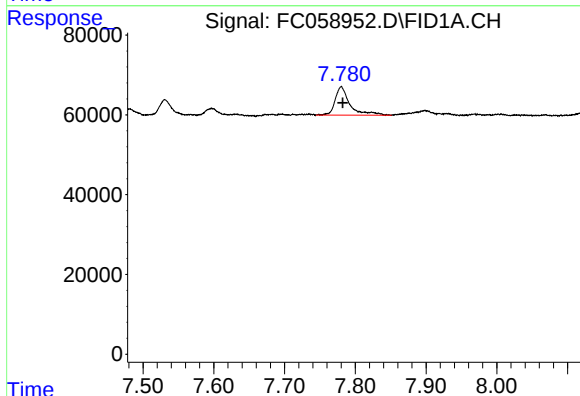


#6 n-Tetradecane (C14)

R.T.: 7.780 min
Delta R.T.: -0.002 min
Response: 101710
Conc: 0.78 ug/ml

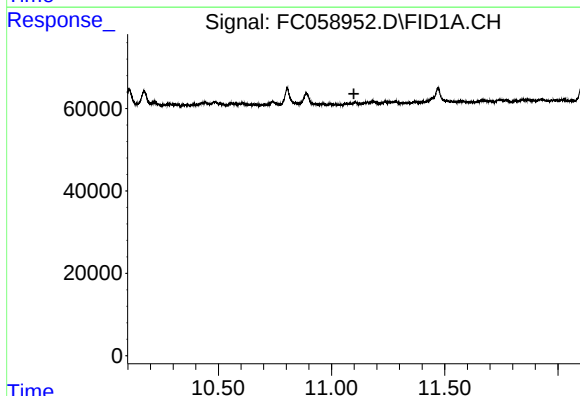


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.099 min
Response: 0
Conc: N.D.

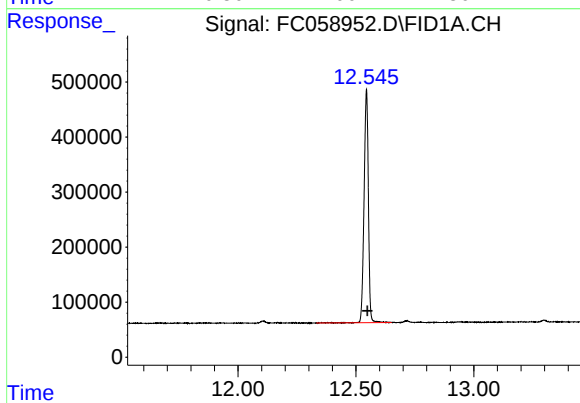

#12 1-chlorooctadecane (SURRE)


R.T.: 12.544 min
Delta R.T.: -0.004 min
Response: 5362815
Conc: 47.84 ug/ml

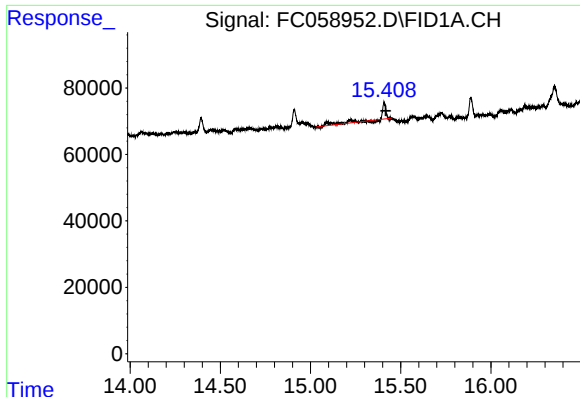

#15 n-Hexacosane (C26)


R.T.: 15.408 min
Delta R.T.: -0.009 min
Response: 88876
Conc: 0.74 ug/ml

Instrument :
FID_C
ClientSampleId :

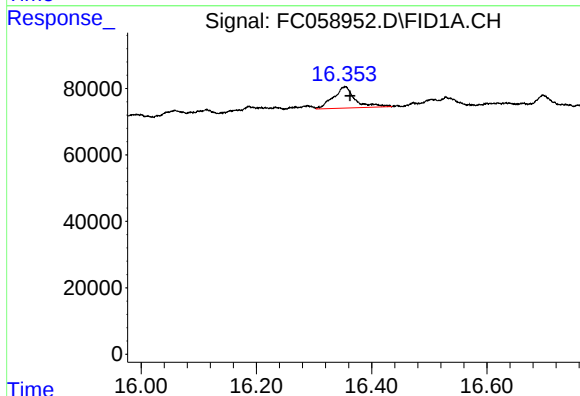


#16 n-Octacosane (C28)

R.T.: 16.354 min
Delta R.T.: -0.009 min
Response: 168436
Conc: 1.42 ug/ml

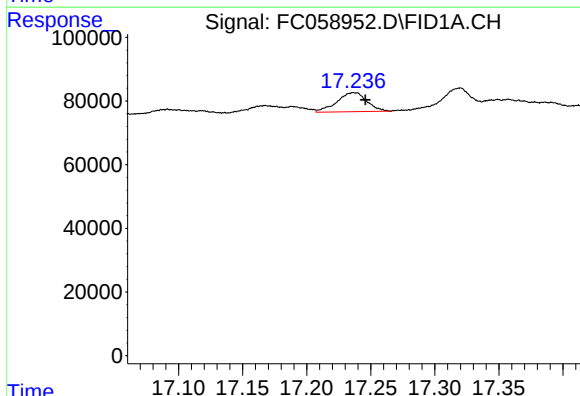

#17 n-Tricontane (C30)

R.T.: 17.237 min
Delta R.T.: -0.009 min
Response: 97089
Conc: 0.85 ug/ml

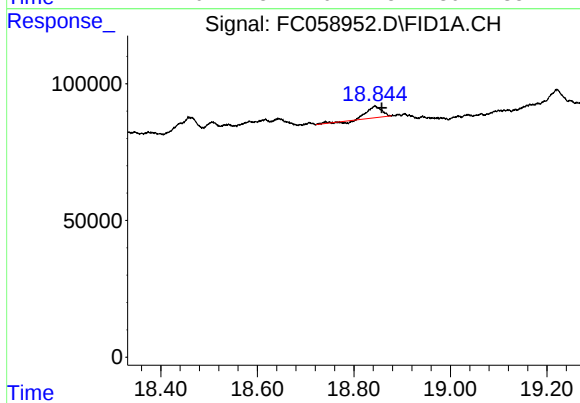

#19 n-Tetratriacontane (C34)

R.T.: 18.844 min
Delta R.T.: -0.014 min
Response: 84908
Conc: 0.84 ug/ml