

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032922AL\
 Data File : FC058966.D
 Signal(s) : FID1A.CH
 Acq On : 30 Mar 2022 6:16
 Operator : UA/NP
 Sample : N2149-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 PILE-LINDEN-SWITCH

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/30/2022
 Supervised By :mohammad ahmed 04/01/2022

Integration File: sample.E
 Quant Time: Mar 30 07:17:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.094	4033968	27.998 ug/ml
Spiked Amount 50.000		Recovery =	56.00%
12) S 1-chlorooctadecane (S...	12.540	3088672	27.554 ug/mlm
Spiked Amount 50.000		Recovery =	55.11%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC032922AL\
Data File : FC058966.D
Signal(s) : FID1A.CH
Acq On : 30 Mar 2022 6:16
Operator : UA/NP
Sample : N2149-01
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
PILE-LINDEN-SWITCH


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/30/2022
Supervised By :mohammad ahmed 04/01/2022

Integration File: sample.E
Quant Time: Mar 30 07:17:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

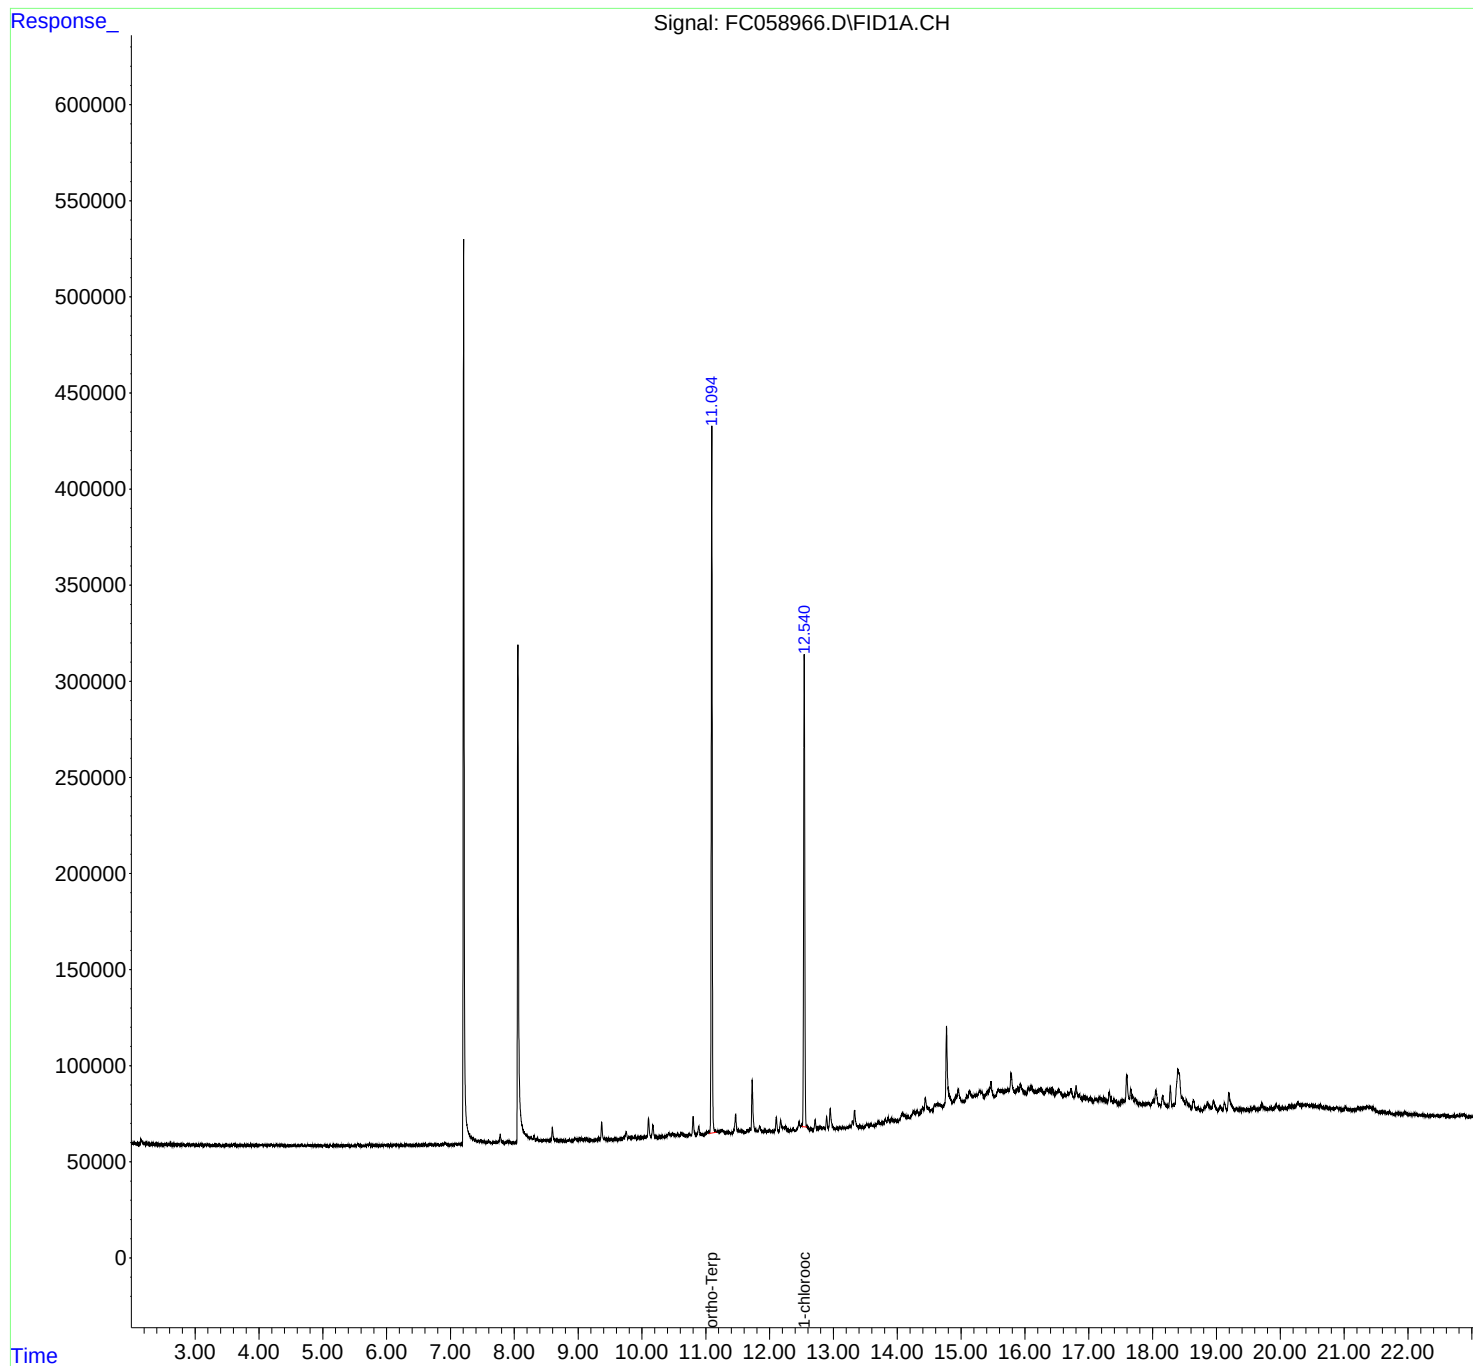

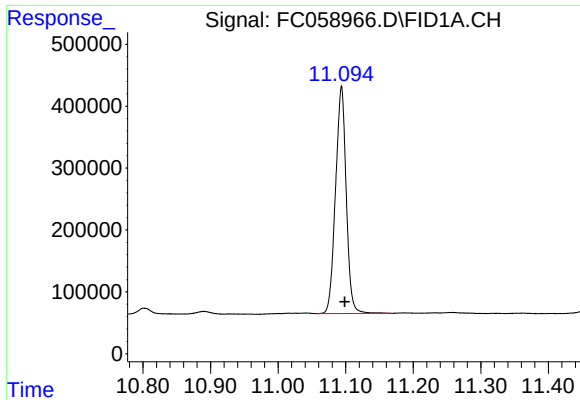


#9 ortho-Terphenyl (SURR)

R.T.: 11.094 min
Delta R.T.: -0.005 min
Response: 4033968
Conc: 28.00 ug/ml

Instrument :
FID_C
ClientSampleId :
PILE-LINDEN-SWITCH

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/30/2022
Supervised By :mohammad ahmed 04/01/2022

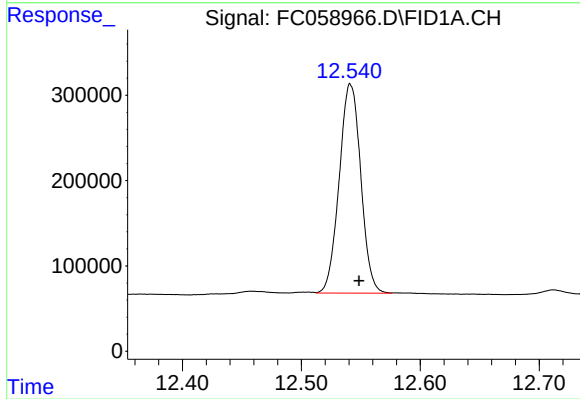

#12 1-chlorooctadecane (SURR)

R.T.: 12.540 min
Delta R.T.: -0.008 min
Response: 3088672
Conc: 27.55 ug/ml m